

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048019.D
 Acq On : 13 Apr 2022 21:35
 Operator : SY/MD
 Sample : N2386-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ8

Quant Time: Apr 14 07:17:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 14 06:53:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	356628	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	372503	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	194830	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	108796	42.069	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.140%
7) Chloroethane-d5	1.916	69	94223	46.206	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.420%
11) 1,1-Dichloroethene-d2	2.568	63	143342	30.295	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.580%
21) 2-Butanone-d5	4.620	46	196691	88.610	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.610%
24) Chloroform-d	5.067	84	209197	44.209	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.420%
26) 1,2-Dichloroethane-d4	5.703	65	136671	47.092	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.180%
32) Benzene-d6	5.729	84	428072	45.670	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.340%
36) 1,2-Dichloropropane-d6	6.690	67	142131	49.375	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.760%
41) Toluene-d8	7.899	98	381648	41.791	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.580%
43) trans-1,3-Dichloroprop...	8.179	79	58399	40.044	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.080%
47) 2-Hexanone-d5	8.632	63	144721	85.881	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.880%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	212667	43.048	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.100%
66) 1,2-Dichlorobenzene-d4	12.195	152	165049	47.617	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.240%
Target Compounds						
13) Acetone	2.629	43	6072	2.939	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048019.D
Acq On : 13 Apr 2022 21:35
Operator : SY/MD
Sample : N2386-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ8


Quant Time: Apr 14 07:17:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 14 06:53:20 2022
Response via : Initial Calibration

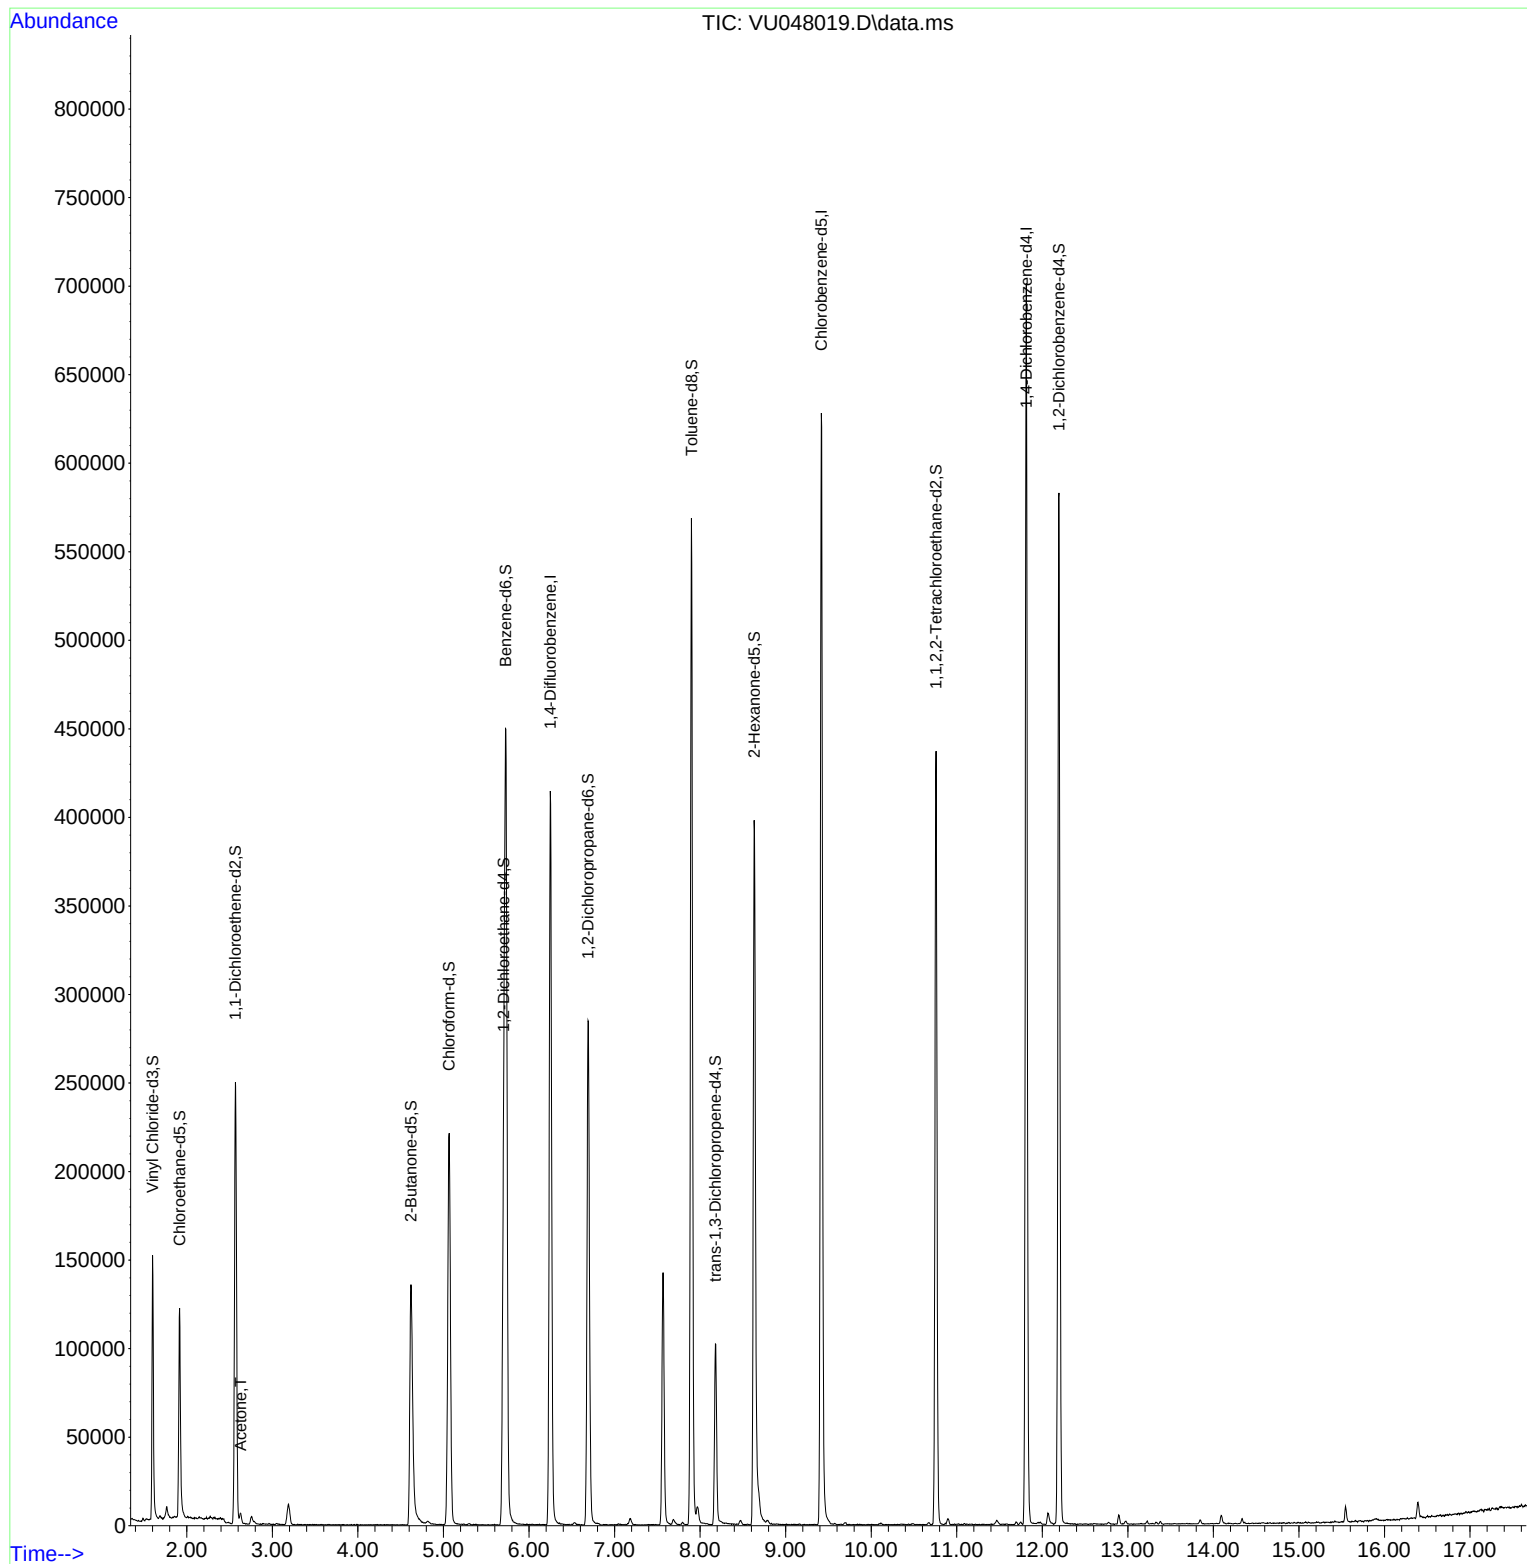


Abundance Scan 399 (2.623 min): VU048017.D\data.ms (-38

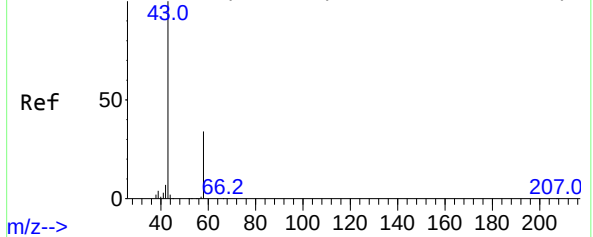

Abundance Scan 401 (2.629 min): VU048019.D\data.ms

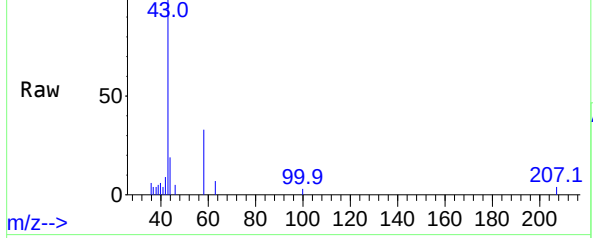

Abundance Scan 401 (2.629 min): VU048019.D\data.ms (-30

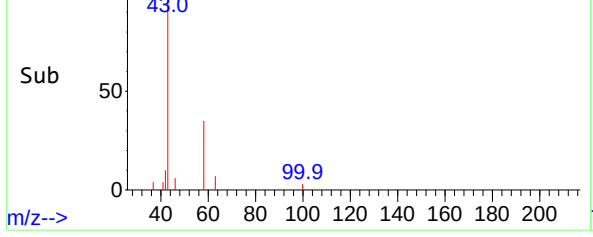

#13

Acetone

Concen: 2.939 ug/L

RT: 2.629 min Scan# 401

Delta R.T. 0.006 min

Lab File: VU048019.D

Acq: 13 Apr 2022 21:35

Instrument :

MSVOA_U

ClientSampleId :

C0HZ8

Tgt Ion: 43 Resp: 6072

Ion Ratio Lower Upper

43 100

58 32.1 0.0 70.0

Abundance

