

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048029.D
 Acq On : 14 Apr 2022 01:27
 Operator : SY/MD
 Sample : N2386-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J33

Quant Time: Apr 14 07:19:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 14 06:53:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	336134	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	357485	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	186210	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	102870	42.203	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.400%
7) Chloroethane-d5	1.916	69	92386	48.068	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.140%
11) 1,1-Dichloroethene-d2	2.568	63	138603	31.079	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.160%
21) 2-Butanone-d5	4.620	46	189580	90.614	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.610%
24) Chloroform-d	5.067	84	205284	46.028	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.060%
26) 1,2-Dichloroethane-d4	5.703	65	132829	48.559	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.120%
32) Benzene-d6	5.729	84	411408	45.736	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.480%
36) 1,2-Dichloropropane-d6	6.694	67	135752	49.140	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.280%
41) Toluene-d8	7.899	98	367599	41.944	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.880%
43) trans-1,3-Dichloroprop...	8.179	79	53272	38.063	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.120%
47) 2-Hexanone-d5	8.632	63	136324	84.297	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.300%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	209126	44.110	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.220%
66) 1,2-Dichlorobenzene-d4	12.195	152	160345	48.401	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds						
13) Acetone	2.629	43	5553	2.852	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048029.D
Acq On : 14 Apr 2022 01:27
Operator : SY/MD
Sample : N2386-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J33

Quant Time: Apr 14 07:19:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 14 06:53:20 2022
Response via : Initial Calibration

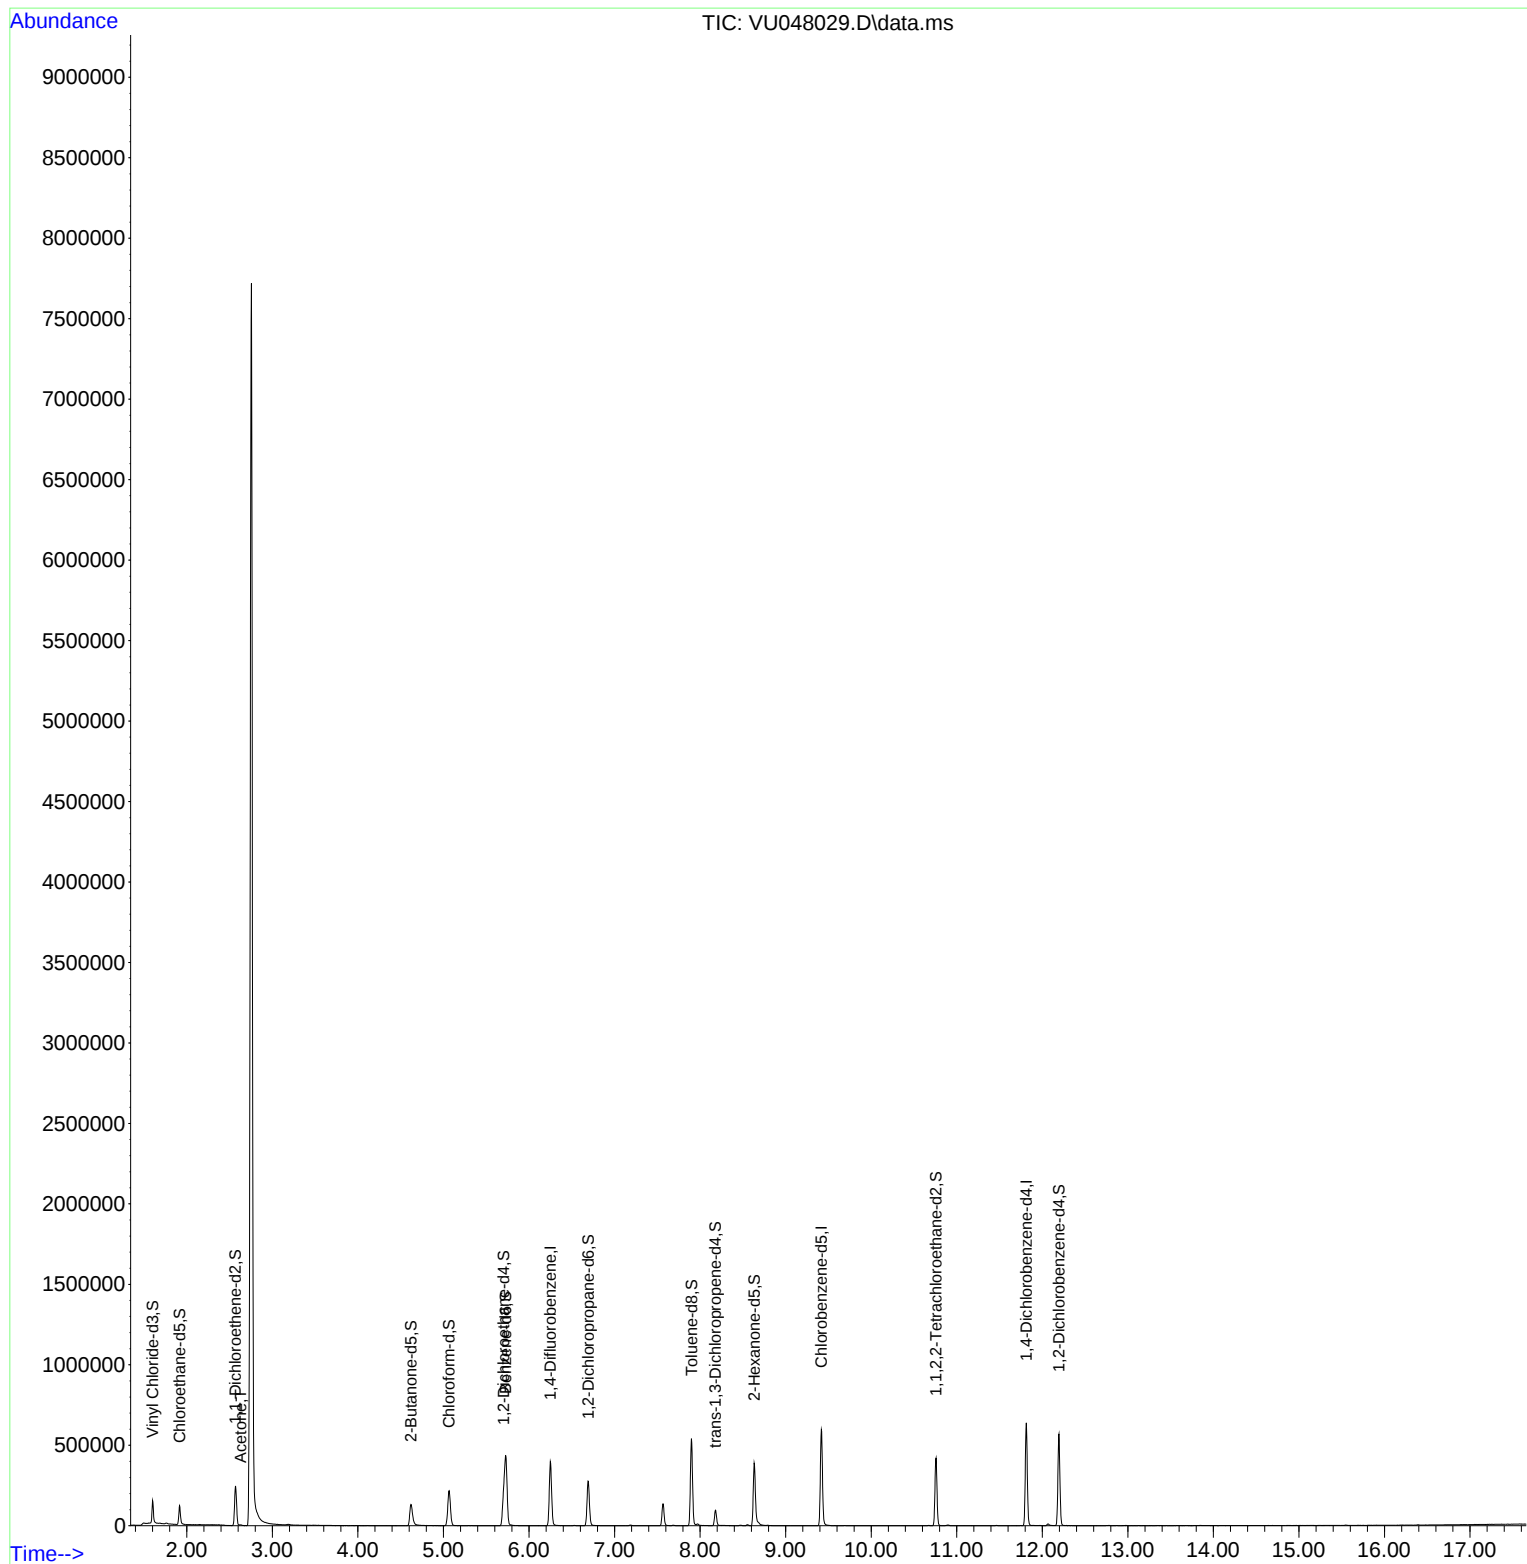

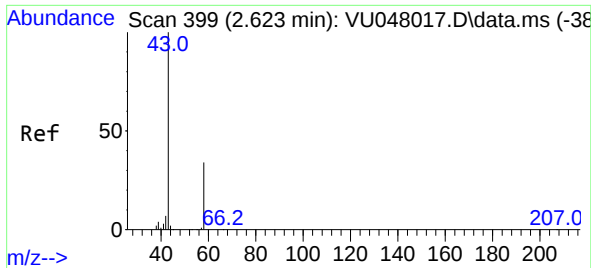

#13

Acetone

Concen: 2.852 ug/L

RT: 2.629 min Scan# 401

Delta R.T. 0.006 min

Lab File: VU048029.D


Acq: 14 Apr 2022 01:27

Instrument :

MSVOA_U

ClientSampleId :

C0J33

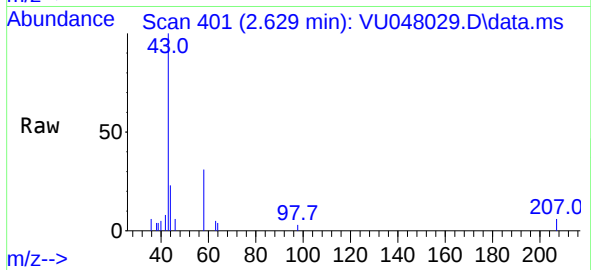

Tgt Ion: 43 Resp: 5553

Ion Ratio Lower Upper

43 100

58 31.0 0.0 70.0

