

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048005.D
 Acq On : 13 Apr 2022 15:48
 Operator : SY/MD
 Sample : N2293-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	102	rBV	154350	181010	14.20%	1.732%
2	1.916	170	179	198	rBV	125473	175734	13.78%	1.682%
3	2.485	354	356	360	rVB2	414	280	0.02%	0.003%
4	2.568	370	382	398	rBV	262147	430824	33.79%	4.123%
5	2.752	435	439	440	rBV	469	333	0.03%	0.003%
6	2.800	451	454	458	rVB3	553	398	0.03%	0.004%
7	2.823	458	461	463	rBV2	318	238	0.02%	0.002%
8	2.848	467	469	473	rBV2	317	221	0.02%	0.002%
9	2.948	496	500	501	rBV	417	280	0.02%	0.003%
10	3.054	522	533	544	rBV4	3755	6960	0.55%	0.067%
11	3.157	561	565	566	rBV4	381	261	0.02%	0.002%
12	3.224	583	586	589	rBV2	262	199	0.02%	0.002%
13	3.289	601	606	608	rBV2	229	207	0.02%	0.002%
14	3.353	623	626	628	rVV2	280	201	0.02%	0.002%
15	3.437	649	652	655	rVB	496	289	0.02%	0.003%
16	3.491	661	669	670	rBV3	373	429	0.03%	0.004%
17	3.668	721	724	727	rVB2	412	300	0.02%	0.003%
18	3.697	727	733	738	rBV2	360	397	0.03%	0.004%
19	4.015	827	832	835	rBV2	348	345	0.03%	0.003%
20	4.221	894	896	902	rVB2	299	194	0.02%	0.002%
21	4.260	902	908	911	rBV2	177	239	0.02%	0.002%
22	4.276	911	913	917	rVB	504	265	0.02%	0.003%
23	4.305	917	922	923	rBV	363	324	0.03%	0.003%
24	4.356	932	938	941	rBV2	461	529	0.04%	0.005%
25	4.375	941	944	949	rVV3	436	441	0.03%	0.004%
26	4.620	1007	1020	1049	rBV	136605	330255	25.90%	3.161%
27	5.067	1142	1159	1181	rBV	228820	502016	39.37%	4.805%
28	5.234	1209	1211	1215	rVB3	324	208	0.02%	0.002%
29	5.340	1240	1244	1248	rBV2	275	256	0.02%	0.002%
30	5.433	1266	1273	1274	rBV	334	361	0.03%	0.003%
31	5.729	1343	1365	1393	rBV2	462659	1275074	100.00%	12.203%
32	6.025	1453	1457	1459	rBV2	358	277	0.02%	0.003%
33	6.041	1459	1462	1465	rBV2	536	395	0.03%	0.004%
34	6.125	1486	1488	1495	rVB2	686	578	0.05%	0.006%
35	6.250	1511	1527	1559	rBV	413121	774041	60.71%	7.408%
36	6.527	1607	1613	1617	rBV3	1669	2053	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048005.D
 Acq On : 13 Apr 2022 15:48
 Operator : SY/MD
 Sample : N2293-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1650	1665	1688	rBV	291476	579005	45.41%	5.541%
38	6.813	1699	1702	1707	rVB4	627	489	0.04%	0.005%
39	6.906	1728	1731	1735	rVB	328	288	0.02%	0.003%
40	7.047	1769	1775	1777	rBV2	547	489	0.04%	0.005%
41	7.105	1790	1793	1796	rVB	422	216	0.02%	0.002%
42	7.186	1807	1818	1831	rBV3	3468	6866	0.54%	0.066%
43	7.253	1836	1839	1847	rVB3	279	196	0.02%	0.002%
44	7.401	1883	1885	1890	rVB	229	198	0.02%	0.002%
45	7.440	1893	1897	1900	rBV2	284	262	0.02%	0.003%
46	7.507	1916	1918	1923	rVB	345	252	0.02%	0.002%
47	7.568	1923	1937	1955	rBV	152428	268609	21.07%	2.571%
48	7.687	1967	1974	1991	rVB7	2908	5800	0.45%	0.056%
49	7.899	2026	2040	2056	rBV	582715	1001712	78.56%	9.587%
50	8.179	2115	2127	2143	rBV	105833	182372	14.30%	1.745%
51	8.633	2255	2268	2297	rBV	405240	755861	59.28%	7.234%
52	9.073	2399	2405	2407	rBV2	378	276	0.02%	0.003%
53	9.153	2424	2430	2432	rBV3	499	461	0.04%	0.004%
54	9.417	2498	2512	2547	rBV	614225	1047292	82.14%	10.023%
55	9.562	2554	2557	2560	rBV2	528	456	0.04%	0.004%
56	9.600	2566	2569	2575	rVB2	358	315	0.02%	0.003%
57	9.642	2576	2582	2586	rBV3	479	515	0.04%	0.005%
58	9.690	2592	2597	2606	rBV4	1091	1534	0.12%	0.015%
59	9.854	2645	2648	2653	rVB2	258	188	0.01%	0.002%
60	9.951	2675	2678	2685	rVB3	400	479	0.04%	0.005%
61	10.102	2720	2725	2729	rBV3	576	690	0.05%	0.007%
62	10.205	2753	2757	2760	rVB2	301	196	0.02%	0.002%
63	10.305	2784	2788	2792	rBV	252	188	0.01%	0.002%
64	10.497	2844	2848	2849	rBV2	338	214	0.02%	0.002%
65	10.533	2855	2859	2862	rBV	240	192	0.02%	0.002%
66	10.674	2895	2903	2910	rBV4	1643	2439	0.19%	0.023%
67	10.758	2916	2929	2951	rVB	450653	721507	56.59%	6.905%
68	10.848	2954	2957	2959	rBV2	337	205	0.02%	0.002%
69	10.867	2959	2963	2965	rBV2	420	366	0.03%	0.004%
70	10.886	2967	2969	2973	rBV3	420	346	0.03%	0.003%
71	10.938	2980	2985	2986	rBV2	304	236	0.02%	0.002%
72	11.086	3026	3031	3036	rBV3	376	421	0.03%	0.004%
73	11.124	3041	3043	3050	rVB4	478	412	0.03%	0.004%
74	11.160	3051	3054	3056	rVB3	410	222	0.02%	0.002%
75	11.298	3095	3097	3102	rVB3	302	210	0.02%	0.002%
76	11.462	3141	3148	3151	rBV2	1579	1819	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048005.D
 Acq On : 13 Apr 2022 15:48
 Operator : SY/MD
 Sample : N2293-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.578	3181	3184	3187	rBV2	342	283	0.02%	0.003%
78	11.681	3213	3216	3218	rBV2	363	245	0.02%	0.002%
79	11.697	3218	3221	3227	rVB4	872	897	0.07%	0.009%
80	11.751	3234	3238	3242	rVB4	607	564	0.04%	0.005%
81	11.812	3244	3257	3280	rBV	672445	1090825	85.55%	10.440%
82	12.012	3317	3319	3322	rBV2	350	199	0.02%	0.002%
83	12.031	3322	3325	3328	rVB	311	195	0.02%	0.002%
84	12.195	3361	3376	3395	rVV	602035	1000101	78.43%	9.572%
85	12.314	3411	3413	3416	rVB3	649	318	0.02%	0.003%
86	12.330	3416	3418	3420	rBV	753	352	0.03%	0.003%
87	12.404	3438	3441	3447	rVB4	485	551	0.04%	0.005%
88	12.520	3471	3477	3480	rBV3	538	525	0.04%	0.005%
89	12.587	3495	3498	3502	rBV3	354	301	0.02%	0.003%
90	12.636	3510	3513	3516	rBV	437	282	0.02%	0.003%
91	12.970	3608	3617	3618	rBV4	3596	3007	0.24%	0.029%
92	13.333	3722	3730	3738	rVB3	2743	3732	0.29%	0.036%
93	13.382	3738	3745	3752	rBV5	2471	3459	0.27%	0.033%
94	13.838	3885	3887	3888	rBV	543	217	0.02%	0.002%
95	14.362	4048	4050	4057	rVB4	1308	1375	0.11%	0.013%
96	14.716	4158	4160	4166	rVB2	574	351	0.03%	0.003%
97	14.941	4227	4230	4232	rBV2	544	367	0.03%	0.004%
98	15.099	4276	4279	4282	rBV	807	602	0.05%	0.006%
99	15.545	4409	4418	4431	rBV5	22180	34068	2.67%	0.326%
100	16.388	4673	4680	4691	rVB2	23246	35546	2.79%	0.340%




Sum of corrected areas: 10448568

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048005.D
Acq On : 13 Apr 2022 15:48
Operator : SY/MD
Sample : N2293-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

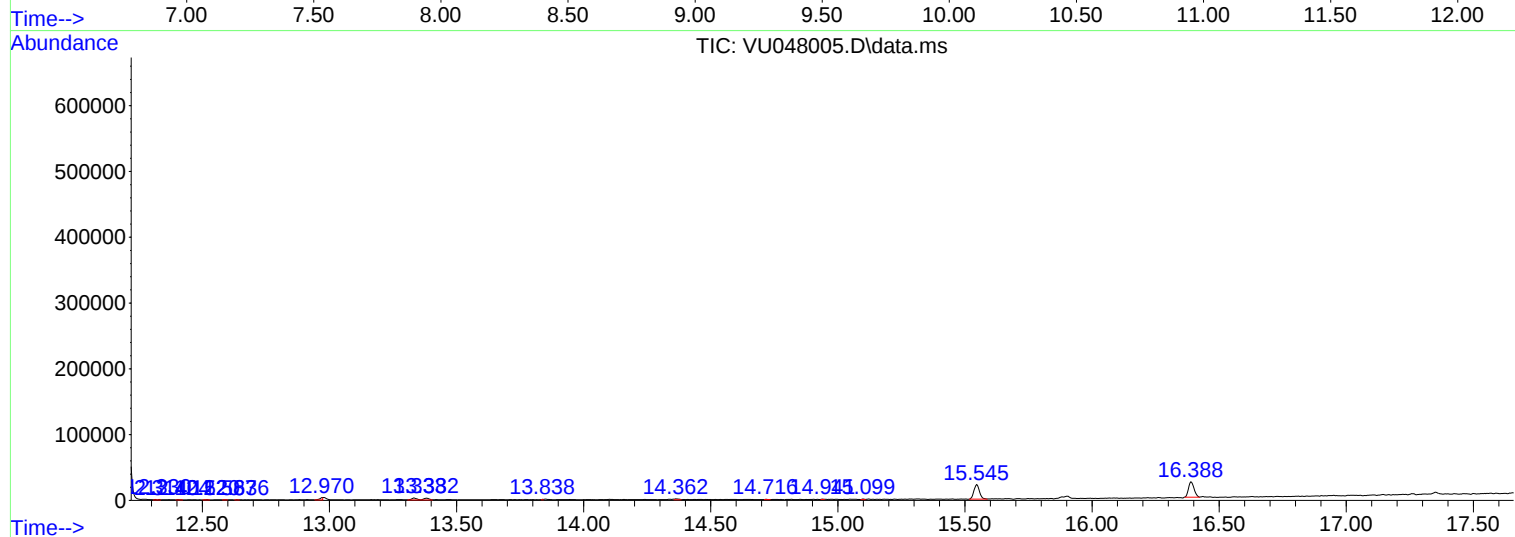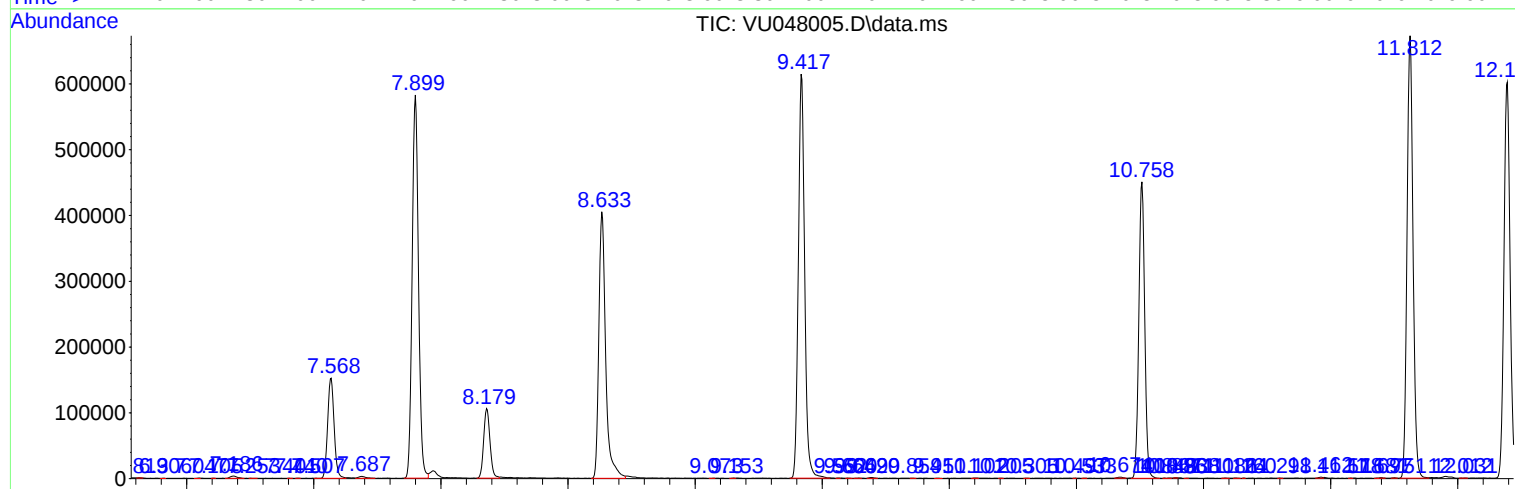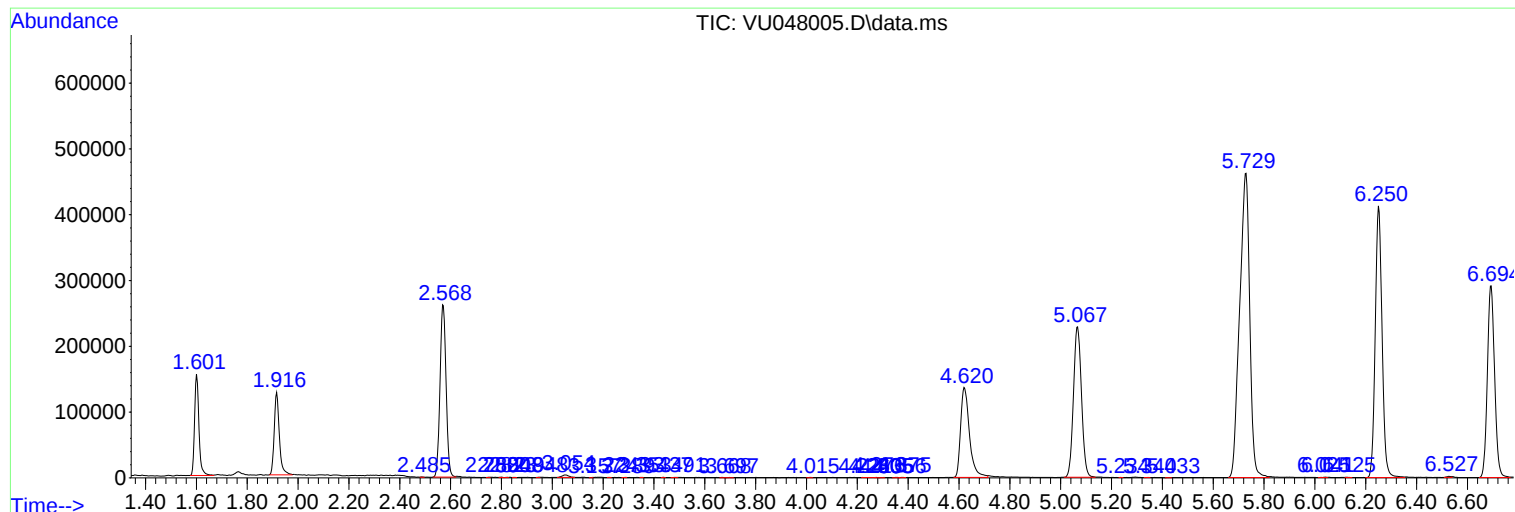

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048005.D
Acq On : 13 Apr 2022 15:48
Operator : SY/MD
Sample : N2293-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048005.D
Acq On : 13 Apr 2022 15:48
Operator : SY/MD
Sample : N2293-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------