

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048018.D
 Acq On : 13 Apr 2022 21:12
 Operator : SY/MD
 Sample : VU0413WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	100	rBV	167926	194511	14.63%	1.820%
2	1.916	170	179	202	rVB	128069	182982	13.76%	1.712%
3	2.498	358	360	369	rVB3	719	507	0.04%	0.005%
4	2.568	370	382	401	rBV	281809	459475	34.55%	4.300%
5	2.771	442	445	446	rBV2	319	194	0.01%	0.002%
6	2.800	446	454	462	rVB	1038	1758	0.13%	0.016%
7	2.912	485	489	492	rBV	650	569	0.04%	0.005%
8	3.044	524	530	531	rBV4	1314	1301	0.10%	0.012%
9	3.186	571	574	576	rBV2	405	272	0.02%	0.003%
10	3.234	584	589	592	rBV3	399	339	0.03%	0.003%
11	3.282	600	604	608	rBV3	272	275	0.02%	0.003%
12	3.363	624	629	637	rVB2	537	659	0.05%	0.006%
13	3.398	637	640	643	rBV	284	187	0.01%	0.002%
14	3.488	661	668	671	rBV2	271	289	0.02%	0.003%
15	3.636	708	714	715	rBV2	333	275	0.02%	0.003%
16	3.649	715	718	720	rVV	331	228	0.02%	0.002%
17	3.858	775	783	787	rBV3	286	355	0.03%	0.003%
18	3.980	818	821	824	rVB	490	343	0.03%	0.003%
19	4.060	842	846	849	rBV3	260	190	0.01%	0.002%
20	4.279	911	914	922	rVB2	444	589	0.04%	0.006%
21	4.491	974	980	982	rBV	234	220	0.02%	0.002%
22	4.620	1007	1020	1060	rVV	137324	336169	25.28%	3.146%
23	5.067	1141	1159	1184	rBV2	237770	517067	38.88%	4.838%
24	5.224	1205	1208	1216	rVB4	492	437	0.03%	0.004%
25	5.282	1222	1226	1228	rBV2	488	454	0.03%	0.004%
26	5.334	1240	1242	1245	rVB2	315	217	0.02%	0.002%
27	5.382	1253	1257	1261	rBV2	263	247	0.02%	0.002%
28	5.485	1287	1289	1292	rVB2	297	191	0.01%	0.002%
29	5.504	1292	1295	1298	rBV2	310	251	0.02%	0.002%
30	5.726	1342	1364	1392	rBV2	489370	1329866	100.00%	12.444%
31	6.047	1458	1464	1467	rBV4	345	449	0.03%	0.004%
32	6.128	1484	1489	1494	rVB3	393	436	0.03%	0.004%
33	6.153	1494	1497	1499	rBV2	250	190	0.01%	0.002%
34	6.192	1505	1509	1513	rVB2	257	247	0.02%	0.002%
35	6.250	1513	1527	1560	rBV	404518	774443	58.23%	7.247%
36	6.526	1607	1613	1624	rVB5	1829	3584	0.27%	0.034%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048018.D
 Acq On : 13 Apr 2022 21:12
 Operator : SY/MD
 Sample : VU0413WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1687	rBV	303690	596379	44.85%	5.581%
38	6.983	1751	1755	1757	rBV2	411	251	0.02%	0.002%
39	7.018	1762	1766	1768	rBV	302	239	0.02%	0.002%
40	7.186	1808	1818	1834	rVB3	4139	7673	0.58%	0.072%
41	7.436	1893	1896	1899	rBV2	309	247	0.02%	0.002%
42	7.568	1924	1937	1963	rBV2	151809	272392	20.48%	2.549%
43	7.687	1966	1974	1976	rBV3	2083	2466	0.19%	0.023%
44	7.793	2002	2007	2018	rVB4	1609	2126	0.16%	0.020%
45	7.899	2024	2040	2056	rBV	610295	1059169	79.64%	9.911%
46	8.128	2108	2111	2113	rBV	332	202	0.02%	0.002%
47	8.179	2115	2127	2147	rBV	108491	185468	13.95%	1.736%
48	8.340	2174	2177	2181	rBV2	407	348	0.03%	0.003%
49	8.359	2181	2183	2186	rVV	713	461	0.03%	0.004%
50	8.375	2186	2188	2192	rVV	423	212	0.02%	0.002%
51	8.440	2206	2208	2211	rVB3	355	204	0.02%	0.002%
52	8.494	2222	2225	2228	rVB4	287	196	0.01%	0.002%
53	8.536	2236	2238	2240	rBV	446	234	0.02%	0.002%
54	8.552	2240	2243	2245	rVV2	390	266	0.02%	0.002%
55	8.632	2256	2268	2297	rBV	416152	775661	58.33%	7.258%
56	8.848	2332	2335	2338	rVB4	340	206	0.02%	0.002%
57	8.976	2373	2375	2379	rBV4	341	303	0.02%	0.003%
58	9.025	2388	2390	2394	rVB	314	212	0.02%	0.002%
59	9.140	2423	2426	2428	rVV3	294	217	0.02%	0.002%
60	9.157	2429	2431	2434	rVV2	441	261	0.02%	0.002%
61	9.182	2437	2439	2442	rVB2	369	212	0.02%	0.002%
62	9.250	2457	2460	2461	rBV2	385	240	0.02%	0.002%
63	9.417	2499	2512	2538	rBV	609066	1026691	77.20%	9.607%
64	9.571	2553	2560	2562	rBV2	771	849	0.06%	0.008%
65	9.655	2583	2586	2590	rVB	481	327	0.02%	0.003%
66	9.700	2590	2600	2609	rBV5	1498	2585	0.19%	0.024%
67	9.761	2617	2619	2623	rVB2	283	193	0.01%	0.002%
68	9.841	2642	2644	2650	rBV	370	238	0.02%	0.002%
69	9.944	2670	2676	2677	rBV	262	189	0.01%	0.002%
70	10.112	2718	2728	2729	rBV4	1355	1884	0.14%	0.018%
71	10.362	2800	2806	2809	rBV3	319	358	0.03%	0.003%
72	10.411	2819	2821	2826	rVB3	346	218	0.02%	0.002%
73	10.484	2837	2844	2851	rBV4	1345	1807	0.14%	0.017%
74	10.526	2853	2857	2860	rVV3	459	409	0.03%	0.004%
75	10.674	2895	2903	2909	rBV4	2002	2870	0.22%	0.027%
76	10.758	2916	2929	2945	rBV	459128	731947	55.04%	6.849%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048018.D
 Acq On : 13 Apr 2022 21:12
 Operator : SY/MD
 Sample : VU0413WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.870	2959	2964	2966	rBV	412	343	0.03%	0.003%
78	10.893	2966	2971	2982	rVB5	715	1203	0.09%	0.011%
79	10.960	2988	2992	2995	rBV	286	258	0.02%	0.002%
80	11.031	3012	3014	3018	rVB2	340	235	0.02%	0.002%
81	11.086	3026	3031	3032	rBV3	787	553	0.04%	0.005%
82	11.468	3138	3150	3161	rVV5	2650	4922	0.37%	0.046%
83	11.751	3230	3238	3244	rBV5	1929	2961	0.22%	0.028%
84	11.812	3244	3257	3281	rBV	667520	1080849	81.28%	10.114%
85	11.947	3293	3299	3301	rBV4	628	762	0.06%	0.007%
86	12.086	3338	3342	3350	rBV3	376	490	0.04%	0.005%
87	12.195	3362	3376	3396	rBV	625358	1027827	77.29%	9.618%
88	12.414	3442	3444	3447	rBV	384	190	0.01%	0.002%
89	12.642	3511	3515	3517	rBV2	475	342	0.03%	0.003%
90	12.873	3581	3587	3592	rBV3	314	503	0.04%	0.005%
91	12.976	3612	3619	3621	rBV3	1284	1607	0.12%	0.015%
92	13.144	3666	3671	3675	rBV3	577	613	0.05%	0.006%
93	13.224	3688	3696	3708	rBV6	3233	4699	0.35%	0.044%
94	13.333	3726	3730	3737	rVB3	998	1310	0.10%	0.012%
95	13.378	3738	3744	3751	rVB6	1501	1859	0.14%	0.017%
96	13.844	3879	3889	3896	rBV4	5067	7872	0.59%	0.074%
97	14.092	3957	3966	3980	rVB	12518	20826	1.57%	0.195%
98	14.333	4032	4041	4048	rBV3	5846	8835	0.66%	0.083%
99	15.545	4410	4418	4428	rBV5	9755	14946	1.12%	0.140%
100	16.391	4673	4681	4690	rBV5	11426	16502	1.24%	0.154%


Sum of corrected areas: 10686683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048018.D
Acq On : 13 Apr 2022 21:12
Operator : SY/MD
Sample : VU0413WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK090

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

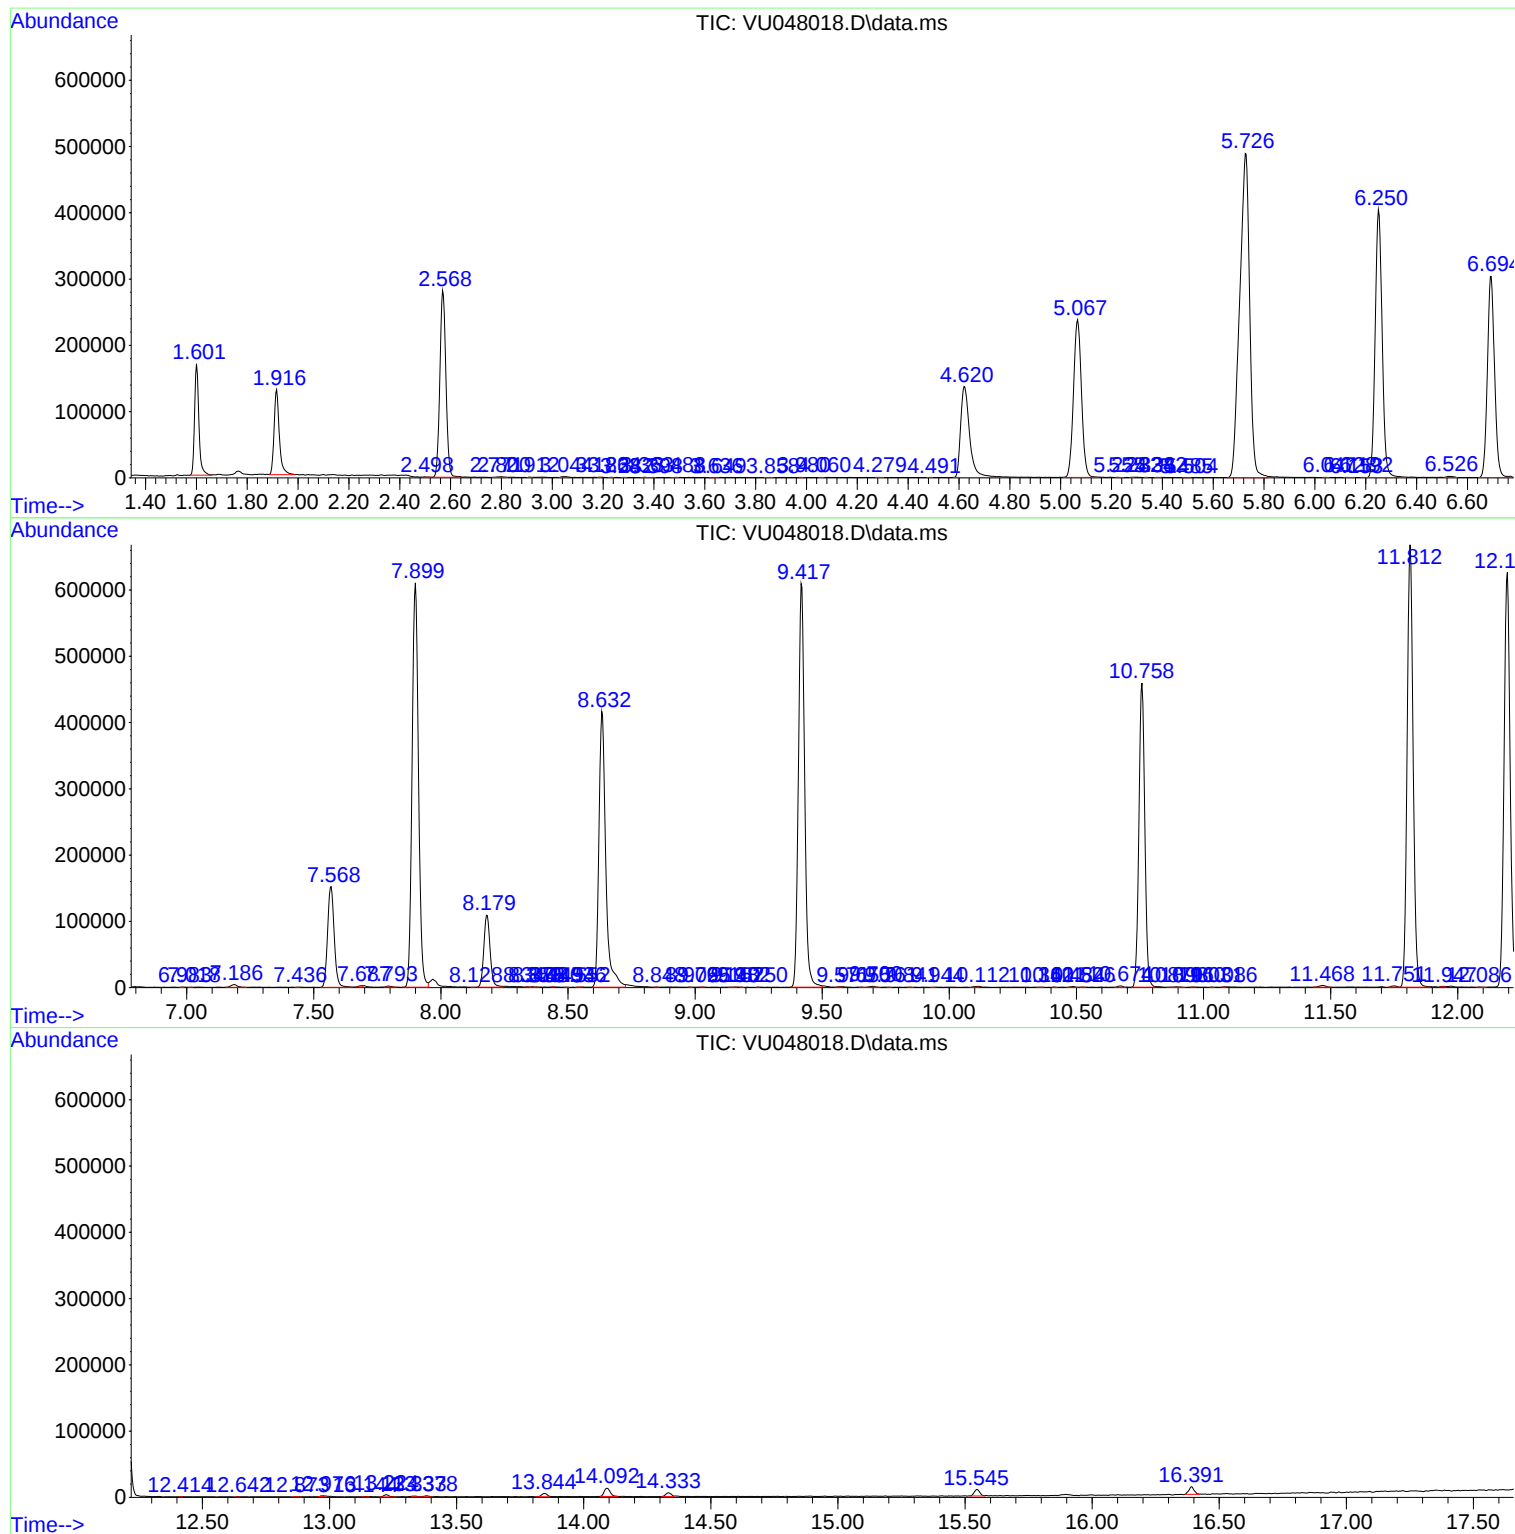

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048018.D
Acq On : 13 Apr 2022 21:12
Operator : SY/MD
Sample : VU0413WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK090

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048018.D
Acq On : 13 Apr 2022 21:12
Operator : SY/MD
Sample : VU0413WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK090

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------