

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048024.D
 Acq On : 13 Apr 2022 23:31
 Operator : SY/MD
 Sample : N2386-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	101	rBV	146744	168959	13.85%	1.664%
2	1.915	170	179	199	rBV	118042	164897	13.51%	1.624%
3	2.485	353	356	364	rVB3	972	1205	0.10%	0.012%
4	2.571	370	383	397	rBV	248577	410575	33.65%	4.043%
5	2.755	431	440	452	rBV2	10102	19139	1.57%	0.188%
6	2.854	469	471	474	rBV2	305	216	0.02%	0.002%
7	2.941	496	498	501	rBV3	358	258	0.02%	0.003%
8	2.980	507	510	514	rVB3	591	400	0.03%	0.004%
9	3.044	527	530	532	rBV2	567	341	0.03%	0.003%
10	3.076	537	540	544	rVB3	304	223	0.02%	0.002%
11	3.189	559	575	596	rBV2	43846	100878	8.27%	0.993%
12	3.385	632	636	637	rBV	326	234	0.02%	0.002%
13	3.555	686	689	694	rBV2	270	216	0.02%	0.002%
14	3.591	695	700	702	rBV	277	233	0.02%	0.002%
15	3.851	778	781	784	rVB	317	217	0.02%	0.002%
16	3.870	784	787	791	rBV3	319	244	0.02%	0.002%
17	4.009	823	830	833	rBV2	269	260	0.02%	0.003%
18	4.163	874	878	883	rBV3	287	235	0.02%	0.002%
19	4.202	883	890	894	rBV2	252	276	0.02%	0.003%
20	4.394	947	950	956	rVB3	242	209	0.02%	0.002%
21	4.517	982	988	995	rVB2	253	318	0.03%	0.003%
22	4.620	1007	1020	1052	rBV	136545	339520	27.83%	3.343%
23	4.835	1083	1087	1091	rBV3	253	262	0.02%	0.003%
24	4.967	1126	1128	1136	rVB4	470	412	0.03%	0.004%
25	5.066	1143	1159	1178	rBV	223387	482673	39.56%	4.753%
26	5.584	1317	1320	1326	rVB2	266	268	0.02%	0.003%
27	5.610	1326	1328	1332	rBV2	321	202	0.02%	0.002%
28	5.729	1338	1365	1395	rBV2	450389	1220140	100.00%	12.015%
29	6.182	1502	1506	1510	rBV2	278	227	0.02%	0.002%
30	6.250	1513	1527	1553	rBV	395323	757571	62.09%	7.460%
31	6.452	1585	1590	1592	rBV4	246	228	0.02%	0.002%
32	6.529	1605	1614	1622	rVB5	1344	2300	0.19%	0.023%
33	6.693	1650	1665	1686	rBV	280939	551876	45.23%	5.434%
34	6.870	1718	1720	1724	rVB2	312	207	0.02%	0.002%
35	6.890	1724	1726	1730	rBV2	267	197	0.02%	0.002%
36	7.002	1758	1761	1765	rVB	324	198	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048024.D
 Acq On : 13 Apr 2022 23:31
 Operator : SY/MD
 Sample : N2386-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.054	1771	1777	1787	rVV3	563	679	0.06%	0.007%
38	7.182	1809	1817	1828	rBV4	3424	5632	0.46%	0.055%
39	7.568	1924	1937	1959	rBV	139261	247568	20.29%	2.438%
40	7.690	1967	1975	1985	rVV4	2426	4184	0.34%	0.041%
41	7.754	1988	1995	1997	rBV3	334	222	0.02%	0.002%
42	7.899	2026	2040	2056	rBV	547744	954668	78.24%	9.401%
43	8.076	2093	2095	2099	rVB3	547	326	0.03%	0.003%
44	8.182	2116	2128	2142	rBV	99373	169352	13.88%	1.668%
45	8.471	2209	2218	2228	rBV4	2080	3740	0.31%	0.037%
46	8.549	2239	2242	2244	rBV2	275	203	0.02%	0.002%
47	8.632	2254	2268	2311	rBV	380363	732113	60.00%	7.209%
48	8.787	2312	2316	2323	rVB4	1443	1929	0.16%	0.019%
49	8.873	2337	2343	2345	rBV	372	321	0.03%	0.003%
50	9.031	2388	2392	2395	rVB2	246	201	0.02%	0.002%
51	9.092	2409	2411	2415	rVB2	392	220	0.02%	0.002%
52	9.172	2432	2436	2440	rVB3	658	545	0.04%	0.005%
53	9.195	2440	2443	2449	rVB2	353	351	0.03%	0.003%
54	9.320	2478	2482	2487	rVB2	394	411	0.03%	0.004%
55	9.417	2499	2512	2545	rBV	595553	1036341	84.94%	10.205%
56	9.561	2554	2557	2559	rBV2	630	360	0.03%	0.004%
57	9.639	2578	2581	2587	rBV3	393	453	0.04%	0.004%
58	9.700	2594	2600	2607	rVB3	955	1205	0.10%	0.012%
59	9.777	2621	2624	2632	rVB	274	250	0.02%	0.002%
60	9.819	2634	2637	2640	rBV	308	221	0.02%	0.002%
61	10.102	2722	2725	2729	rVB3	558	404	0.03%	0.004%
62	10.259	2770	2774	2778	rVB	294	260	0.02%	0.003%
63	10.298	2783	2786	2789	rBV3	332	253	0.02%	0.002%
64	10.381	2809	2812	2818	rVB2	352	288	0.02%	0.003%
65	10.430	2824	2827	2833	rVB2	401	360	0.03%	0.004%
66	10.465	2833	2838	2839	rBV2	347	291	0.02%	0.003%
67	10.565	2866	2869	2875	rVB2	439	319	0.03%	0.003%
68	10.671	2894	2902	2909	rBV4	1665	2205	0.18%	0.022%
69	10.758	2915	2929	2947	rBV	423691	688118	56.40%	6.776%
70	10.841	2952	2955	2961	rBV	345	312	0.03%	0.003%
71	10.896	2963	2972	2979	rBV	3445	5581	0.46%	0.055%
72	10.967	2992	2994	3003	rVV3	284	245	0.02%	0.002%
73	11.040	3012	3017	3021	rBV2	256	294	0.02%	0.003%
74	11.224	3072	3074	3079	rVB2	357	252	0.02%	0.002%
75	11.266	3079	3087	3093	rVB3	504	767	0.06%	0.008%
76	11.295	3093	3096	3099	rBV	450	353	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048024.D
 Acq On : 13 Apr 2022 23:31
 Operator : SY/MD
 Sample : N2386-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.340	3105	3110	3114	rBV2	307	339	0.03%	0.003%
78	11.458	3141	3147	3150	rBV2	1237	1594	0.13%	0.016%
79	11.568	3178	3181	3185	rVV2	307	233	0.02%	0.002%
80	11.700	3216	3222	3231	rVB4	1120	1421	0.12%	0.014%
81	11.751	3231	3238	3244	rBV5	2588	3296	0.27%	0.032%
82	11.812	3244	3257	3275	rBV	662048	1064507	87.24%	10.482%
83	12.002	3314	3316	3320	rVB2	403	222	0.02%	0.002%
84	12.073	3330	3338	3346	rBV7	3444	5706	0.47%	0.056%
85	12.195	3362	3376	3401	rBV	582870	964292	79.03%	9.495%
86	12.774	3550	3556	3564	rBV4	985	1629	0.13%	0.016%
87	12.896	3587	3594	3604	rVB5	4623	6313	0.52%	0.062%
88	12.976	3612	3619	3626	rBV4	1228	1683	0.14%	0.017%
89	13.105	3656	3659	3661	rBV2	332	238	0.02%	0.002%
90	13.227	3694	3697	3702	rVB2	744	584	0.05%	0.006%
91	13.323	3725	3727	3729	rBV2	411	234	0.02%	0.002%
92	13.375	3740	3743	3744	rBV	481	277	0.02%	0.003%
93	13.847	3882	3890	3902	rBV4	3372	4597	0.38%	0.045%
94	14.262	4016	4019	4023	rBV2	564	463	0.04%	0.005%
95	14.343	4037	4044	4047	rBV3	689	957	0.08%	0.009%
96	14.536	4102	4104	4113	rBV	358	358	0.03%	0.004%
97	14.581	4114	4118	4125	rVB4	699	746	0.06%	0.007%
98	14.822	4191	4193	4198	rBV2	446	295	0.02%	0.003%
99	15.548	4412	4419	4427	rVB6	4568	6123	0.50%	0.060%
100	15.998	4556	4559	4566	rBV4	1363	1576	0.13%	0.016%




Sum of corrected areas: 10155294

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048024.D
Acq On : 13 Apr 2022 23:31
Operator : SY/MD
Sample : N2386-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

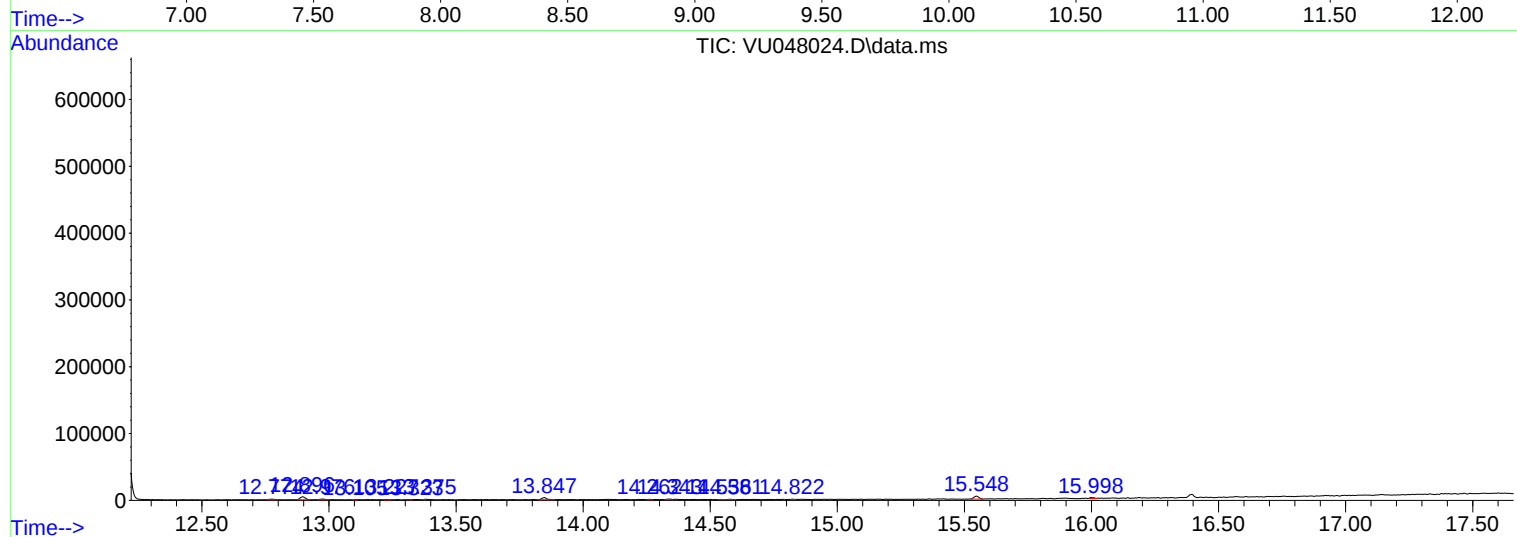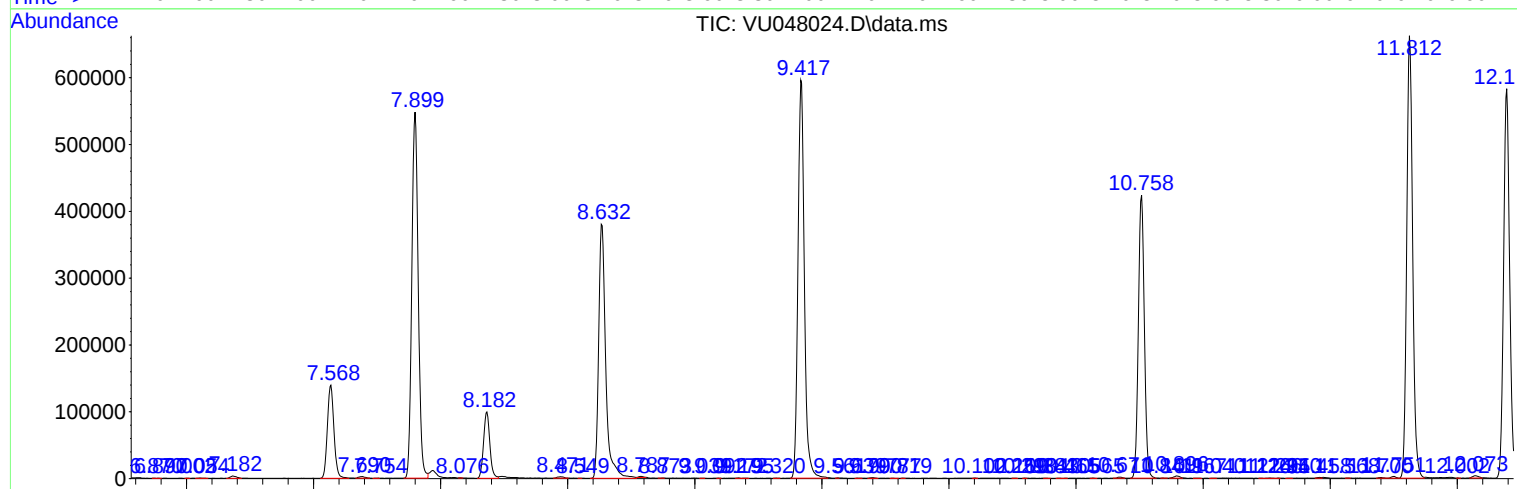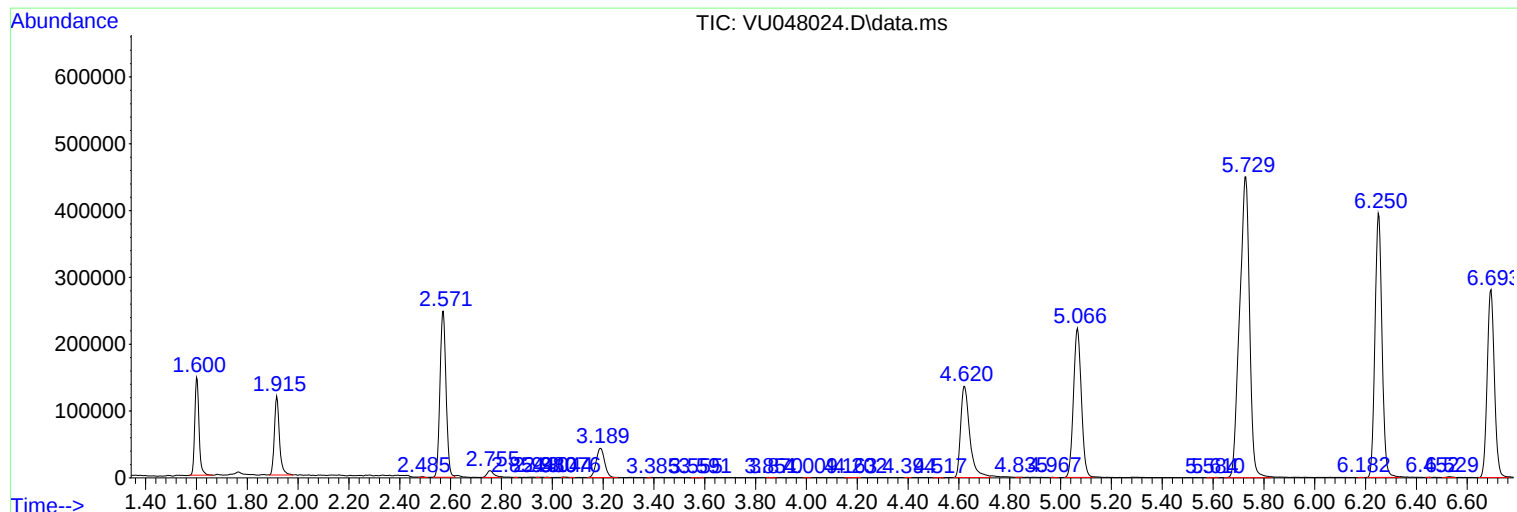

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048024.D
Acq On : 13 Apr 2022 23:31
Operator : SY/MD
Sample : N2386-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048024.D
Acq On : 13 Apr 2022 23:31
Operator : SY/MD
Sample : N2386-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc