

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048025.D
 Acq On : 13 Apr 2022 23:54
 Operator : SY/MD
 Sample : N2386-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rVB	145001	166921	13.74%	1.647%
2	1.916	169	179	196	rBV	118364	169410	13.95%	1.672%
3	2.488	351	357	361	rBV3	525	713	0.06%	0.007%
4	2.568	370	382	398	rBV	248255	408027	33.59%	4.026%
5	2.755	433	440	448	rBV2	3245	4997	0.41%	0.049%
6	2.903	484	486	490	rBV	324	245	0.02%	0.002%
7	2.951	496	501	504	rVB3	553	542	0.04%	0.005%
8	2.977	504	509	513	rBV2	552	645	0.05%	0.006%
9	3.009	517	519	525	rVB2	275	188	0.02%	0.002%
10	3.041	525	529	537	rBV5	842	1306	0.11%	0.013%
11	3.186	559	574	590	rBV	11418	26629	2.19%	0.263%
12	3.260	593	597	606	rVB2	266	415	0.03%	0.004%
13	3.385	635	636	641	rVB3	341	213	0.02%	0.002%
14	3.427	646	649	655	rVB2	298	313	0.03%	0.003%
15	3.597	699	702	706	rVB2	227	189	0.02%	0.002%
16	3.916	795	801	803	rBV2	262	229	0.02%	0.002%
17	3.970	815	818	822	rBV2	197	213	0.02%	0.002%
18	4.221	893	896	899	rBV3	276	192	0.02%	0.002%
19	4.324	925	928	932	rVB2	275	253	0.02%	0.002%
20	4.401	948	952	959	rBV2	223	336	0.03%	0.003%
21	4.620	1003	1020	1056	rBV	132039	329300	27.11%	3.249%
22	5.067	1143	1159	1186	rBV2	231158	570415	46.96%	5.629%
23	5.199	1198	1200	1204	rVB2	406	274	0.02%	0.003%
24	5.224	1204	1208	1213	rBV4	352	332	0.03%	0.003%
25	5.289	1223	1228	1230	rBV2	486	392	0.03%	0.004%
26	5.337	1240	1243	1246	rVB3	453	299	0.02%	0.003%
27	5.520	1296	1300	1302	rBV2	510	390	0.03%	0.004%
28	5.533	1302	1304	1311	rVV3	555	603	0.05%	0.006%
29	5.726	1343	1364	1391	rBV2	447542	1214729	100.00%	11.986%
30	5.999	1444	1449	1454	rBV3	392	481	0.04%	0.005%
31	6.044	1460	1463	1467	rVV2	316	300	0.02%	0.003%
32	6.112	1481	1484	1487	rVB2	341	220	0.02%	0.002%
33	6.134	1487	1491	1494	rVB2	414	291	0.02%	0.003%
34	6.250	1513	1527	1547	rBV	399205	757627	62.37%	7.476%
35	6.401	1572	1574	1576	rBV2	308	189	0.02%	0.002%
36	6.533	1607	1615	1624	rVV4	1114	2118	0.17%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048025.D
 Acq On : 13 Apr 2022 23:54
 Operator : SY/MD
 Sample : N2386-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.588	1627	1632	1634	rBV3	310	285	0.02%	0.003%
38	6.694	1648	1665	1687	rBV	280758	550710	45.34%	5.434%
39	6.893	1721	1727	1728	rBV2	561	514	0.04%	0.005%
40	6.909	1728	1732	1735	rVB2	362	261	0.02%	0.003%
41	7.102	1786	1792	1800	rVB4	478	847	0.07%	0.008%
42	7.186	1807	1818	1830	rVV5	3858	6233	0.51%	0.062%
43	7.231	1830	1832	1839	rVB2	374	280	0.02%	0.003%
44	7.279	1843	1847	1849	rBV	222	189	0.02%	0.002%
45	7.424	1888	1892	1895	rBV2	230	233	0.02%	0.002%
46	7.568	1921	1937	1964	rBV	139169	249678	20.55%	2.464%
47	7.687	1967	1974	1988	rVB5	3010	4947	0.41%	0.049%
48	7.899	2025	2040	2056	rBV	551320	958181	78.88%	9.455%
49	8.179	2115	2127	2142	rBV	97726	168516	13.87%	1.663%
50	8.359	2178	2183	2186	rVB3	422	374	0.03%	0.004%
51	8.472	2212	2218	2219	rBV3	1072	842	0.07%	0.008%
52	8.633	2255	2268	2308	rBV	385263	736785	60.65%	7.270%
53	8.915	2352	2356	2358	rBV	397	318	0.03%	0.003%
54	8.957	2366	2369	2376	rBV3	501	540	0.04%	0.005%
55	9.054	2394	2399	2401	rBV2	300	236	0.02%	0.002%
56	9.070	2401	2404	2407	rBV	221	196	0.02%	0.002%
57	9.173	2430	2436	2439	rVB4	558	628	0.05%	0.006%
58	9.227	2449	2453	2457	rVB3	275	230	0.02%	0.002%
59	9.276	2465	2468	2470	rBV2	271	212	0.02%	0.002%
60	9.324	2480	2483	2485	rBV2	482	254	0.02%	0.003%
61	9.417	2498	2512	2554	rVV	602788	1031991	84.96%	10.183%
62	9.581	2560	2563	2569	rVB4	509	401	0.03%	0.004%
63	9.613	2569	2573	2578	rBV2	355	248	0.02%	0.002%
64	9.642	2578	2582	2586	rBV2	330	332	0.03%	0.003%
65	9.694	2592	2598	2599	rBV2	812	822	0.07%	0.008%
66	9.829	2638	2640	2646	rVB2	400	362	0.03%	0.004%
67	10.095	2718	2723	2725	rBV2	424	317	0.03%	0.003%
68	10.269	2772	2777	2779	rBV	247	229	0.02%	0.002%
69	10.327	2792	2795	2800	rVB	294	252	0.02%	0.002%
70	10.375	2806	2810	2816	rBV2	327	351	0.03%	0.003%
71	10.468	2835	2839	2840	rBV2	360	240	0.02%	0.002%
72	10.520	2850	2855	2860	rBV2	219	294	0.02%	0.003%
73	10.626	2886	2888	2894	rVB2	339	260	0.02%	0.003%
74	10.674	2895	2903	2911	rBV5	1458	1971	0.16%	0.019%
75	10.758	2915	2929	2952	rVB	430861	692516	57.01%	6.833%
76	10.890	2962	2970	2971	rBV4	2221	1705	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048025.D
 Acq On : 13 Apr 2022 23:54
 Operator : SY/MD
 Sample : N2386-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.092	3031	3033	3037	rVV2	491	188	0.02%	0.002%
78	11.153	3050	3052	3058	rVB3	339	296	0.02%	0.003%
79	11.340	3105	3110	3114	rBV2	305	288	0.02%	0.003%
80	11.394	3124	3127	3130	rBV	332	269	0.02%	0.003%
81	11.456	3141	3146	3149	rBV4	1113	1197	0.10%	0.012%
82	11.703	3216	3223	3226	rVB5	758	998	0.08%	0.010%
83	11.748	3230	3237	3244	rVV5	2542	3218	0.26%	0.032%
84	11.812	3244	3257	3282	rBV	663449	1066006	87.76%	10.519%
85	11.999	3313	3315	3319	rBV2	285	260	0.02%	0.003%
86	12.066	3330	3336	3349	rBV5	3728	6765	0.56%	0.067%
87	12.195	3362	3376	3392	rBV	580827	958236	78.88%	9.455%
88	12.546	3482	3485	3488	rBV2	231	195	0.02%	0.002%
89	12.767	3551	3554	3556	rBV2	380	298	0.02%	0.003%
90	12.816	3564	3569	3572	rBV3	257	307	0.03%	0.003%
91	12.896	3589	3594	3602	rVB6	1665	1899	0.16%	0.019%
92	12.973	3614	3618	3626	rVB3	1223	1479	0.12%	0.015%
93	13.291	3712	3717	3726	rVB3	495	621	0.05%	0.006%
94	13.333	3726	3730	3733	rBV2	986	903	0.07%	0.009%
95	13.382	3742	3745	3751	rBV4	587	418	0.03%	0.004%
96	13.845	3881	3889	3899	rBV5	5722	8365	0.69%	0.083%
97	14.333	4036	4041	4048	rBV5	2317	2666	0.22%	0.026%
98	14.809	4187	4189	4199	rVB3	605	820	0.07%	0.008%
99	14.870	4206	4208	4214	rBV3	431	333	0.03%	0.003%
100	15.545	4412	4418	4427	rBV8	3218	4515	0.37%	0.045%




Sum of corrected areas: 10134256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048025.D
Acq On : 13 Apr 2022 23:54
Operator : SY/MD
Sample : N2386-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

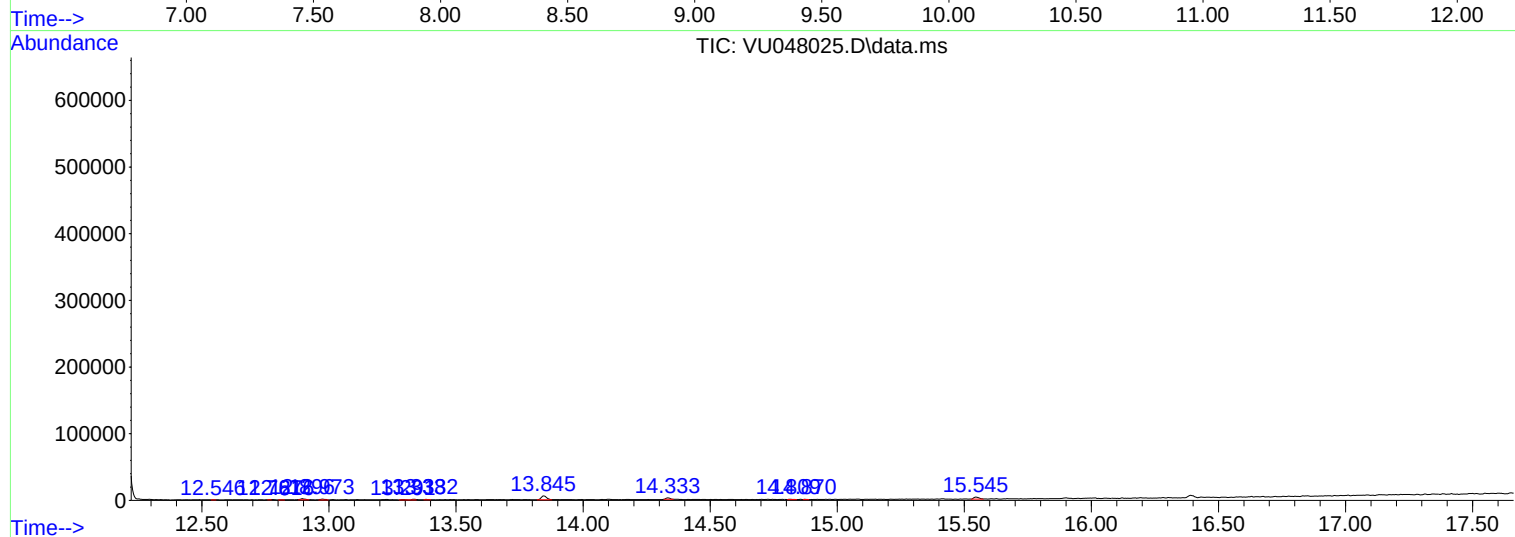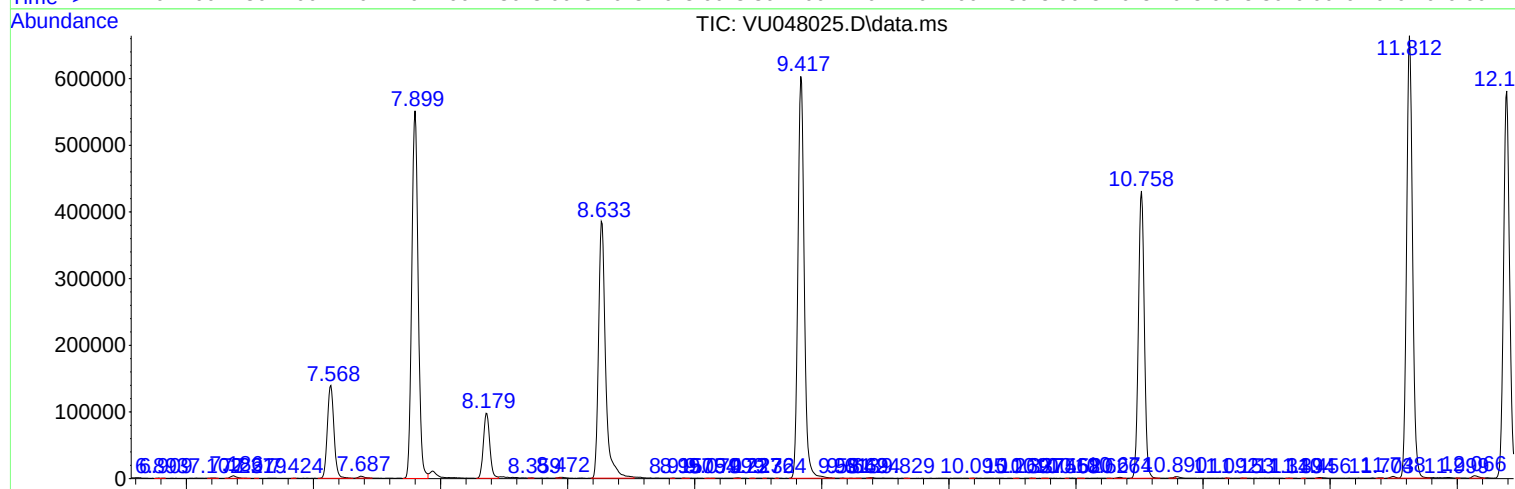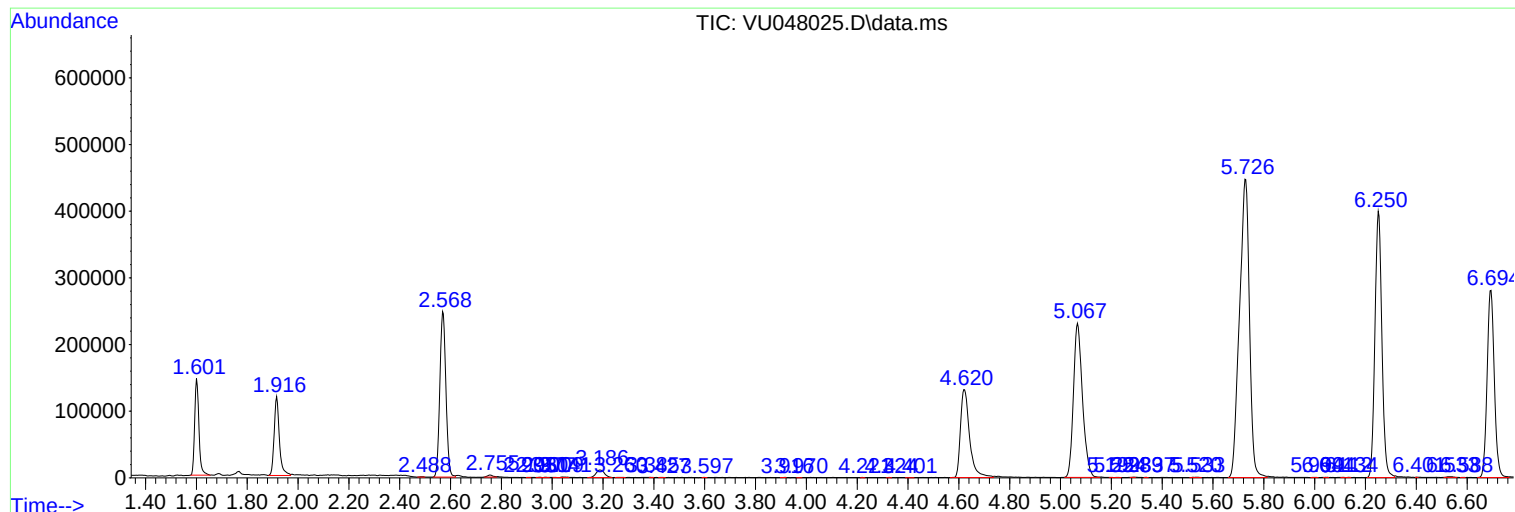

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048025.D
Acq On : 13 Apr 2022 23:54
Operator : SY/MD
Sample : N2386-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048025.D
Acq On : 13 Apr 2022 23:54
Operator : SY/MD
Sample : N2386-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc