

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048031.D
 Acq On : 14 Apr 2022 02:13
 Operator : SY/MD
 Sample : N2387-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rBV	137536	160052	2.75%	0.735%
2	1.916	171	179	203	rVB	118810	165829	2.84%	0.762%
3	2.572	370	383	399	rBV	247467	403312	6.92%	1.852%
4	2.684	414	418	422	rBV2	441	404	0.01%	0.002%
5	2.755	430	440	460	rBV	6615	14975	0.26%	0.069%
6	2.925	491	493	496	rBV	405	293	0.01%	0.001%
7	2.944	496	499	500	rBV2	244	169	0.00%	0.001%
8	3.051	523	532	542	rBV2	5110	9272	0.16%	0.043%
9	3.121	550	554	557	rBV2	487	410	0.01%	0.002%
10	3.179	566	572	574	rBV4	818	692	0.01%	0.003%
11	3.285	600	605	608	rBV2	318	242	0.00%	0.001%
12	3.417	639	646	651	rVB3	487	581	0.01%	0.003%
13	3.449	651	656	658	rBV2	406	353	0.01%	0.002%
14	3.742	744	747	755	rVB2	441	480	0.01%	0.002%
15	3.777	755	758	759	rBV2	329	183	0.00%	0.001%
16	3.835	773	776	779	rVV2	263	201	0.00%	0.001%
17	3.983	818	822	826	rBV	346	308	0.01%	0.001%
18	4.025	832	835	840	rBV2	298	324	0.01%	0.001%
19	4.112	855	862	863	rBV	264	291	0.00%	0.001%
20	4.253	903	906	908	rBV3	388	254	0.00%	0.001%
21	4.620	1005	1020	1045	rBV	131347	314342	5.39%	1.444%
22	5.067	1142	1159	1184	rBV	218918	483555	8.30%	2.221%
23	5.250	1211	1216	1221	rBV2	209	171	0.00%	0.001%
24	5.279	1221	1225	1226	rBV	415	288	0.00%	0.001%
25	5.333	1238	1242	1248	rVV2	359	363	0.01%	0.002%
26	5.398	1257	1262	1265	rVV2	515	425	0.01%	0.002%
27	5.427	1265	1271	1275	rVB2	262	285	0.00%	0.001%
28	5.523	1293	1301	1313	rVB5	1649	3195	0.05%	0.015%
29	5.623	1326	1332	1334	rBV	245	267	0.00%	0.001%
30	5.729	1342	1365	1370	rBV2	443502	1127958	19.35%	5.180%
31	5.777	1372	1380	1415	rVB	1397089	2748180	47.14%	12.621%
32	6.083	1473	1475	1477	rBV2	439	237	0.00%	0.001%
33	6.250	1512	1527	1558	rBV	395400	743994	12.76%	3.417%
34	6.395	1569	1572	1575	rBV2	425	238	0.00%	0.001%
35	6.446	1586	1588	1595	rVB4	242	237	0.00%	0.001%
36	6.526	1607	1613	1621	rVB4	1262	1744	0.03%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048031.D
 Acq On : 14 Apr 2022 02:13
 Operator : SY/MD
 Sample : N2387-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1690	rBV	280320	547624	9.39%	2.515%
38	6.796	1694	1697	1698	rBV2	596	288	0.00%	0.001%
39	6.864	1715	1718	1721	rBV2	275	215	0.00%	0.001%
40	6.973	1748	1752	1756	rVB3	245	206	0.00%	0.001%
41	7.038	1766	1772	1773	rBV2	385	297	0.01%	0.001%
42	7.182	1809	1817	1828	rBV3	3550	6249	0.11%	0.029%
43	7.304	1852	1855	1859	rBV3	270	233	0.00%	0.001%
44	7.378	1873	1878	1881	rBV2	377	346	0.01%	0.002%
45	7.452	1897	1901	1903	rBV2	206	207	0.00%	0.001%
46	7.568	1923	1937	1960	rBV	134382	238910	4.10%	1.097%
47	7.687	1965	1974	1984	rBV4	2573	4277	0.07%	0.020%
48	7.800	2005	2009	2012	rBV3	318	272	0.00%	0.001%
49	7.899	2026	2040	2055	rBV	552044	940043	16.13%	4.317%
50	8.179	2116	2127	2141	rBV	95096	161805	2.78%	0.743%
51	8.407	2196	2198	2202	rVB3	286	171	0.00%	0.001%
52	8.430	2202	2205	2206	rBV	291	170	0.00%	0.001%
53	8.578	2247	2251	2256	rBV3	253	310	0.01%	0.001%
54	8.632	2256	2268	2314	rBV	394897	737400	12.65%	3.387%
55	8.954	2365	2368	2371	rVV	325	266	0.00%	0.001%
56	8.973	2371	2374	2377	rVB2	588	445	0.01%	0.002%
57	9.018	2386	2388	2390	rBV	356	188	0.00%	0.001%
58	9.076	2403	2406	2410	rVB2	284	208	0.00%	0.001%
59	9.124	2418	2421	2426	rVV2	210	253	0.00%	0.001%
60	9.166	2429	2434	2440	rVB4	648	655	0.01%	0.003%
61	9.201	2440	2445	2448	rVB2	315	286	0.00%	0.001%
62	9.333	2482	2486	2490	rBV2	228	198	0.00%	0.001%
63	9.449	2499	2522	2558	rBV2	2928627	5829224	100.00%	26.772%
64	9.690	2592	2597	2603	rBV3	1265	1349	0.02%	0.006%
65	9.761	2615	2619	2623	rVB	579	404	0.01%	0.002%
66	9.816	2634	2636	2642	rVB	352	306	0.01%	0.001%
67	9.947	2671	2677	2680	rVB2	278	296	0.01%	0.001%
68	9.970	2680	2684	2687	rBV2	297	263	0.00%	0.001%
69	10.095	2720	2723	2725	rBV2	465	296	0.01%	0.001%
70	10.144	2735	2738	2742	rVB2	311	196	0.00%	0.001%
71	10.449	2831	2833	2836	rVB	262	160	0.00%	0.001%
72	10.668	2896	2901	2909	rVB4	1163	1374	0.02%	0.006%
73	10.758	2915	2929	2949	rBV	433801	702731	12.06%	3.227%
74	10.893	2967	2971	2979	rVV2	751	999	0.02%	0.005%
75	10.925	2979	2981	2985	rVB3	408	306	0.01%	0.001%
76	10.976	2994	2997	3000	rBV2	274	234	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048031.D
 Acq On : 14 Apr 2022 02:13
 Operator : SY/MD
 Sample : N2387-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

77	11.025	3006	3012	3015	rBV2	237	224	0.00%	0.001%
78	11.301	3095	3098	3100	rBV2	326	201	0.00%	0.001%
79	11.465	3144	3149	3159	rVB5	988	1600	0.03%	0.007%
80	11.645	3203	3205	3208	rBV2	314	177	0.00%	0.001%
81	11.697	3215	3221	3225	rBV3	745	807	0.01%	0.004%
82	11.745	3225	3236	3246	rBV	80762	127124	2.18%	0.584%
83	11.835	3246	3264	3287	rVB2	1553365	3385289	58.07%	15.548%
84	12.015	3316	3320	3321	rBV	436	319	0.01%	0.001%
85	12.047	3328	3330	3333	rVB	334	198	0.00%	0.001%
86	12.076	3333	3339	3341	rBV3	484	558	0.01%	0.003%
87	12.211	3361	3381	3402	rBV2	1204035	2647781	45.42%	12.160%
88	12.629	3508	3511	3512	rBV	385	201	0.00%	0.001%
89	12.668	3519	3523	3524	rBV2	327	248	0.00%	0.001%
90	12.774	3553	3556	3559	rBV2	490	343	0.01%	0.002%
91	12.973	3614	3618	3626	rVB6	1295	1669	0.03%	0.008%
92	13.086	3649	3653	3658	rBV2	402	443	0.01%	0.002%
93	13.221	3685	3695	3705	rBV6	1720	3786	0.06%	0.017%
94	13.433	3758	3761	3764	rBV2	418	302	0.01%	0.001%
95	13.565	3799	3802	3807	rBV3	542	497	0.01%	0.002%
96	13.713	3846	3848	3852	rBV4	346	229	0.00%	0.001%
97	13.841	3877	3888	3905	rBV	133433	214343	3.68%	0.984%
98	14.333	4031	4041	4054	rVB2	13885	22754	0.39%	0.105%
99	14.381	4054	4056	4059	rBV	368	239	0.00%	0.001%
100	15.147	4290	4294	4296	rBV3	889	722	0.01%	0.003%




Sum of corrected areas: 21773818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048031.D
Acq On : 14 Apr 2022 02:13
Operator : SY/MD
Sample : N2387-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

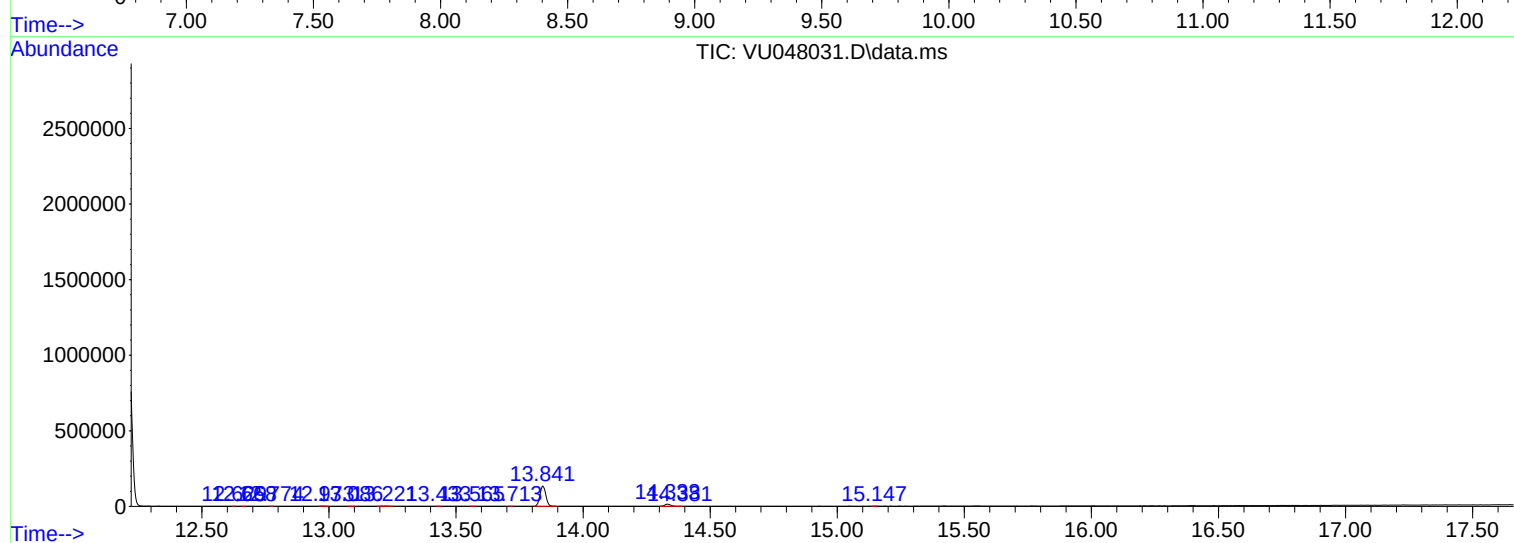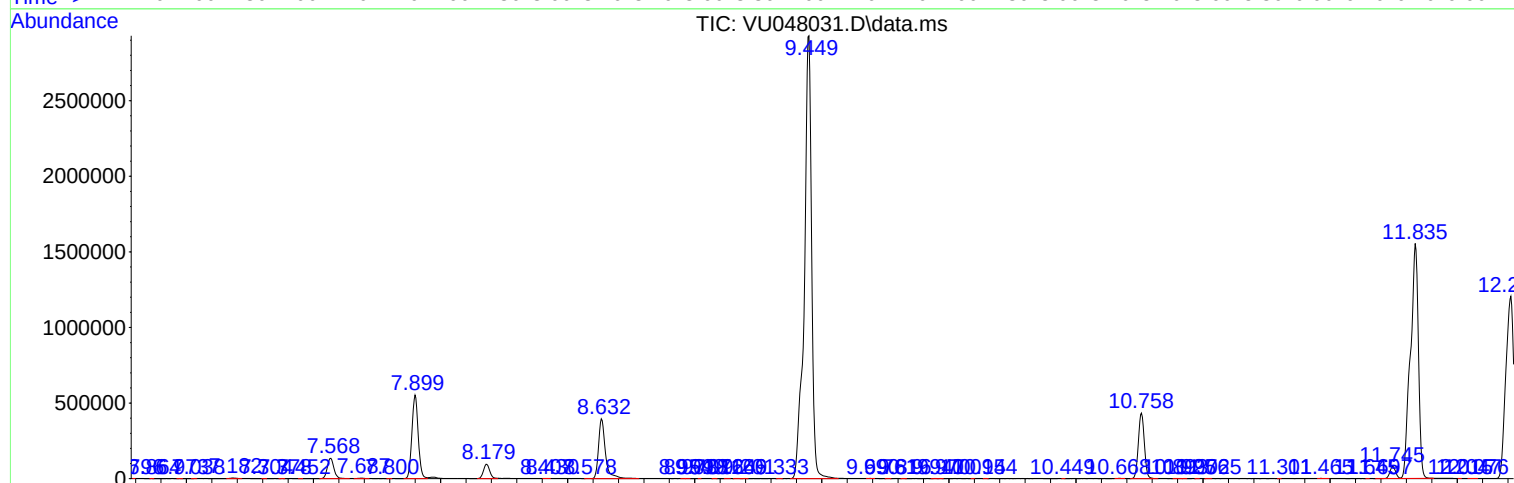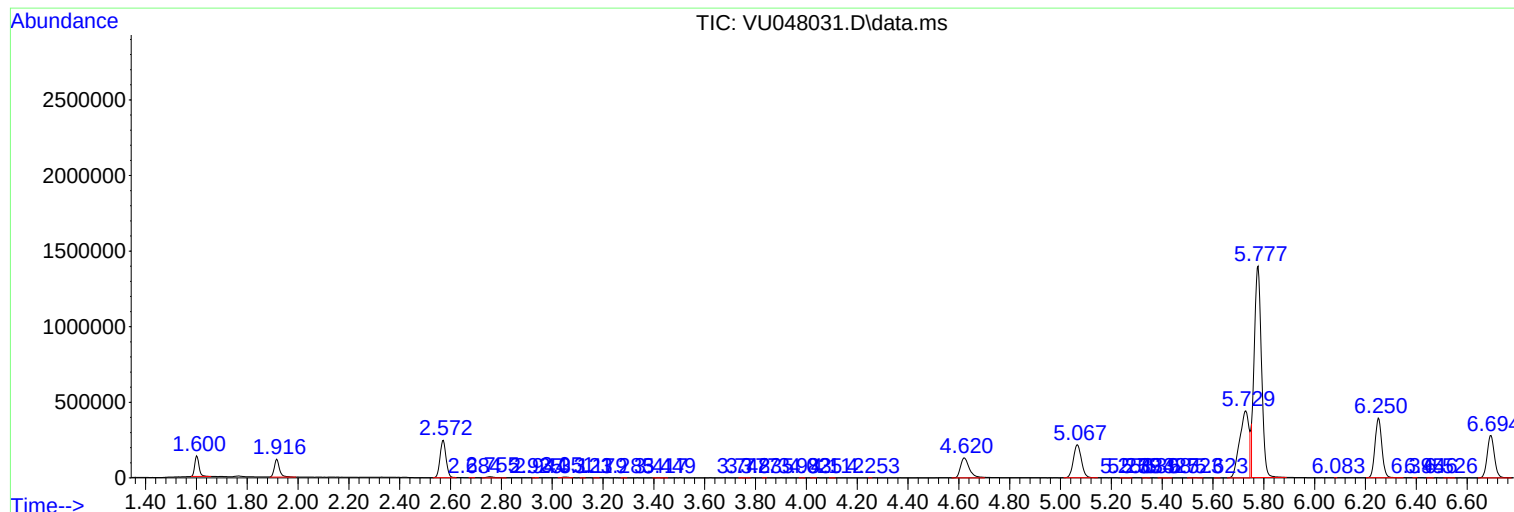

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048031.D
Acq On : 14 Apr 2022 02:13
Operator : SY/MD
Sample : N2387-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048031.D
Acq On : 14 Apr 2022 02:13
Operator : SY/MD
Sample : N2387-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc