

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048032.D
 Acq On : 14 Apr 2022 02:36
 Operator : SY/MD
 Sample : N2387-03 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rBV	144508	166388	13.38%	1.637%
2	1.916	171	179	198	rVB	121916	170536	13.71%	1.678%
3	2.572	370	383	397	rBV	249861	411151	33.06%	4.045%
4	2.681	414	417	420	rBV2	243	185	0.01%	0.002%
5	2.758	431	441	453	rBV2	2895	6438	0.52%	0.063%
6	2.803	453	455	458	rVB3	445	245	0.02%	0.002%
7	2.958	501	503	506	rVV2	417	244	0.02%	0.002%
8	3.051	522	532	544	rVV2	5361	9998	0.80%	0.098%
9	3.250	591	594	603	rVB2	223	286	0.02%	0.003%
10	3.298	606	609	612	rBV	355	251	0.02%	0.002%
11	3.511	670	675	681	rVB2	351	392	0.03%	0.004%
12	3.565	688	692	696	rVB2	303	234	0.02%	0.002%
13	3.591	696	700	704	rBV3	381	364	0.03%	0.004%
14	3.713	733	738	739	rBV2	256	240	0.02%	0.002%
15	3.729	739	743	748	rVB3	355	311	0.03%	0.003%
16	3.842	777	778	783	rVB3	307	239	0.02%	0.002%
17	3.877	783	789	791	rBV2	395	367	0.03%	0.004%
18	3.957	809	814	817	rBV	409	339	0.03%	0.003%
19	4.295	916	919	923	rBV2	449	406	0.03%	0.004%
20	4.620	1008	1020	1059	rBV	132866	327724	26.35%	3.224%
21	5.067	1142	1159	1184	rVV	224730	491732	39.54%	4.837%
22	5.295	1219	1230	1238	rBV4	738	1169	0.09%	0.011%
23	5.408	1261	1265	1270	rVV2	296	325	0.03%	0.003%
24	5.572	1312	1316	1318	rBV2	290	231	0.02%	0.002%
25	5.726	1343	1364	1389	rBV2	451425	1243601	100.00%	12.233%
26	5.912	1420	1422	1423	rBV	381	182	0.01%	0.002%
27	5.983	1439	1444	1448	rVB4	369	414	0.03%	0.004%
28	6.012	1448	1453	1455	rBV3	357	381	0.03%	0.004%
29	6.041	1458	1462	1466	rVB2	541	439	0.04%	0.004%
30	6.250	1512	1527	1551	rBV	395152	757614	60.92%	7.453%
31	6.494	1599	1603	1607	rVV2	356	423	0.03%	0.004%
32	6.536	1607	1616	1628	rVB6	1487	2709	0.22%	0.027%
33	6.588	1628	1632	1635	rBV3	287	227	0.02%	0.002%
34	6.694	1648	1665	1686	rBV	289957	564887	45.42%	5.557%
35	6.797	1695	1697	1698	rBV	628	304	0.02%	0.003%
36	6.851	1708	1714	1717	rBV3	370	272	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048032.D
 Acq On : 14 Apr 2022 02:36
 Operator : SY/MD
 Sample : N2387-03 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.938	1736	1741	1742	rBV	416	280	0.02%	0.003%
38	6.999	1756	1760	1762	rBV	243	211	0.02%	0.002%
39	7.051	1769	1776	1778	rBV2	398	405	0.03%	0.004%
40	7.080	1783	1785	1791	rBV3	195	223	0.02%	0.002%
41	7.112	1791	1795	1798	rVB2	301	220	0.02%	0.002%
42	7.137	1798	1803	1808	rBV2	289	421	0.03%	0.004%
43	7.186	1808	1818	1827	rVV5	3913	6653	0.53%	0.065%
44	7.568	1919	1937	1960	rBV	140272	248591	19.99%	2.445%
45	7.684	1966	1973	1975	rBV4	2408	2453	0.20%	0.024%
46	7.723	1983	1985	1992	rVB5	712	578	0.05%	0.006%
47	7.797	2006	2008	2014	rBV3	388	323	0.03%	0.003%
48	7.899	2022	2040	2055	rBV	567915	969331	77.95%	9.535%
49	8.179	2115	2127	2141	rBV	97137	166825	13.41%	1.641%
50	8.417	2195	2201	2205	rBV4	277	351	0.03%	0.003%
51	8.465	2213	2216	2219	rBV2	252	187	0.02%	0.002%
52	8.633	2255	2268	2303	rBV	399969	750813	60.37%	7.386%
53	8.896	2346	2350	2356	rVB2	458	310	0.02%	0.003%
54	8.941	2360	2364	2370	rBV2	414	463	0.04%	0.005%
55	8.967	2370	2372	2375	rBV2	354	202	0.02%	0.002%
56	8.999	2379	2382	2384	rBV	286	181	0.01%	0.002%
57	9.134	2421	2424	2426	rBV	326	224	0.02%	0.002%
58	9.292	2469	2473	2478	rBV3	385	469	0.04%	0.005%
59	9.346	2487	2490	2492	rVV	245	186	0.01%	0.002%
60	9.417	2496	2512	2555	rBV	601783	1052013	84.59%	10.349%
61	9.578	2560	2562	2567	rVB2	393	287	0.02%	0.003%
62	9.639	2579	2581	2588	rVB4	436	447	0.04%	0.004%
63	9.694	2588	2598	2605	rBV2	1003	1682	0.14%	0.017%
64	9.764	2617	2620	2625	rVB2	257	186	0.01%	0.002%
65	9.835	2638	2642	2646	rVB3	258	236	0.02%	0.002%
66	10.099	2721	2724	2729	rVV3	323	369	0.03%	0.004%
67	10.192	2749	2753	2757	rVV	208	193	0.02%	0.002%
68	10.263	2772	2775	2780	rVB2	246	214	0.02%	0.002%
69	10.449	2831	2833	2837	rBV2	204	187	0.02%	0.002%
70	10.604	2877	2881	2886	rBV2	389	298	0.02%	0.003%
71	10.632	2886	2890	2892	rVV2	217	179	0.01%	0.002%
72	10.671	2896	2902	2909	rVB3	1451	1625	0.13%	0.016%
73	10.758	2914	2929	2954	rVV	444662	712892	57.32%	7.013%
74	10.903	2971	2974	2977	rVB3	481	272	0.02%	0.003%
75	11.018	3007	3010	3013	rBV3	288	223	0.02%	0.002%
76	11.160	3047	3054	3061	rBV3	451	682	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048032.D
 Acq On : 14 Apr 2022 02:36
 Operator : SY/MD
 Sample : N2387-03 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.192	3061	3064	3070	rBV3	287	317	0.03%	0.003%
78	11.327	3103	3106	3111	rBV3	301	256	0.02%	0.003%
79	11.353	3111	3114	3119	rBV2	345	257	0.02%	0.003%
80	11.462	3144	3148	3151	rBV4	756	628	0.05%	0.006%
81	11.581	3182	3185	3189	rVB3	434	347	0.03%	0.003%
82	11.668	3208	3212	3214	rBV2	438	355	0.03%	0.003%
83	11.703	3219	3223	3228	rVB4	537	436	0.04%	0.004%
84	11.751	3228	3238	3244	rBV4	1276	1983	0.16%	0.020%
85	11.812	3244	3257	3277	rBV	660464	1082202	87.02%	10.646%
86	12.038	3324	3327	3329	rBV	330	178	0.01%	0.002%
87	12.095	3343	3345	3349	rVB2	339	229	0.02%	0.002%
88	12.128	3352	3355	3358	rVB	298	171	0.01%	0.002%
89	12.195	3363	3376	3394	rBV	587431	983603	79.09%	9.676%
90	12.378	3431	3433	3436	rBV3	295	207	0.02%	0.002%
91	12.581	3494	3496	3498	rBV	346	186	0.01%	0.002%
92	12.642	3512	3515	3519	rBV3	346	306	0.02%	0.003%
93	12.816	3566	3569	3573	rBB3	247	177	0.01%	0.002%
94	12.976	3616	3619	3623	rVB4	466	332	0.03%	0.003%
95	13.288	3713	3716	3718	rBV3	304	204	0.02%	0.002%
96	13.391	3746	3748	3753	rVB3	299	199	0.02%	0.002%
97	13.845	3881	3889	3901	rBV2	5778	9038	0.73%	0.089%
98	14.250	4012	4015	4018	rBV2	407	316	0.03%	0.003%
99	14.365	4049	4051	4056	rVB3	473	254	0.02%	0.002%
100	14.880	4209	4211	4214	rVB2	501	259	0.02%	0.003%




Sum of corrected areas: 10165573

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048032.D
Acq On : 14 Apr 2022 02:36
Operator : SY/MD
Sample : N2387-03 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

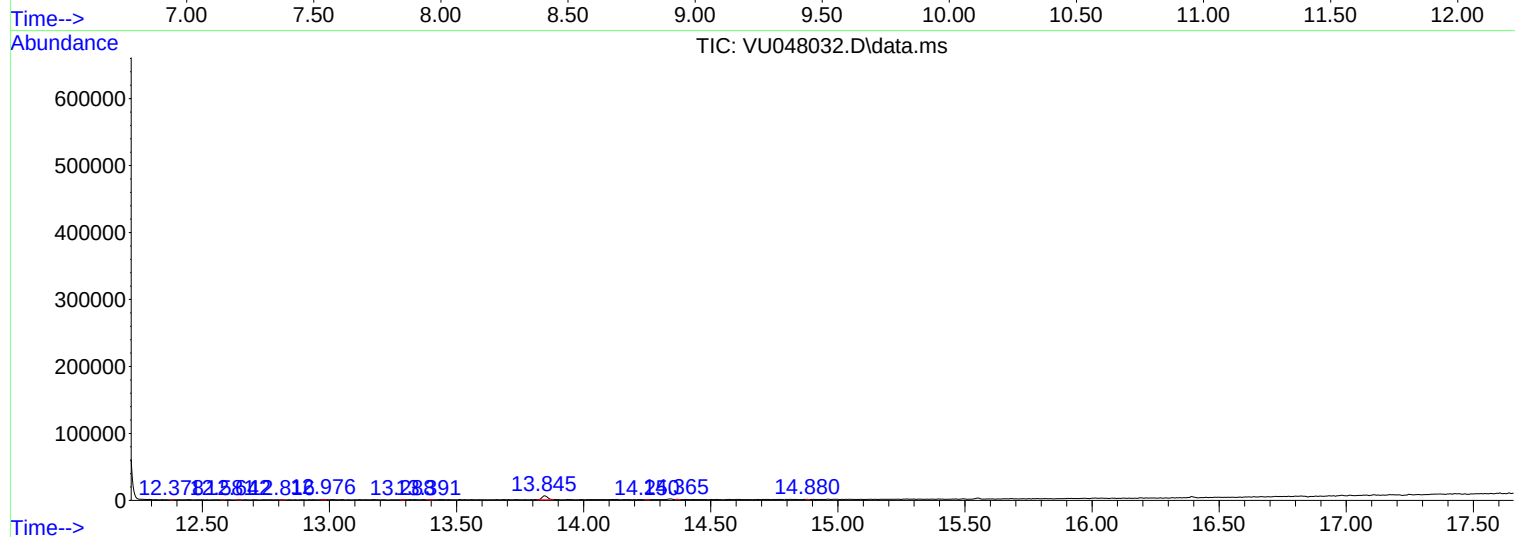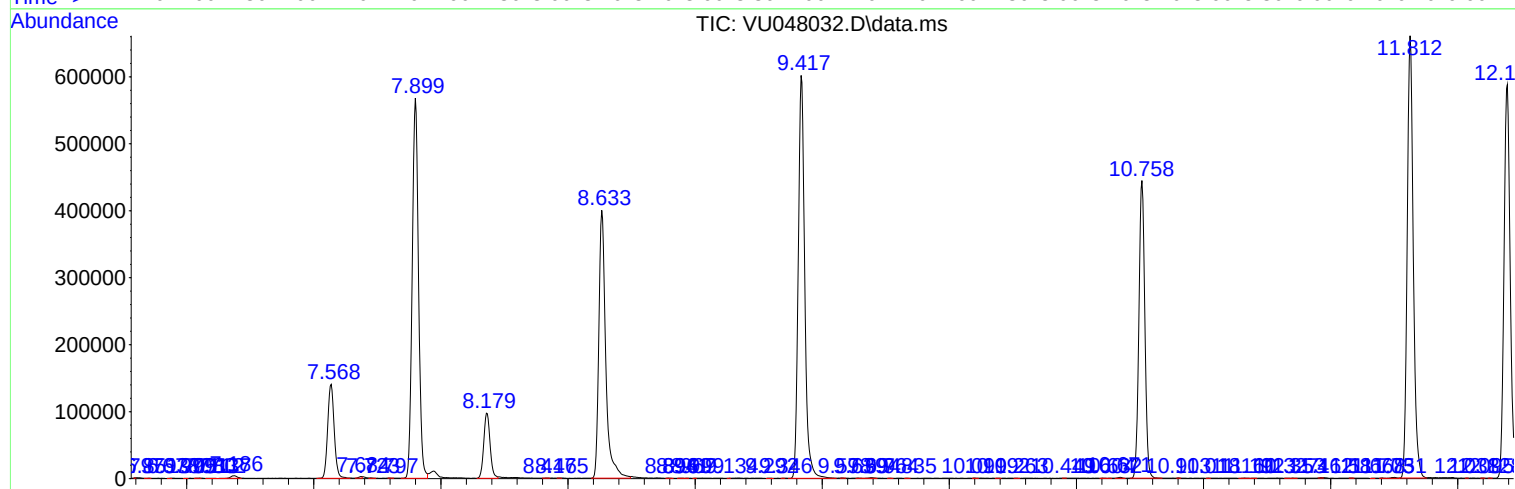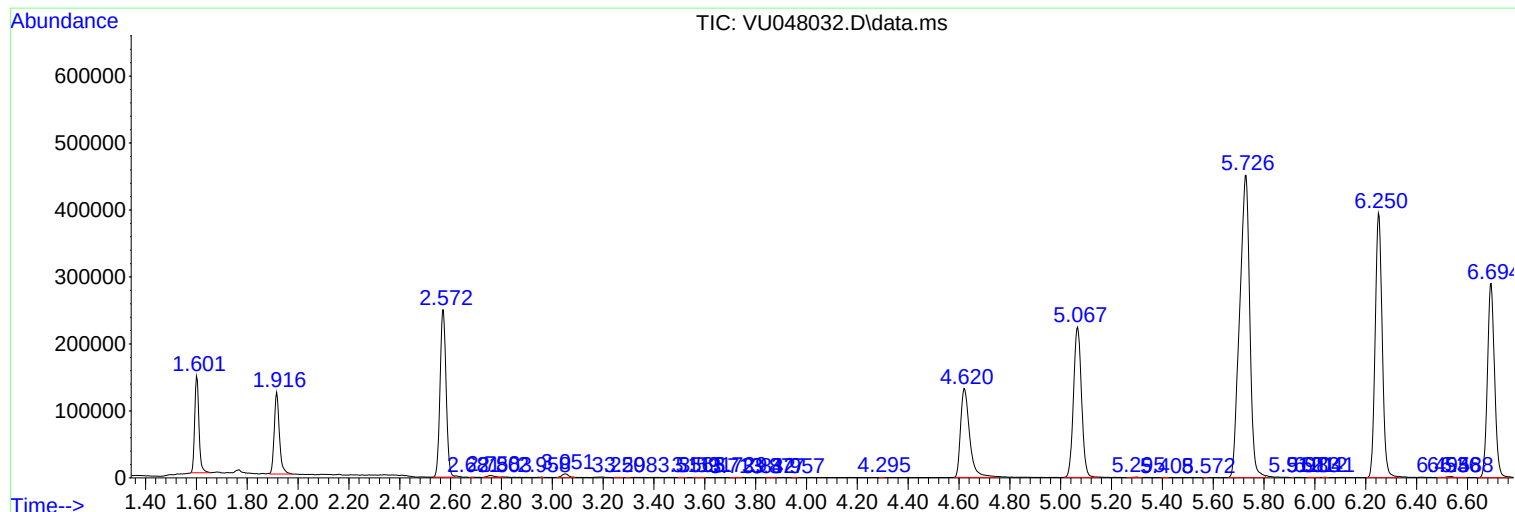

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048032.D
Acq On : 14 Apr 2022 02:36
Operator : SY/MD
Sample : N2387-03 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048032.D
Acq On : 14 Apr 2022 02:36
Operator : SY/MD
Sample : N2387-03 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc