

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048033.D
 Acq On : 14 Apr 2022 02:59
 Operator : SY/MD
 Sample : N2387-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	95	rBV	140234	162172	13.26%	1.634%
2	1.916	171	179	199	rVB	118684	163691	13.38%	1.649%
3	2.572	370	383	399	rBV	248868	407535	33.32%	4.106%
4	2.671	411	414	416	rBV2	317	208	0.02%	0.002%
5	2.713	425	427	430	rBV3	299	231	0.02%	0.002%
6	2.755	432	440	453	rVV4	1656	3356	0.27%	0.034%
7	2.938	492	497	502	rBV3	337	484	0.04%	0.005%
8	2.964	502	505	511	rVB3	527	497	0.04%	0.005%
9	3.051	522	532	543	rBV3	5410	10443	0.85%	0.105%
10	3.192	571	576	580	rVB3	686	668	0.05%	0.007%
11	3.346	619	624	628	rVB3	226	231	0.02%	0.002%
12	3.372	628	632	635	rBV2	287	230	0.02%	0.002%
13	3.472	659	663	666	rVB3	299	240	0.02%	0.002%
14	3.526	675	680	685	rVB2	375	487	0.04%	0.005%
15	3.600	699	703	709	rVB2	262	221	0.02%	0.002%
16	3.652	717	719	722	rVB	357	226	0.02%	0.002%
17	3.681	722	728	732	rBV3	306	423	0.03%	0.004%
18	3.935	803	807	810	rVV2	246	243	0.02%	0.002%
19	4.038	834	839	842	rBV2	321	295	0.02%	0.003%
20	4.083	850	853	856	rVV2	222	194	0.02%	0.002%
21	4.163	870	878	881	rBV	290	434	0.04%	0.004%
22	4.231	894	899	904	rBV3	324	310	0.03%	0.003%
23	4.269	904	911	917	rBV2	170	233	0.02%	0.002%
24	4.420	954	958	963	rVB3	353	334	0.03%	0.003%
25	4.449	963	967	972	rBV2	252	282	0.02%	0.003%
26	4.485	972	978	983	rBV2	169	188	0.02%	0.002%
27	4.623	1004	1021	1072	rBV	130598	328002	26.81%	3.305%
28	4.896	1104	1106	1108	rBV	357	212	0.02%	0.002%
29	5.067	1139	1159	1185	rBV	221883	487316	39.84%	4.910%
30	5.292	1224	1229	1236	rBV	747	829	0.07%	0.008%
31	5.382	1256	1257	1262	rVB2	349	228	0.02%	0.002%
32	5.427	1262	1271	1273	rBV2	319	476	0.04%	0.005%
33	5.565	1311	1314	1317	rBV2	226	200	0.02%	0.002%
34	5.729	1342	1365	1393	rBV2	446987	1223231	100.00%	12.325%
35	6.044	1460	1463	1471	rVB3	246	234	0.02%	0.002%
36	6.195	1507	1510	1513	rVB2	354	200	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048033.D
 Acq On : 14 Apr 2022 02:59
 Operator : SY/MD
 Sample : N2387-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1513	1527	1560	rBV	391441	744922	60.90%	7.506%
38	6.472	1592	1596	1602	rVB3	384	442	0.04%	0.004%
39	6.526	1602	1613	1622	rBV5	1338	2453	0.20%	0.025%
40	6.629	1642	1645	1649	rVB2	353	257	0.02%	0.003%
41	6.694	1649	1665	1687	rBV	282540	555424	45.41%	5.596%
42	6.857	1713	1716	1723	rVB3	316	398	0.03%	0.004%
43	6.909	1730	1732	1735	rBV	269	214	0.02%	0.002%
44	7.047	1768	1775	1777	rBV3	321	391	0.03%	0.004%
45	7.144	1801	1805	1808	rBV	291	244	0.02%	0.002%
46	7.185	1808	1818	1826	rBV4	3361	6198	0.51%	0.062%
47	7.269	1842	1844	1848	rVB2	369	255	0.02%	0.003%
48	7.292	1848	1851	1854	rBV2	224	198	0.02%	0.002%
49	7.423	1888	1892	1896	rBV2	232	203	0.02%	0.002%
50	7.568	1924	1937	1951	rBV	135552	241303	19.73%	2.431%
51	7.687	1967	1974	1983	rBV5	2294	3354	0.27%	0.034%
52	7.796	2004	2008	2012	rVB3	451	346	0.03%	0.003%
53	7.899	2026	2040	2056	rBV	548304	950641	77.72%	9.578%
54	8.179	2116	2127	2142	rBV	95637	164579	13.45%	1.658%
55	8.491	2221	2224	2230	rVB2	385	377	0.03%	0.004%
56	8.517	2230	2232	2241	rVB3	352	443	0.04%	0.004%
57	8.632	2256	2268	2303	rBV	390966	740480	60.53%	7.461%
58	8.867	2337	2341	2342	rBV2	258	217	0.02%	0.002%
59	8.886	2345	2347	2353	rVB3	306	218	0.02%	0.002%
60	8.912	2353	2355	2362	rVB2	460	298	0.02%	0.003%
61	9.166	2430	2434	2439	rBV2	371	439	0.04%	0.004%
62	9.234	2451	2455	2458	rBV	306	214	0.02%	0.002%
63	9.250	2458	2460	2466	rVB3	351	245	0.02%	0.002%
64	9.417	2499	2512	2550	rVV	587305	1016053	83.06%	10.237%
65	9.562	2554	2557	2560	rBV3	259	234	0.02%	0.002%
66	9.677	2590	2593	2594	rVV	322	196	0.02%	0.002%
67	9.690	2594	2597	2606	rVV2	977	1232	0.10%	0.012%
68	9.729	2606	2609	2612	rVV3	322	284	0.02%	0.003%
69	10.057	2708	2711	2713	rBV	307	212	0.02%	0.002%
70	10.144	2734	2738	2743	rVB2	268	261	0.02%	0.003%
71	10.282	2779	2781	2787	rVB	342	246	0.02%	0.002%
72	10.401	2812	2818	2819	rBV	255	196	0.02%	0.002%
73	10.558	2863	2867	2871	rBV2	302	320	0.03%	0.003%
74	10.581	2871	2874	2878	rVV2	353	259	0.02%	0.003%
75	10.671	2895	2902	2907	rBV5	973	1077	0.09%	0.011%
76	10.758	2913	2929	2958	rBV	434151	705111	57.64%	7.104%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048033.D
 Acq On : 14 Apr 2022 02:59
 Operator : SY/MD
 Sample : N2387-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.877	2961	2966	2967	rBV2	250	212	0.02%	0.002%
78	11.163	3050	3055	3062	rBV3	268	280	0.02%	0.003%
79	11.365	3113	3118	3120	rBV2	263	228	0.02%	0.002%
80	11.465	3144	3149	3153	rBV3	961	1114	0.09%	0.011%
81	11.507	3159	3162	3165	rVB	247	191	0.02%	0.002%
82	11.578	3181	3184	3188	rVB2	226	201	0.02%	0.002%
83	11.619	3196	3197	3201	rVB2	416	221	0.02%	0.002%
84	11.658	3205	3209	3210	rBV	322	213	0.02%	0.002%
85	11.697	3217	3221	3225	rBV3	697	564	0.05%	0.006%
86	11.742	3231	3235	3242	rBV5	568	669	0.05%	0.007%
87	11.812	3245	3257	3280	rBV	637961	1034386	84.56%	10.422%
88	11.970	3300	3306	3312	rVB5	941	1480	0.12%	0.015%
89	12.070	3334	3337	3339	rBV	378	227	0.02%	0.002%
90	12.086	3339	3342	3345	rVV2	322	253	0.02%	0.003%
91	12.124	3350	3354	3355	rBV2	271	200	0.02%	0.002%
92	12.195	3363	3376	3393	rBV	573556	944923	77.25%	9.521%
93	12.330	3415	3418	3421	rVB2	314	194	0.02%	0.002%
94	12.484	3461	3466	3467	rBV	349	307	0.03%	0.003%
95	12.526	3476	3479	3484	rBV2	406	336	0.03%	0.003%
96	12.581	3493	3496	3498	rBV	283	206	0.02%	0.002%
97	12.597	3499	3501	3504	rVV2	321	203	0.02%	0.002%
98	12.793	3559	3562	3565	rVB2	399	230	0.02%	0.002%
99	13.844	3885	3889	3898	rVB4	1850	2529	0.21%	0.025%
100	13.922	3909	3913	3916	rBV2	361	362	0.03%	0.004%




Sum of corrected areas: 9924947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048033.D
Acq On : 14 Apr 2022 02:59
Operator : SY/MD
Sample : N2387-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

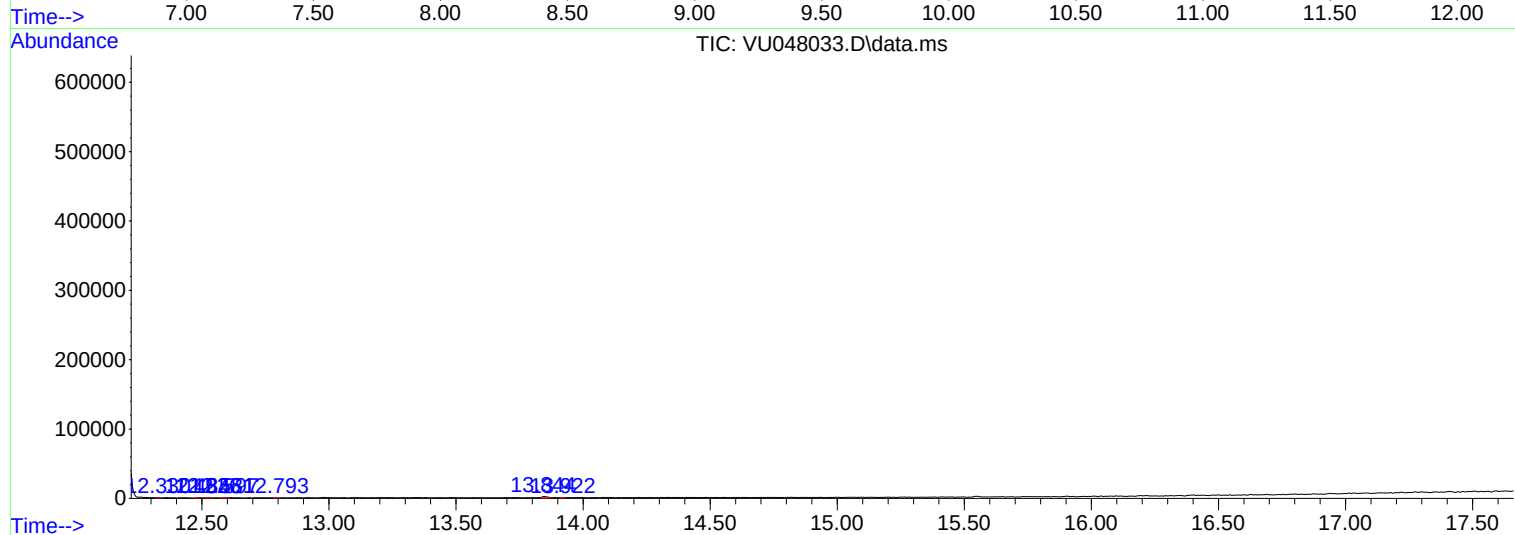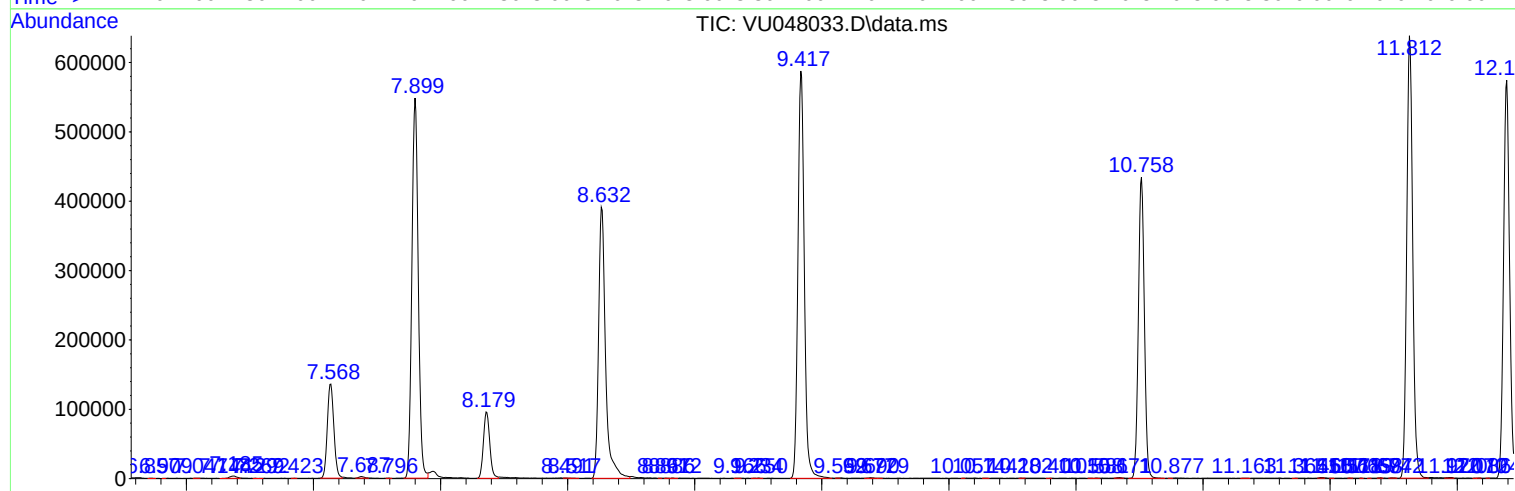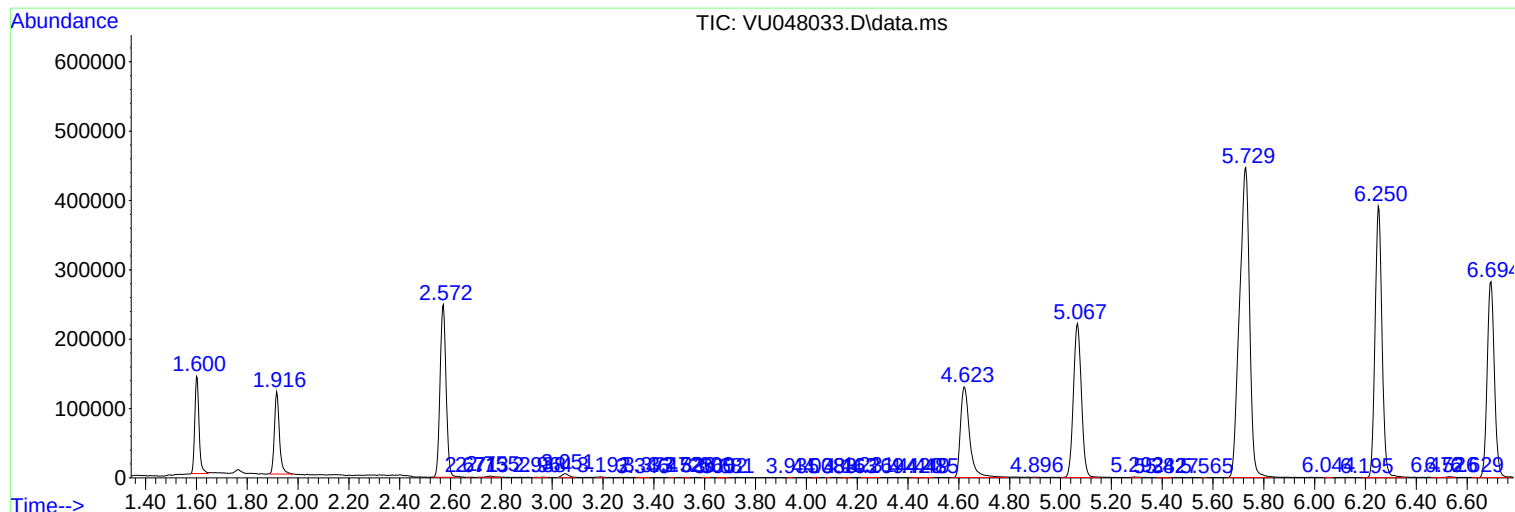

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048033.D
Acq On : 14 Apr 2022 02:59
Operator : SY/MD
Sample : N2387-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048033.D
Acq On : 14 Apr 2022 02:59
Operator : SY/MD
Sample : N2387-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc