

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048034.D
 Acq On : 14 Apr 2022 03:22
 Operator : SY/MD
 Sample : N2387-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rBV	140651	160465	13.29%	1.645%
2	1.916	171	179	201	rVB	118392	164848	13.65%	1.690%
3	2.571	370	383	400	rBV	248178	404048	33.46%	4.142%
4	2.726	428	431	432	rBV	412	174	0.01%	0.002%
5	2.755	434	440	448	rVV3	2062	2781	0.23%	0.029%
6	2.877	474	478	483	rBV3	263	248	0.02%	0.003%
7	2.919	484	491	493	rBV2	280	348	0.03%	0.004%
8	2.941	496	498	500	rBV2	336	165	0.01%	0.002%
9	3.006	515	518	520	rBV2	330	219	0.02%	0.002%
10	3.047	521	531	549	rVB5	6133	12538	1.04%	0.129%
11	3.147	560	562	567	rBV	324	250	0.02%	0.003%
12	3.269	596	600	604	rVB2	402	373	0.03%	0.004%
13	3.353	620	626	628	rBV3	176	190	0.02%	0.002%
14	3.501	670	672	674	rBV	342	190	0.02%	0.002%
15	3.536	678	683	686	rVV2	244	187	0.02%	0.002%
16	3.555	686	689	691	rBV	264	170	0.01%	0.002%
17	3.616	704	708	711	rBV2	264	250	0.02%	0.003%
18	3.681	724	728	730	rBV2	245	209	0.02%	0.002%
19	3.758	748	752	757	rBV	235	182	0.02%	0.002%
20	3.797	761	764	766	rBV2	364	288	0.02%	0.003%
21	3.948	809	811	816	rVV2	322	297	0.02%	0.003%
22	3.977	818	820	827	rVB3	262	277	0.02%	0.003%
23	4.047	839	842	847	rBV2	258	185	0.02%	0.002%
24	4.150	871	874	877	rBV2	209	176	0.01%	0.002%
25	4.231	896	899	903	rBV3	204	188	0.02%	0.002%
26	4.514	982	987	988	rBV2	237	230	0.02%	0.002%
27	4.559	998	1001	1007	rBV2	184	207	0.02%	0.002%
28	4.620	1007	1020	1048	rBV	129413	316279	26.19%	3.242%
29	4.816	1079	1081	1084	rBV	299	229	0.02%	0.002%
30	5.067	1142	1159	1185	rBV	221846	481728	39.89%	4.938%
31	5.295	1220	1230	1232	rBV3	927	1368	0.11%	0.014%
32	5.562	1310	1313	1316	rVB2	269	190	0.02%	0.002%
33	5.587	1316	1321	1323	rBV2	315	303	0.03%	0.003%
34	5.729	1342	1365	1394	rBV2	441188	1207693	100.00%	12.380%
35	6.047	1460	1464	1468	rBV2	490	430	0.04%	0.004%
36	6.115	1481	1485	1489	rBV	346	354	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048034.D
 Acq On : 14 Apr 2022 03:22
 Operator : SY/MD
 Sample : N2387-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1513	1527	1547	rBV	381359	727172	60.21%	7.454%
38	6.452	1585	1590	1592	rBV4	302	273	0.02%	0.003%
39	6.530	1609	1614	1622	rBV3	1178	1747	0.14%	0.018%
40	6.607	1633	1638	1639	rBV	372	269	0.02%	0.003%
41	6.636	1644	1647	1649	rBV	276	181	0.01%	0.002%
42	6.693	1649	1665	1687	rBV	277154	544041	45.05%	5.577%
43	6.803	1695	1699	1701	rBV3	562	460	0.04%	0.005%
44	6.931	1735	1739	1742	rBV2	446	398	0.03%	0.004%
45	6.999	1758	1760	1764	rVB	307	165	0.01%	0.002%
46	7.038	1768	1772	1773	rBV2	371	296	0.02%	0.003%
47	7.179	1808	1816	1828	rVV5	3568	5922	0.49%	0.061%
48	7.250	1835	1838	1844	rVB2	308	246	0.02%	0.003%
49	7.494	1911	1914	1920	rBV2	155	188	0.02%	0.002%
50	7.568	1924	1937	1958	rBV	133830	237623	19.68%	2.436%
51	7.687	1968	1974	1985	rVB5	2392	4026	0.33%	0.041%
52	7.764	1993	1998	1999	rBV	479	315	0.03%	0.003%
53	7.793	2003	2007	2011	rVB3	459	360	0.03%	0.004%
54	7.825	2014	2017	2020	rVB	307	177	0.01%	0.002%
55	7.899	2026	2040	2055	rBV	544416	936214	77.52%	9.597%
56	8.179	2116	2127	2145	rBV	95005	162502	13.46%	1.666%
57	8.439	2205	2208	2210	rBV2	252	177	0.01%	0.002%
58	8.494	2223	2225	2230	rVB3	279	219	0.02%	0.002%
59	8.533	2233	2237	2241	rBV2	335	336	0.03%	0.003%
60	8.632	2256	2268	2300	rBV	382660	730800	60.51%	7.492%
61	8.848	2331	2335	2339	rVV3	334	327	0.03%	0.003%
62	8.925	2356	2359	2361	rBV	255	200	0.02%	0.002%
63	8.973	2369	2374	2377	rBV2	318	314	0.03%	0.003%
64	9.105	2413	2415	2418	rBV2	213	167	0.01%	0.002%
65	9.160	2429	2432	2435	rBV2	288	220	0.02%	0.002%
66	9.214	2446	2449	2453	rVB2	303	186	0.02%	0.002%
67	9.279	2465	2469	2470	rBV2	364	212	0.02%	0.002%
68	9.417	2499	2512	2550	rBV	580916	993105	82.23%	10.181%
69	9.687	2591	2596	2597	rBV2	533	396	0.03%	0.004%
70	9.941	2673	2675	2681	rVB2	256	193	0.02%	0.002%
71	10.234	2763	2766	2770	rBV2	306	219	0.02%	0.002%
72	10.353	2800	2803	2808	rVV2	371	270	0.02%	0.003%
73	10.404	2815	2819	2826	rVB3	295	330	0.03%	0.003%
74	10.497	2842	2848	2852	rBV3	217	213	0.02%	0.002%
75	10.671	2893	2902	2909	rBV4	1480	2026	0.17%	0.021%
76	10.758	2915	2929	2950	rVB	426240	690562	57.18%	7.079%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048034.D
 Acq On : 14 Apr 2022 03:22
 Operator : SY/MD
 Sample : N2387-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.848	2952	2957	2959	rBV3	311	271	0.02%	0.003%
78	10.867	2959	2963	2964	rBV	327	203	0.02%	0.002%
79	10.899	2970	2973	2979	rVB3	637	608	0.05%	0.006%
80	11.012	3002	3008	3010	rBV3	642	568	0.05%	0.006%
81	11.111	3035	3039	3043	rBV2	330	363	0.03%	0.004%
82	11.134	3043	3046	3049	rVV	246	182	0.02%	0.002%
83	11.288	3090	3094	3097	rVB2	331	250	0.02%	0.003%
84	11.311	3097	3101	3108	rBV	332	299	0.02%	0.003%
85	11.391	3122	3126	3127	rBV2	272	168	0.01%	0.002%
86	11.459	3144	3147	3157	rVB4	916	1174	0.10%	0.012%
87	11.642	3200	3204	3207	rBV2	288	254	0.02%	0.003%
88	11.745	3231	3236	3238	rVV3	446	405	0.03%	0.004%
89	11.812	3241	3257	3283	rBV	622213	1012995	83.88%	10.385%
90	12.137	3354	3358	3362	rBV2	356	384	0.03%	0.004%
91	12.195	3362	3376	3397	rBV	563195	931812	77.16%	9.552%
92	12.462	3455	3459	3460	rBV	241	199	0.02%	0.002%
93	12.668	3520	3523	3526	rBV	387	257	0.02%	0.003%
94	12.754	3544	3550	3551	rBV2	356	345	0.03%	0.004%
95	12.767	3552	3554	3556	rBV2	361	206	0.02%	0.002%
96	13.484	3771	3777	3780	rBV3	336	396	0.03%	0.004%
97	13.558	3792	3800	3806	rBV3	450	796	0.07%	0.008%
98	14.655	4138	4141	4143	rBV2	356	218	0.02%	0.002%
99	15.442	4383	4386	4388	rBV2	837	547	0.05%	0.006%
100	15.523	4408	4411	4413	rBV3	904	647	0.05%	0.007%




Sum of corrected areas: 9754851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048034.D
Acq On : 14 Apr 2022 03:22
Operator : SY/MD
Sample : N2387-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

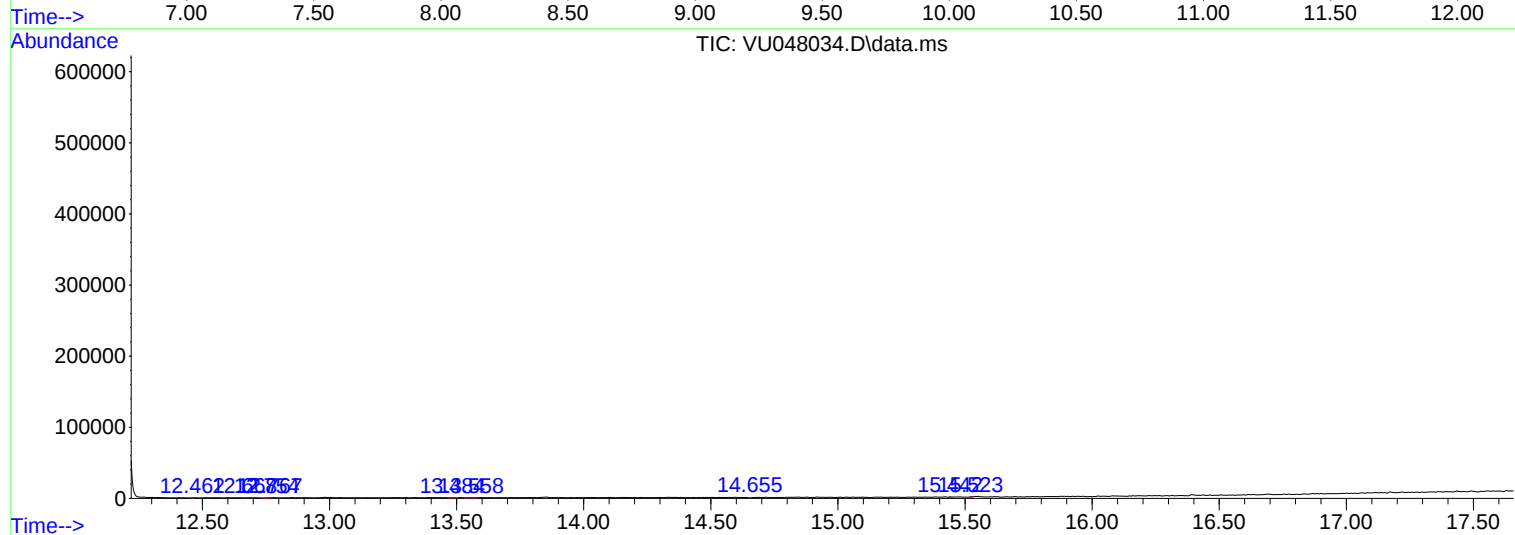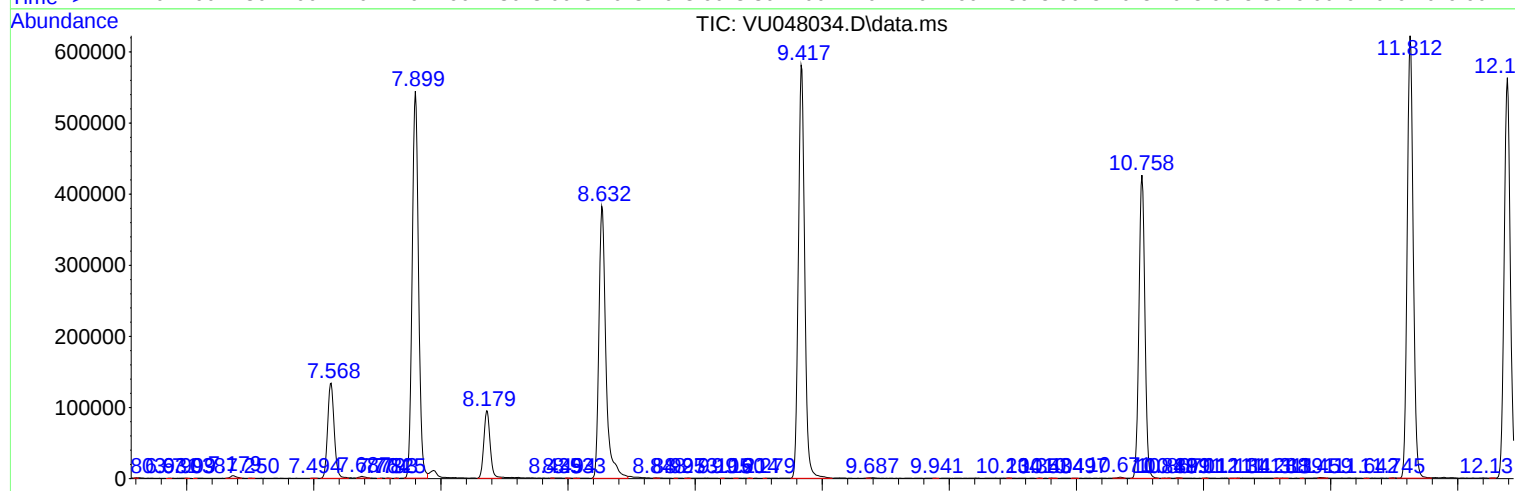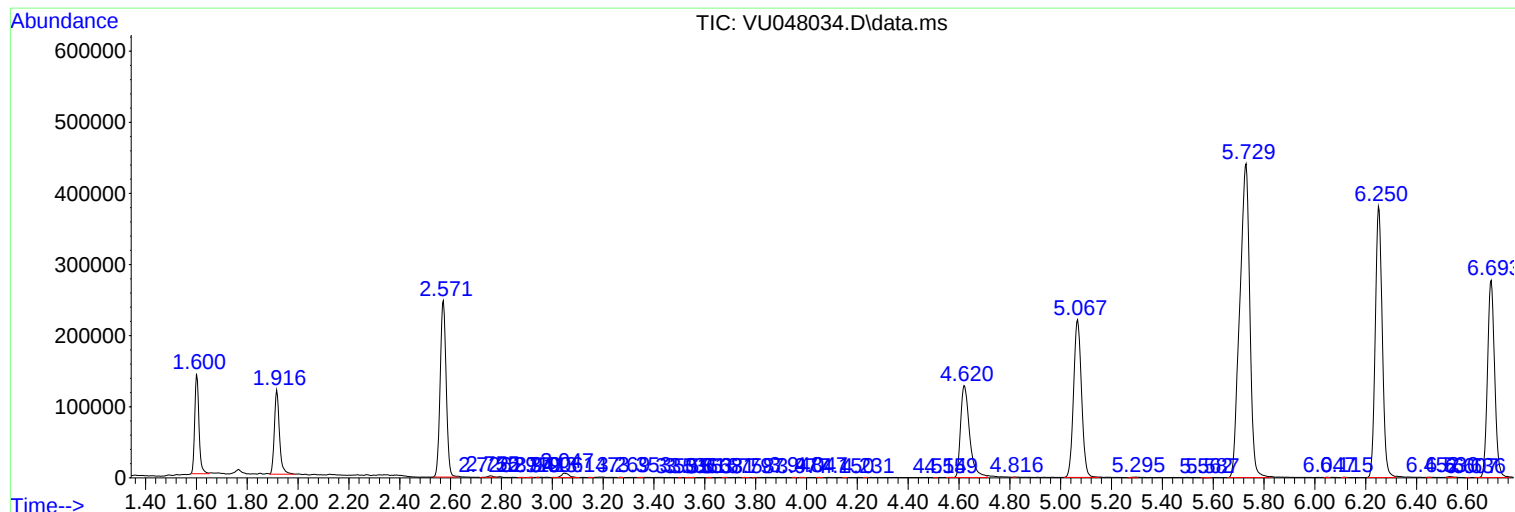

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048034.D
Acq On : 14 Apr 2022 03:22
Operator : SY/MD
Sample : N2387-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048034.D
Acq On : 14 Apr 2022 03:22
Operator : SY/MD
Sample : N2387-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc