

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048035.D
 Acq On : 14 Apr 2022 03:45
 Operator : SY/MD
 Sample : N2387-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rBV	137654	158754	13.23%	1.650%
2	1.916	171	179	205	rVB	115754	163906	13.66%	1.703%
3	2.514	360	365	366	rBV	409	377	0.03%	0.004%
4	2.572	370	383	403	rVV	241077	395393	32.95%	4.109%
5	2.867	472	475	478	rBV3	286	261	0.02%	0.003%
6	2.954	497	502	504	rBV4	346	296	0.02%	0.003%
7	3.047	523	531	547	rVB3	6615	12347	1.03%	0.128%
8	3.183	564	573	574	rBV2	694	668	0.06%	0.007%
9	3.318	610	615	617	rBV	298	280	0.02%	0.003%
10	3.363	625	629	633	rBV2	464	470	0.04%	0.005%
11	3.388	633	637	640	rVB2	219	177	0.01%	0.002%
12	3.414	640	645	646	rBV2	239	220	0.02%	0.002%
13	3.459	656	659	662	rBV3	281	216	0.02%	0.002%
14	3.543	681	685	687	rBV	277	196	0.02%	0.002%
15	3.591	696	700	704	rBV	264	198	0.02%	0.002%
16	3.636	710	714	719	rVB3	196	188	0.02%	0.002%
17	3.842	775	778	781	rBV2	295	199	0.02%	0.002%
18	3.999	820	827	832	rBV3	421	513	0.04%	0.005%
19	4.022	832	834	839	rVV2	248	199	0.02%	0.002%
20	4.054	841	844	848	rVB2	281	210	0.02%	0.002%
21	4.096	850	857	859	rBV	260	230	0.02%	0.002%
22	4.141	867	871	875	rBV2	162	176	0.01%	0.002%
23	4.186	878	885	887	rBV2	213	221	0.02%	0.002%
24	4.202	887	890	894	rBV3	308	221	0.02%	0.002%
25	4.427	957	960	961	rBV	313	205	0.02%	0.002%
26	4.620	1008	1020	1050	rBV	129992	313301	26.11%	3.256%
27	4.964	1123	1127	1129	rBV2	286	247	0.02%	0.003%
28	5.006	1136	1140	1142	rBV2	257	184	0.02%	0.002%
29	5.067	1142	1159	1188	rVV	216442	476265	39.69%	4.949%
30	5.292	1223	1229	1230	rBV	460	424	0.04%	0.004%
31	5.523	1298	1301	1305	rVB2	309	259	0.02%	0.003%
32	5.617	1326	1330	1333	rBV2	239	195	0.02%	0.002%
33	5.726	1342	1364	1397	rBV2	439403	1200057	100.00%	12.470%
34	5.919	1421	1424	1428	rBV2	269	191	0.02%	0.002%
35	6.038	1457	1461	1464	rBV3	470	448	0.04%	0.005%
36	6.118	1482	1486	1492	rVB3	591	616	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048035.D
 Acq On : 14 Apr 2022 03:45
 Operator : SY/MD
 Sample : N2387-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1549	rBV	372937	710447	59.20%	7.382%
38	6.530	1609	1614	1625	rVB5	1398	1897	0.16%	0.020%
39	6.597	1630	1635	1637	rBV2	304	244	0.02%	0.003%
40	6.694	1649	1665	1690	rBV	275405	541998	45.16%	5.632%
41	6.803	1694	1699	1708	rVB5	1018	1697	0.14%	0.018%
42	6.842	1709	1711	1715	rVB	413	199	0.02%	0.002%
43	6.870	1715	1720	1722	rBV	271	223	0.02%	0.002%
44	6.996	1753	1759	1762	rVB2	195	217	0.02%	0.002%
45	7.047	1773	1775	1781	rVB2	423	302	0.03%	0.003%
46	7.179	1809	1816	1831	rVB5	3284	6361	0.53%	0.066%
47	7.353	1867	1870	1873	rBV3	340	246	0.02%	0.003%
48	7.401	1884	1885	1893	rBV2	255	312	0.03%	0.003%
49	7.494	1910	1914	1916	rBV3	396	310	0.03%	0.003%
50	7.568	1923	1937	1958	rBV	131957	234402	19.53%	2.436%
51	7.687	1966	1974	1976	rBV4	1804	2203	0.18%	0.023%
52	7.751	1991	1994	2000	rVB2	453	276	0.02%	0.003%
53	7.899	2025	2040	2056	rBV	542036	924528	77.04%	9.607%
54	8.070	2091	2093	2096	rBV2	340	228	0.02%	0.002%
55	8.179	2111	2127	2144	rBV	94049	162065	13.50%	1.684%
56	8.359	2180	2183	2188	rVB2	354	251	0.02%	0.003%
57	8.420	2199	2202	2204	rBV2	290	210	0.02%	0.002%
58	8.468	2215	2217	2219	rVB	417	178	0.01%	0.002%
59	8.632	2256	2268	2299	rBV	379034	723887	60.32%	7.522%
60	8.986	2373	2378	2385	rVB2	404	549	0.05%	0.006%
61	9.160	2430	2432	2436	rVV2	561	394	0.03%	0.004%
62	9.301	2469	2476	2479	rBV2	335	389	0.03%	0.004%
63	9.417	2499	2512	2552	rVB	569798	969662	80.80%	10.076%
64	9.568	2556	2559	2563	rBV2	562	470	0.04%	0.005%
65	9.610	2568	2572	2573	rBV	311	181	0.02%	0.002%
66	9.690	2595	2597	2605	rVB3	1184	1379	0.11%	0.014%
67	9.735	2605	2611	2615	rBV	437	480	0.04%	0.005%
68	9.851	2642	2647	2651	rVB2	241	260	0.02%	0.003%
69	9.906	2659	2664	2670	rVB3	303	306	0.03%	0.003%
70	9.960	2679	2681	2686	rVB3	259	187	0.02%	0.002%
71	10.282	2778	2781	2783	rBV2	401	239	0.02%	0.002%
72	10.298	2783	2786	2790	rVB2	365	252	0.02%	0.003%
73	10.375	2806	2810	2813	rBV2	360	398	0.03%	0.004%
74	10.481	2839	2843	2847	rVB2	394	359	0.03%	0.004%
75	10.671	2895	2902	2912	rVB5	1159	1706	0.14%	0.018%
76	10.758	2916	2929	2952	rVB	427778	690037	57.50%	7.170%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048035.D
 Acq On : 14 Apr 2022 03:45
 Operator : SY/MD
 Sample : N2387-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.883	2965	2968	2970	rBV	447	274	0.02%	0.003%
78	10.970	2991	2995	2999	rBV3	262	234	0.02%	0.002%
79	10.996	2999	3003	3005	rVB2	474	312	0.03%	0.003%
80	11.015	3005	3009	3011	rBV2	305	218	0.02%	0.002%
81	11.128	3040	3044	3047	rBV	400	383	0.03%	0.004%
82	11.420	3131	3135	3137	rVB2	352	257	0.02%	0.003%
83	11.462	3141	3148	3159	rVB5	1603	2735	0.23%	0.028%
84	11.510	3159	3163	3165	rBV2	300	228	0.02%	0.002%
85	11.632	3198	3201	3207	rBV2	205	226	0.02%	0.002%
86	11.674	3209	3214	3216	rBV2	183	191	0.02%	0.002%
87	11.690	3216	3219	3221	rBV2	497	262	0.02%	0.003%
88	11.812	3243	3257	3279	rBV	618337	984516	82.04%	10.230%
89	11.922	3288	3291	3294	rBV5	458	405	0.03%	0.004%
90	12.028	3321	3324	3326	rBV2	458	307	0.03%	0.003%
91	12.121	3350	3353	3356	rVB	305	185	0.02%	0.002%
92	12.195	3358	3376	3397	rBV	558094	921676	76.80%	9.577%
93	12.449	3453	3455	3458	rVB2	349	197	0.02%	0.002%
94	12.472	3458	3462	3465	rBV	369	359	0.03%	0.004%
95	12.568	3486	3492	3496	rBV3	264	352	0.03%	0.004%
96	12.883	3587	3590	3600	rVB4	304	429	0.04%	0.004%
97	12.976	3615	3619	3621	rBV4	586	367	0.03%	0.004%
98	13.070	3643	3648	3650	rBV3	402	375	0.03%	0.004%
99	13.163	3671	3677	3680	rBV2	403	481	0.04%	0.005%
100	14.886	4210	4213	4217	rBV	479	416	0.03%	0.004%


Sum of corrected areas: 9623622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048035.D
Acq On : 14 Apr 2022 03:45
Operator : SY/MD
Sample : N2387-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

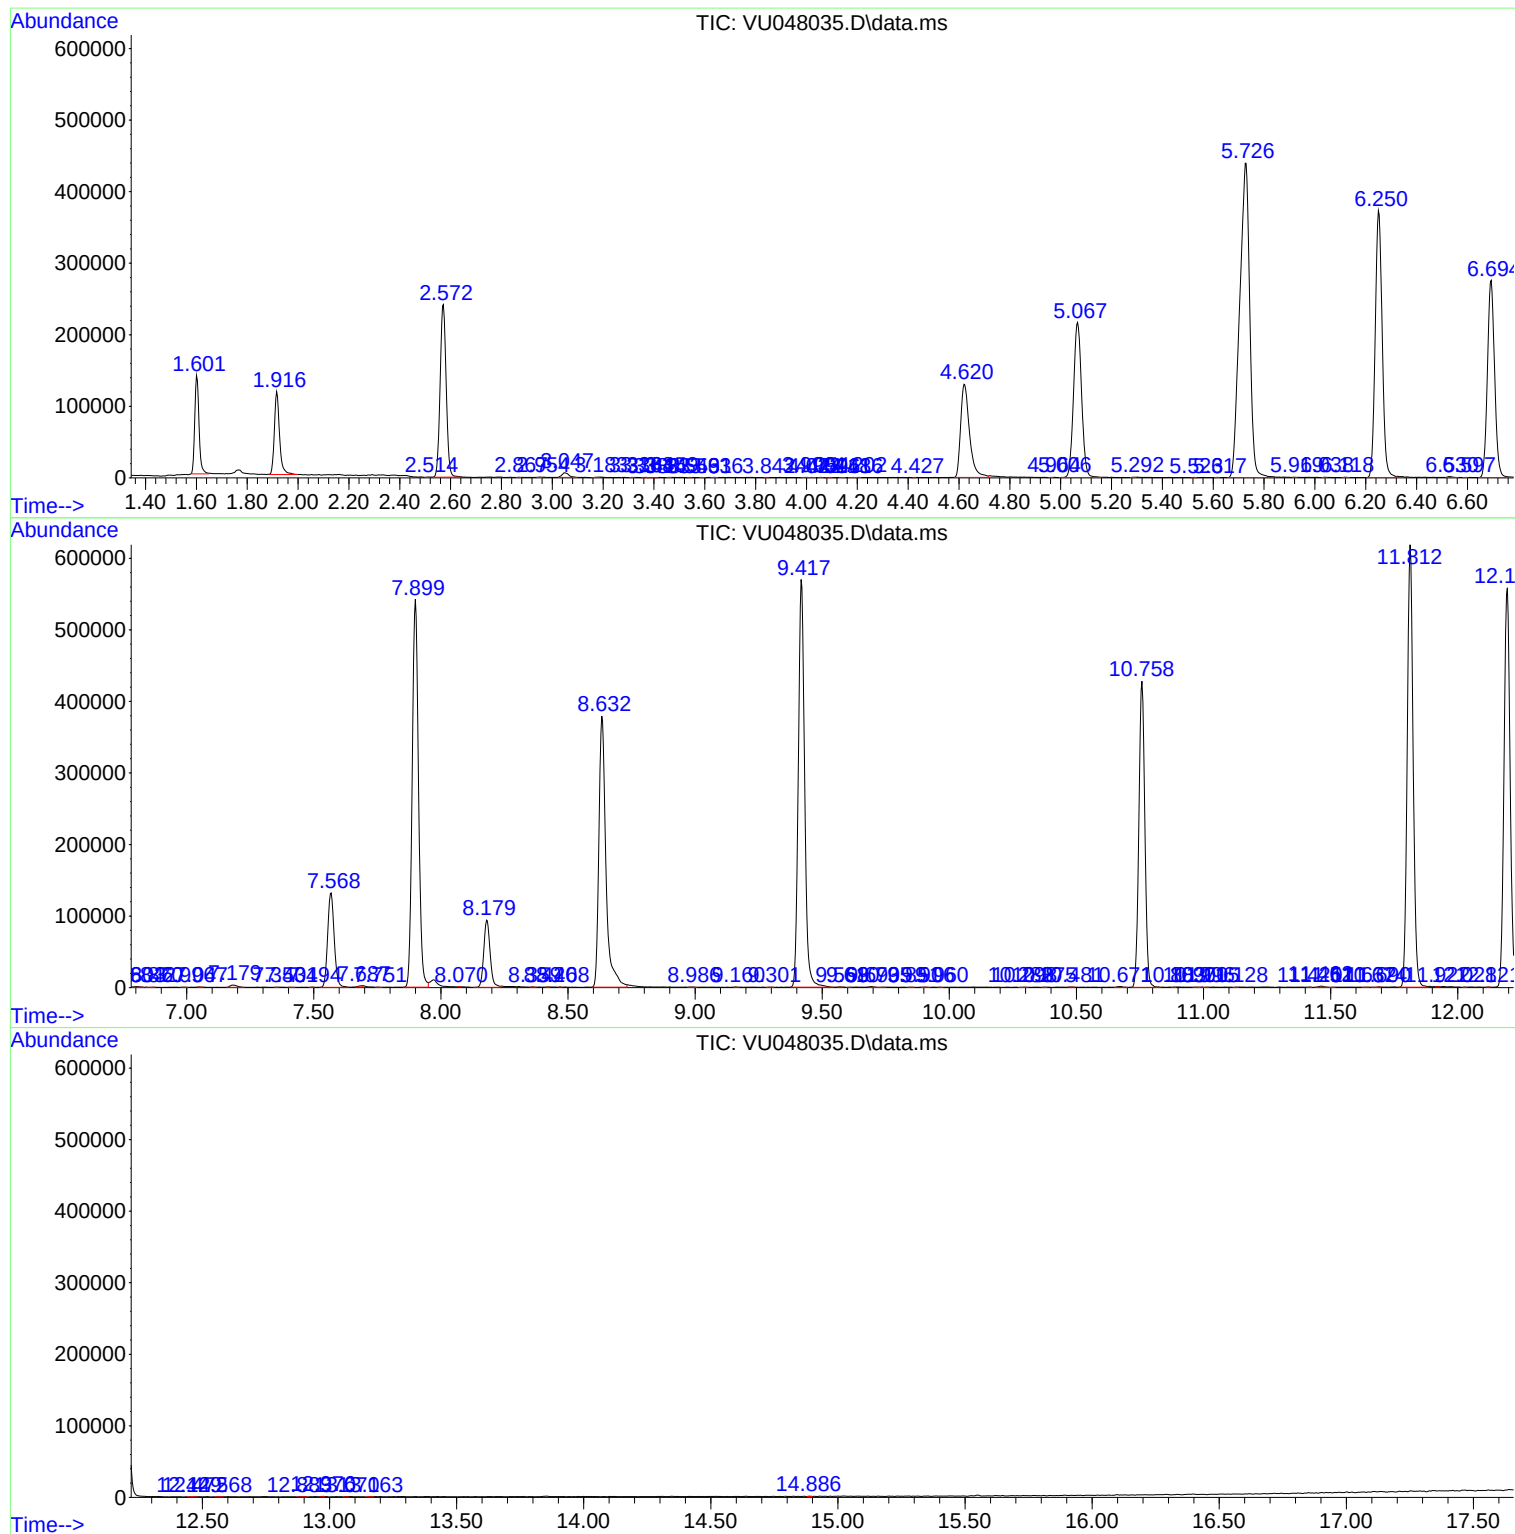

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048035.D
Acq On : 14 Apr 2022 03:45
Operator : SY/MD
Sample : N2387-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048035.D
Acq On : 14 Apr 2022 03:45
Operator : SY/MD
Sample : N2387-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc