

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048037.D
 Acq On : 14 Apr 2022 04:31
 Operator : SY/MD
 Sample : N2386-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rBV	139923	160900	0.79%	0.356%
2	1.916	171	179	199	rVB	116196	161968	0.79%	0.358%
3	2.572	370	383	411	rBV	242270	399416	1.95%	0.884%
4	2.755	432	440	449	rBV3	3113	5669	0.03%	0.013%
5	2.877	475	478	482	rVB2	278	208	0.00%	0.000%
6	2.912	486	489	494	rVB3	454	391	0.00%	0.001%
7	2.951	498	501	504	rBV3	333	265	0.00%	0.001%
8	3.051	519	532	544	rVB2	4940	9229	0.05%	0.020%
9	3.134	555	558	560	rVB	322	211	0.00%	0.000%
10	3.157	560	565	567	rBV3	422	421	0.00%	0.001%
11	3.182	567	573	576	rBV3	790	945	0.00%	0.002%
12	3.330	616	619	624	rVB2	435	408	0.00%	0.001%
13	3.356	624	627	629	rBV2	315	208	0.00%	0.000%
14	3.379	629	634	637	rBV2	277	310	0.00%	0.001%
15	3.565	687	692	694	rBV2	412	379	0.00%	0.001%
16	3.581	695	697	701	rVB	471	253	0.00%	0.001%
17	3.610	701	706	708	rBV2	404	361	0.00%	0.001%
18	3.665	718	723	730	rBV3	374	530	0.00%	0.001%
19	3.713	732	738	741	rBV2	231	226	0.00%	0.000%
20	3.771	752	756	761	rVB	350	294	0.00%	0.001%
21	3.800	761	765	767	rBV	326	213	0.00%	0.000%
22	3.887	788	792	797	rVB2	465	481	0.00%	0.001%
23	3.919	797	802	806	rBV2	371	384	0.00%	0.001%
24	4.006	826	829	832	rVB	251	192	0.00%	0.000%
25	4.260	904	908	913	rVB2	250	193	0.00%	0.000%
26	4.385	941	947	950	rVB2	355	333	0.00%	0.001%
27	4.407	950	954	956	rBV	218	191	0.00%	0.000%
28	4.536	990	994	997	rBV3	430	360	0.00%	0.001%
29	4.620	1008	1020	1054	rBV	129376	314775	1.54%	0.696%
30	5.067	1142	1159	1184	rBV	218478	477989	2.33%	1.057%
31	5.231	1207	1210	1212	rBV3	343	252	0.00%	0.001%
32	5.263	1218	1220	1223	rBV2	347	192	0.00%	0.000%
33	5.292	1226	1229	1239	rVB2	570	748	0.00%	0.002%
34	5.388	1253	1259	1261	rBV	387	402	0.00%	0.001%
35	5.497	1286	1293	1296	rBV2	240	280	0.00%	0.001%
36	5.729	1342	1365	1395	rBV2	439557	1214399	5.93%	2.687%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048037.D
 Acq On : 14 Apr 2022 04:31
 Operator : SY/MD
 Sample : N2386-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.050	1462	1465	1469	rVB2	328	196	0.00%	0.000%
38	6.163	1498	1500	1505	rVB3	392	290	0.00%	0.001%
39	6.250	1511	1527	1554	rBV	386752	734249	3.58%	1.624%
40	6.536	1605	1616	1623	rVB6	1329	2425	0.01%	0.005%
41	6.607	1635	1638	1640	rVB	349	214	0.00%	0.000%
42	6.694	1651	1665	1686	rBV	274153	539087	2.63%	1.193%
43	6.970	1749	1751	1760	rVB2	342	355	0.00%	0.001%
44	7.015	1760	1765	1768	rBV2	176	212	0.00%	0.000%
45	7.038	1768	1772	1775	rBV2	374	376	0.00%	0.001%
46	7.185	1808	1818	1831	rVB3	3316	6319	0.03%	0.014%
47	7.308	1850	1856	1860	rBV2	299	284	0.00%	0.001%
48	7.568	1924	1937	1952	rBV	131361	233031	1.14%	0.516%
49	7.642	1957	1960	1965	rVV4	750	705	0.00%	0.002%
50	7.687	1968	1974	1986	rVB6	2380	4291	0.02%	0.009%
51	7.767	1995	1999	2001	rBV	232	201	0.00%	0.000%
52	7.899	2025	2040	2056	rBV	545897	942497	4.60%	2.085%
53	8.179	2116	2127	2143	rBV	95506	160604	0.78%	0.355%
54	8.292	2160	2162	2165	rBV2	552	354	0.00%	0.001%
55	8.526	2232	2235	2238	rBV	375	191	0.00%	0.000%
56	8.632	2256	2268	2300	rBV	385568	725189	3.54%	1.604%
57	8.915	2352	2356	2358	rBV3	429	331	0.00%	0.001%
58	9.121	2416	2420	2422	rBV	249	206	0.00%	0.000%
59	9.166	2432	2434	2442	rVB2	401	322	0.00%	0.001%
60	9.218	2447	2450	2454	rBV2	269	221	0.00%	0.000%
61	9.292	2469	2473	2476	rBV2	340	277	0.00%	0.001%
62	9.314	2476	2480	2484	rBV3	326	278	0.00%	0.001%
63	9.359	2488	2494	2497	rBV3	298	245	0.00%	0.001%
64	9.449	2497	2522	2567	rBV	12031371	20494138	100.00%	45.340%
65	9.690	2594	2597	2598	rBV3	883	508	0.00%	0.001%
66	9.738	2609	2612	2616	rBV4	390	273	0.00%	0.001%
67	9.902	2660	2663	2666	rVB2	308	201	0.00%	0.000%
68	9.944	2673	2676	2678	rBV2	327	246	0.00%	0.001%
69	10.041	2703	2706	2708	rBV2	268	198	0.00%	0.000%
70	10.099	2719	2724	2726	rBV3	368	328	0.00%	0.001%
71	10.153	2738	2741	2745	rBV	292	264	0.00%	0.001%
72	10.182	2748	2750	2755	rVB3	204	202	0.00%	0.000%
73	10.227	2761	2764	2767	rBV2	307	229	0.00%	0.001%
74	10.674	2896	2903	2911	rVB3	1248	1714	0.01%	0.004%
75	10.758	2911	2929	2949	rBV	425398	691619	3.37%	1.530%
76	10.835	2951	2953	2960	rVB2	296	241	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048037.D
 Acq On : 14 Apr 2022 04:31
 Operator : SY/MD
 Sample : N2386-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.896	2968	2972	2975	rBV2	338	224	0.00%	0.000%
78	10.989	2996	3001	3003	rBV3	447	341	0.00%	0.001%
79	11.089	3026	3032	3035	rBV4	533	620	0.00%	0.001%
80	11.185	3059	3062	3066	rBV2	305	246	0.00%	0.001%
81	11.230	3068	3076	3080	rVV3	389	487	0.00%	0.001%
82	11.462	3141	3148	3151	rBV4	1064	1211	0.01%	0.003%
83	11.697	3216	3221	3225	rBV4	783	698	0.00%	0.002%
84	11.745	3225	3236	3246	rVV	271563	431460	2.11%	0.955%
85	11.835	3246	3264	3288	rVB2	1317307	3068449	14.97%	6.788%
86	12.021	3317	3322	3326	rBV3	515	622	0.00%	0.001%
87	12.111	3347	3350	3353	rBV2	291	255	0.00%	0.001%
88	12.214	3362	3382	3420	rBV2	7312385	12338991	60.21%	27.298%
89	12.751	3545	3549	3551	rBV3	333	267	0.00%	0.001%
90	12.973	3609	3618	3627	rBV2	11230	17111	0.08%	0.038%
91	13.028	3633	3635	3637	rBV2	316	204	0.00%	0.000%
92	13.153	3671	3674	3683	rVB2	932	1098	0.01%	0.002%
93	13.333	3722	3730	3739	rVB5	5112	7764	0.04%	0.017%
94	13.841	3874	3888	3910	rBV	1082217	1705547	8.32%	3.773%
95	14.089	3959	3965	3976	rBV3	1549	2442	0.01%	0.005%
96	14.330	4028	4040	4058	rBV	173822	280567	1.37%	0.621%
97	14.713	4156	4159	4162	rBV2	499	370	0.00%	0.001%
98	15.417	4369	4378	4384	rBV6	3891	6491	0.03%	0.014%
99	15.548	4414	4419	4424	rBV5	1345	1383	0.01%	0.003%
100	15.999	4551	4559	4573	rVB2	23329	36850	0.18%	0.082%




Sum of corrected areas: 45200785

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048037.D
Acq On : 14 Apr 2022 04:31
Operator : SY/MD
Sample : N2386-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

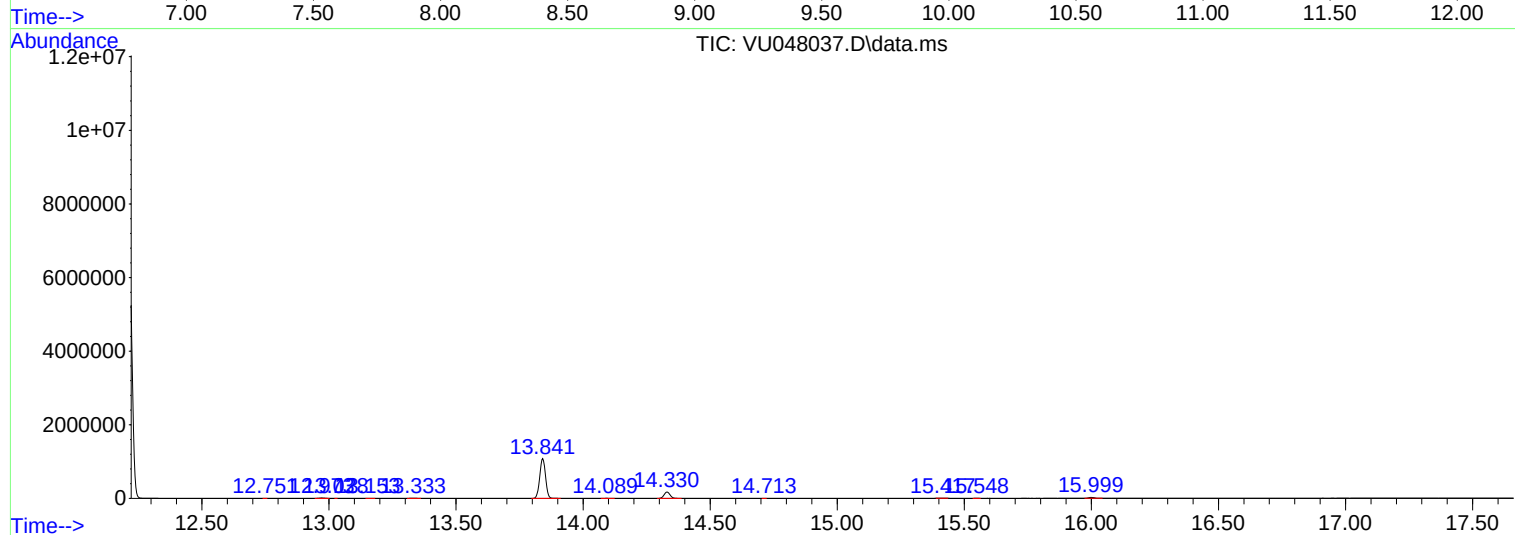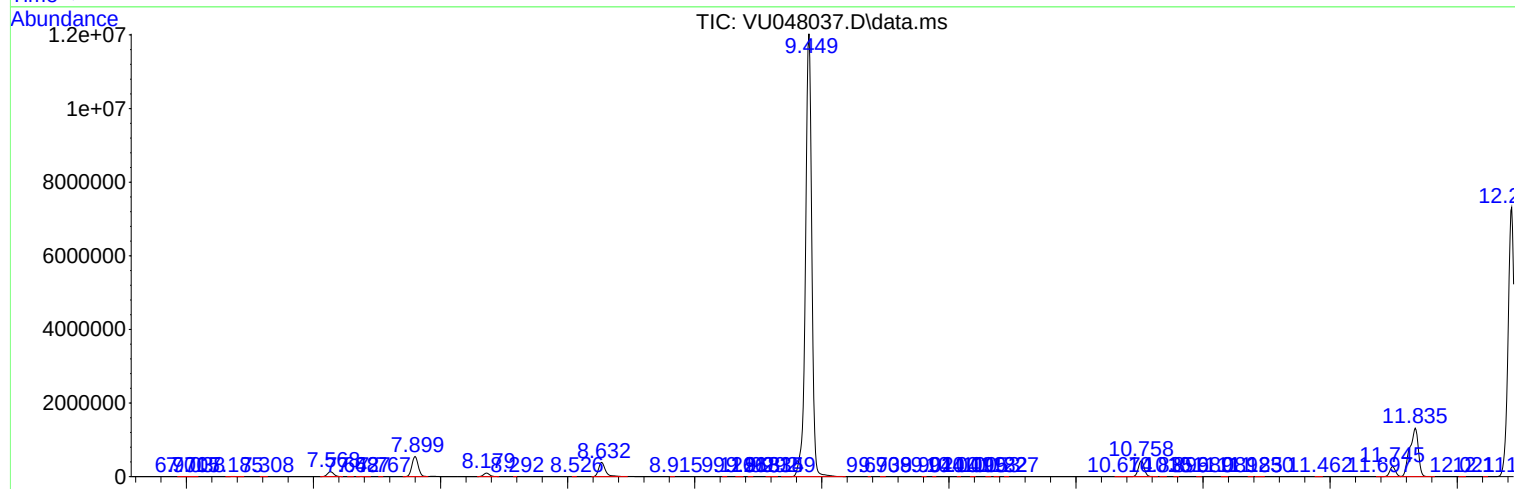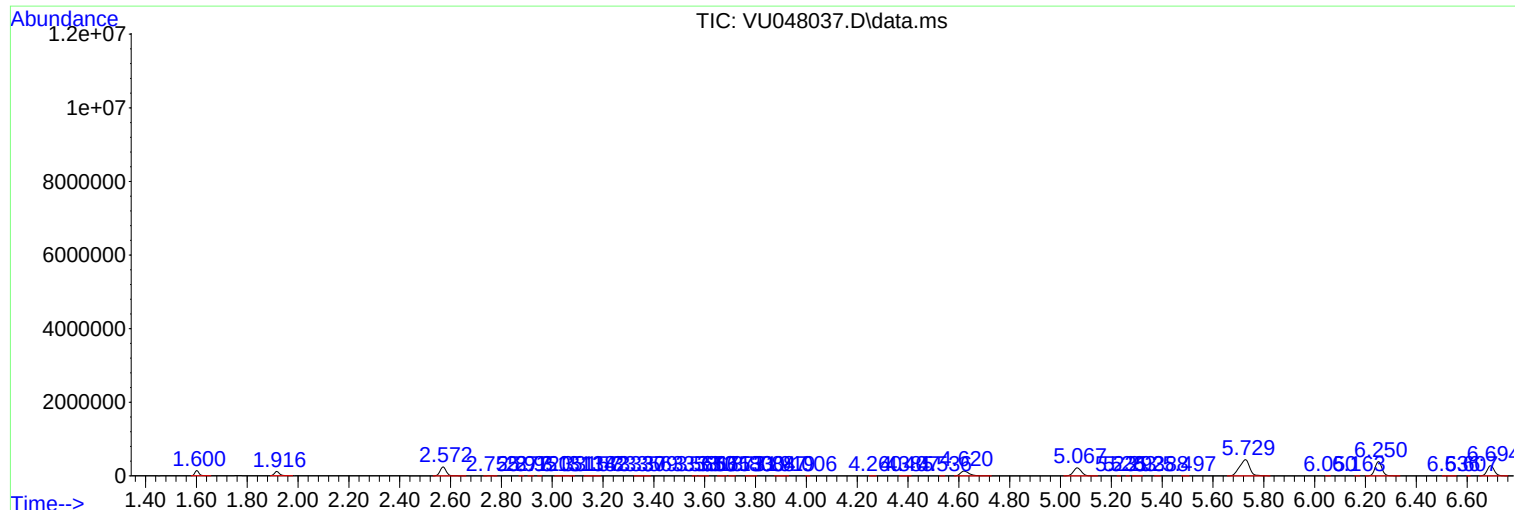

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048037.D
Acq On : 14 Apr 2022 04:31
Operator : SY/MD
Sample : N2386-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048037.D
Acq On : 14 Apr 2022 04:31
Operator : SY/MD
Sample : N2386-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------