

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048038.D
 Acq On : 14 Apr 2022 04:54
 Operator : SY/MD
 Sample : N2386-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rBV	140235	161958	13.40%	1.607%
2	1.915	170	179	203	rVB	116966	164919	13.65%	1.637%
3	2.571	370	383	398	rBV	244398	399346	33.04%	3.963%
4	2.822	458	461	463	rBV	299	217	0.02%	0.002%
5	2.874	475	477	482	rVB2	377	312	0.03%	0.003%
6	2.903	482	486	491	rBV4	482	541	0.04%	0.005%
7	3.009	516	519	523	rBV3	340	261	0.02%	0.003%
8	3.050	523	532	540	rBV5	4762	8414	0.70%	0.083%
9	3.105	545	549	552	rVB3	311	254	0.02%	0.003%
10	3.150	559	563	565	rBV2	196	171	0.01%	0.002%
11	3.182	569	573	576	rBV4	603	492	0.04%	0.005%
12	3.301	607	610	614	rVV2	285	305	0.03%	0.003%
13	3.356	624	627	630	rBV2	335	238	0.02%	0.002%
14	3.452	653	657	660	rBV2	306	242	0.02%	0.002%
15	3.472	660	663	666	rBV2	375	246	0.02%	0.002%
16	3.536	679	683	688	rVB2	440	356	0.03%	0.004%
17	3.681	726	728	734	rVB2	298	210	0.02%	0.002%
18	3.870	784	787	793	rVB2	268	261	0.02%	0.003%
19	4.420	954	958	962	rBV3	405	375	0.03%	0.004%
20	4.542	992	996	997	rBV3	391	208	0.02%	0.002%
21	4.620	1007	1020	1049	rBV	132101	319205	26.41%	3.168%
22	4.951	1119	1123	1126	rBV2	194	175	0.01%	0.002%
23	5.066	1141	1159	1183	rVV	218939	479774	39.70%	4.761%
24	5.189	1194	1197	1199	rVB2	309	177	0.01%	0.002%
25	5.218	1204	1206	1210	rVB3	275	191	0.02%	0.002%
26	5.253	1214	1217	1220	rVB3	427	266	0.02%	0.003%
27	5.295	1223	1230	1240	rVB2	803	1345	0.11%	0.013%
28	5.343	1240	1245	1249	rBV3	302	352	0.03%	0.003%
29	5.365	1249	1252	1256	rBV2	241	195	0.02%	0.002%
30	5.472	1283	1285	1290	rVB2	265	214	0.02%	0.002%
31	5.513	1290	1298	1300	rBV2	196	269	0.02%	0.003%
32	5.552	1305	1310	1313	rBV2	175	172	0.01%	0.002%
33	5.729	1342	1365	1400	rBV2	441035	1208588	100.00%	11.994%
34	5.909	1419	1421	1430	rVB4	386	262	0.02%	0.003%
35	5.976	1440	1442	1446	rBV2	303	187	0.02%	0.002%
36	6.044	1460	1463	1468	rBV3	359	377	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048038.D
 Acq On : 14 Apr 2022 04:54
 Operator : SY/MD
 Sample : N2386-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1513	1527	1556	rBV	382865	731237	60.50%	7.257%
38	6.446	1584	1588	1591	rBV2	209	198	0.02%	0.002%
39	6.526	1607	1613	1614	rBV2	934	814	0.07%	0.008%
40	6.693	1651	1665	1686	rBV	276499	544788	45.08%	5.406%
41	6.812	1697	1702	1711	rVB6	1251	1635	0.14%	0.016%
42	6.915	1729	1734	1735	rBV2	243	217	0.02%	0.002%
43	6.928	1735	1738	1742	rVB2	330	266	0.02%	0.003%
44	6.951	1743	1745	1750	rVB3	307	209	0.02%	0.002%
45	6.989	1750	1757	1759	rBV	294	268	0.02%	0.003%
46	7.057	1776	1778	1782	rVV2	514	311	0.03%	0.003%
47	7.189	1806	1819	1826	rBV3	3778	6274	0.52%	0.062%
48	7.353	1868	1870	1877	rVB2	211	241	0.02%	0.002%
49	7.484	1904	1911	1912	rBV	248	257	0.02%	0.003%
50	7.568	1924	1937	1952	rBV	132424	235958	19.52%	2.342%
51	7.690	1969	1975	1987	rVB3	2419	3925	0.32%	0.039%
52	7.838	2016	2021	2023	rBV2	340	229	0.02%	0.002%
53	7.899	2026	2040	2056	rBV	543543	943937	78.10%	9.367%
54	8.111	2104	2106	2111	rVB	425	181	0.01%	0.002%
55	8.179	2115	2127	2142	rBV	94514	161099	13.33%	1.599%
56	8.436	2202	2207	2210	rVB3	416	393	0.03%	0.004%
57	8.462	2210	2215	2217	rBV4	365	333	0.03%	0.003%
58	8.478	2217	2220	2222	rBV2	305	203	0.02%	0.002%
59	8.517	2229	2232	2234	rBV2	409	293	0.02%	0.003%
60	8.533	2234	2237	2241	rVB2	291	206	0.02%	0.002%
61	8.632	2256	2268	2302	rBV	389903	731519	60.53%	7.259%
62	8.954	2363	2368	2370	rBV2	306	269	0.02%	0.003%
63	9.118	2416	2419	2425	rVB2	294	221	0.02%	0.002%
64	9.253	2457	2461	2465	rBV3	310	359	0.03%	0.004%
65	9.285	2468	2471	2477	rVB3	341	318	0.03%	0.003%
66	9.417	2499	2512	2541	rVV	587051	1089740	90.17%	10.814%
67	9.639	2579	2581	2584	rBV2	263	179	0.01%	0.002%
68	9.697	2593	2599	2607	rVB4	1117	1407	0.12%	0.014%
69	9.787	2625	2627	2630	rVB	626	339	0.03%	0.003%
70	9.806	2630	2633	2635	rBV	257	206	0.02%	0.002%
71	9.963	2677	2682	2686	rBB2	215	205	0.02%	0.002%
72	9.989	2686	2690	2692	rBV3	229	196	0.02%	0.002%
73	10.108	2724	2727	2730	rVB	389	207	0.02%	0.002%
74	10.230	2761	2765	2769	rVB2	292	255	0.02%	0.003%
75	10.372	2806	2809	2812	rVB2	346	248	0.02%	0.002%
76	10.397	2813	2817	2819	rBV2	422	349	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048038.D
 Acq On : 14 Apr 2022 04:54
 Operator : SY/MD
 Sample : N2386-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.433	2825	2828	2833	rBV2	326	281	0.02%	0.003%
78	10.671	2896	2902	2912	rVB4	1044	1498	0.12%	0.015%
79	10.758	2915	2929	2952	rVV	426117	690483	57.13%	6.852%
80	11.086	3023	3031	3033	rBV2	468	588	0.05%	0.006%
81	11.391	3122	3126	3129	rBV2	235	230	0.02%	0.002%
82	11.420	3132	3135	3138	rVB2	451	248	0.02%	0.002%
83	11.452	3141	3145	3148	rBV2	733	619	0.05%	0.006%
84	11.510	3160	3163	3168	rBV	186	203	0.02%	0.002%
85	11.687	3215	3218	3221	rBV2	256	226	0.02%	0.002%
86	11.706	3221	3224	3225	rVV	370	192	0.02%	0.002%
87	11.748	3229	3237	3244	rBV3	3196	4578	0.38%	0.045%
88	11.812	3244	3257	3279	rVV	629419	1027155	84.99%	10.193%
89	11.912	3286	3288	3291	rVB4	472	201	0.02%	0.002%
90	11.928	3291	3293	3295	rBV2	423	191	0.02%	0.002%
91	12.195	3362	3376	3400	rBV2	589522	1055767	87.36%	10.477%
92	12.581	3492	3496	3499	rBV	301	255	0.02%	0.003%
93	12.626	3507	3510	3511	rBV	321	174	0.01%	0.002%
94	12.741	3543	3546	3548	rBV2	238	195	0.02%	0.002%
95	12.793	3558	3562	3564	rBV2	498	418	0.03%	0.004%
96	12.831	3570	3574	3577	rBV2	347	412	0.03%	0.004%
97	12.909	3596	3598	3601	rVB2	380	188	0.02%	0.002%
98	12.979	3614	3620	3624	rBV3	661	777	0.06%	0.008%
99	13.844	3879	3889	3901	rBV2	42564	68958	5.71%	0.684%
100	14.333	4031	4041	4054	rBV3	7723	12382	1.02%	0.123%




Sum of corrected areas: 10076783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048038.D
Acq On : 14 Apr 2022 04:54
Operator : SY/MD
Sample : N2386-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

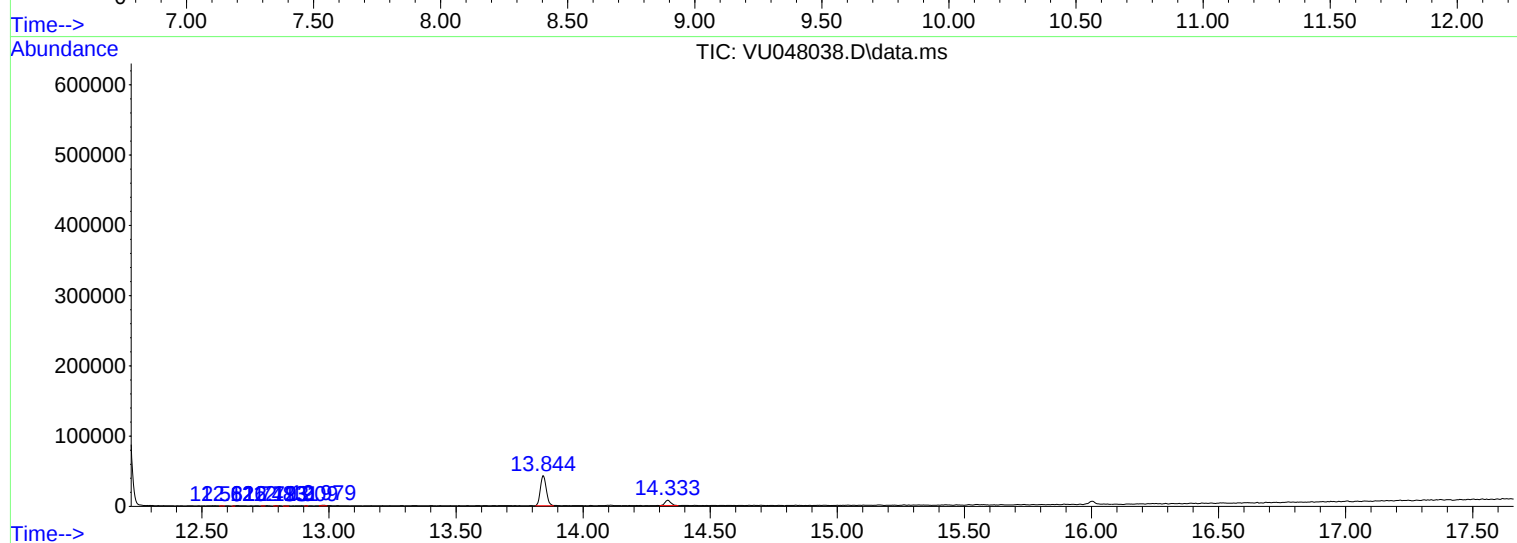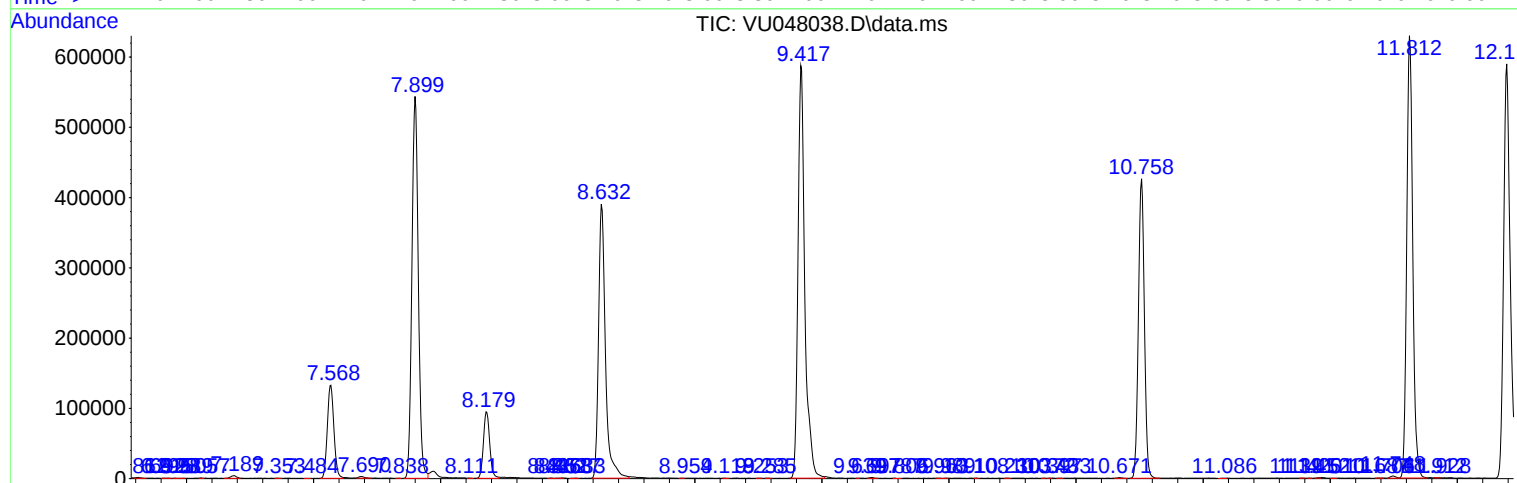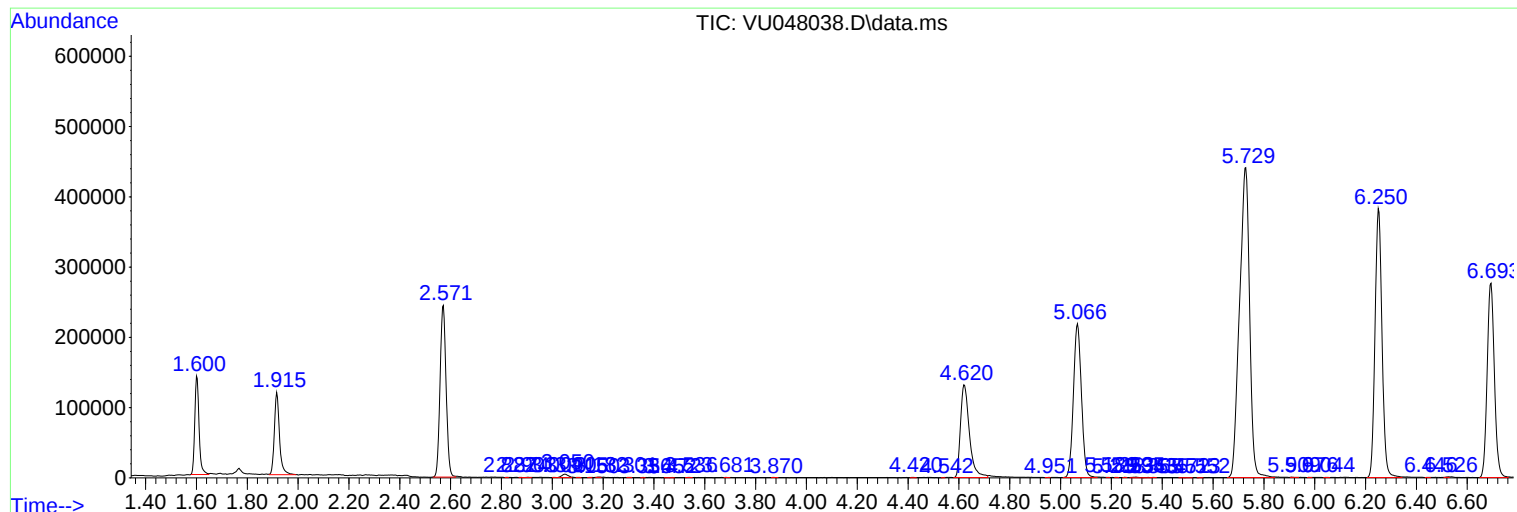

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048038.D
Acq On : 14 Apr 2022 04:54
Operator : SY/MD
Sample : N2386-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048038.D
Acq On : 14 Apr 2022 04:54
Operator : SY/MD
Sample : N2386-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc