

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048039.D
 Acq On : 14 Apr 2022 05:17
 Operator : SY/MD
 Sample : N2386-06 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	101	rVB	136527	158377	13.32%	1.623%
2	1.916	170	179	201	rVB	113872	160036	13.46%	1.640%
3	2.572	370	383	405	rBV	238463	394828	33.22%	4.047%
4	2.745	436	437	440	rVB3	393	193	0.02%	0.002%
5	2.787	448	450	453	rBV2	294	219	0.02%	0.002%
6	2.842	465	467	470	rVB2	351	195	0.02%	0.002%
7	2.864	471	474	478	rBV2	351	348	0.03%	0.004%
8	2.916	487	490	494	rBV	380	299	0.03%	0.003%
9	2.951	497	501	502	rBV2	394	270	0.02%	0.003%
10	2.986	510	512	514	rBV	286	165	0.01%	0.002%
11	3.047	523	531	546	rVB4	3924	7806	0.66%	0.080%
12	3.170	566	569	571	rBV2	347	255	0.02%	0.003%
13	3.189	573	575	581	rVB3	405	320	0.03%	0.003%
14	3.449	653	656	657	rVV	301	190	0.02%	0.002%
15	3.491	665	669	674	rBV2	201	247	0.02%	0.003%
16	3.546	685	686	690	rVB	385	185	0.02%	0.002%
17	3.572	690	694	695	rBV2	279	174	0.01%	0.002%
18	3.662	720	722	725	rBV	238	185	0.02%	0.002%
19	3.681	725	728	732	rVB3	279	209	0.02%	0.002%
20	3.765	749	754	757	rVB	344	233	0.02%	0.002%
21	3.803	762	766	769	rBV	266	225	0.02%	0.002%
22	3.851	778	781	784	rBV	241	163	0.01%	0.002%
23	3.912	797	800	805	rVB2	360	294	0.02%	0.003%
24	3.938	805	808	812	rVB3	370	310	0.03%	0.003%
25	4.038	836	839	843	rVB	235	177	0.01%	0.002%
26	4.539	991	995	997	rBV2	346	304	0.03%	0.003%
27	4.620	1007	1020	1058	rBV	132401	319428	26.87%	3.274%
28	4.925	1112	1115	1118	rBV	250	188	0.02%	0.002%
29	4.951	1120	1123	1126	rVB3	491	339	0.03%	0.003%
30	5.067	1142	1159	1180	rBV	218004	475643	40.01%	4.876%
31	5.221	1205	1207	1212	rVB4	291	241	0.02%	0.002%
32	5.301	1222	1232	1237	rBV4	775	1332	0.11%	0.014%
33	5.324	1237	1239	1243	rVV2	282	217	0.02%	0.002%
34	5.420	1265	1269	1272	rBV	320	341	0.03%	0.003%
35	5.478	1284	1287	1290	rBV2	237	193	0.02%	0.002%
36	5.626	1331	1333	1339	rVB2	293	241	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048039.D
 Acq On : 14 Apr 2022 05:17
 Operator : SY/MD
 Sample : N2386-06 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.729	1342	1365	1393	rBV2	433518	1188679	100.00%	12.184%
38	6.031	1457	1459	1462	rVV2	284	177	0.01%	0.002%
39	6.105	1476	1482	1484	rBV4	521	479	0.04%	0.005%
40	6.125	1486	1488	1491	rVB2	351	211	0.02%	0.002%
41	6.250	1507	1527	1549	rBV	386275	734872	61.82%	7.533%
42	6.526	1607	1613	1622	rBV5	1349	2377	0.20%	0.024%
43	6.578	1627	1629	1633	rVB2	357	192	0.02%	0.002%
44	6.610	1635	1639	1640	rBV2	349	184	0.02%	0.002%
45	6.694	1650	1665	1690	rBV	276965	540229	45.45%	5.538%
46	6.806	1697	1700	1701	rBV2	359	214	0.02%	0.002%
47	7.047	1770	1775	1778	rBV2	351	435	0.04%	0.004%
48	7.112	1790	1795	1802	rBV3	286	259	0.02%	0.003%
49	7.186	1803	1818	1827	rBV5	3398	6367	0.54%	0.065%
50	7.314	1854	1858	1860	rBV2	246	195	0.02%	0.002%
51	7.337	1862	1865	1871	rVV	363	312	0.03%	0.003%
52	7.391	1879	1882	1884	rBV	225	170	0.01%	0.002%
53	7.414	1884	1889	1893	rVV3	190	199	0.02%	0.002%
54	7.568	1923	1937	1956	rBV	129420	232077	19.52%	2.379%
55	7.690	1966	1975	1981	rBV6	2383	3638	0.31%	0.037%
56	7.735	1987	1989	1999	rVB4	369	493	0.04%	0.005%
57	7.899	2023	2040	2056	rBV	533454	926062	77.91%	9.492%
58	8.179	2116	2127	2144	rVV	91369	157868	13.28%	1.618%
59	8.555	2241	2244	2246	rBV	259	164	0.01%	0.002%
60	8.571	2246	2249	2256	rVB3	343	332	0.03%	0.003%
61	8.632	2256	2268	2305	rBV	384180	724967	60.99%	7.431%
62	8.784	2313	2315	2318	rVB4	693	284	0.02%	0.003%
63	8.938	2361	2363	2368	rVB3	298	180	0.02%	0.002%
64	9.108	2411	2416	2421	rBV3	532	622	0.05%	0.006%
65	9.137	2422	2425	2427	rVV2	371	236	0.02%	0.002%
66	9.163	2430	2433	2439	rVB2	501	512	0.04%	0.005%
67	9.198	2439	2444	2447	rBV2	315	335	0.03%	0.003%
68	9.324	2479	2483	2485	rBV3	269	187	0.02%	0.002%
69	9.417	2495	2512	2549	rBV	590668	1022172	85.99%	10.478%
70	9.581	2561	2563	2566	rVB3	395	206	0.02%	0.002%
71	9.652	2583	2585	2589	rVB2	259	175	0.01%	0.002%
72	9.674	2589	2592	2593	rBV	378	229	0.02%	0.002%
73	9.694	2595	2598	2608	rVB3	981	1186	0.10%	0.012%
74	9.970	2679	2684	2686	rBV2	154	167	0.01%	0.002%
75	10.047	2704	2708	2710	rBV2	309	189	0.02%	0.002%
76	10.079	2714	2718	2721	rBV2	280	218	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048039.D
 Acq On : 14 Apr 2022 05:17
 Operator : SY/MD
 Sample : N2386-06 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.359	2802	2805	2807	rBV2	282	211	0.02%	0.002%
78	10.378	2808	2811	2815	rVV	322	252	0.02%	0.003%
79	10.671	2897	2902	2908	rBV2	1049	1069	0.09%	0.011%
80	10.758	2916	2929	2949	rBV	424653	687268	57.82%	7.045%
81	10.829	2949	2951	2955	rVB3	368	252	0.02%	0.003%
82	11.044	3015	3018	3020	rBV2	264	194	0.02%	0.002%
83	11.690	3217	3219	3224	rVB2	534	400	0.03%	0.004%
84	11.748	3228	3237	3244	rBV4	1456	2137	0.18%	0.022%
85	11.812	3244	3257	3276	rBV	636233	1023672	86.12%	10.493%
86	11.967	3302	3305	3308	rBV3	587	551	0.05%	0.006%
87	12.195	3362	3376	3396	rBV	551117	946527	79.63%	9.702%
88	12.269	3396	3399	3403	rVB3	647	554	0.05%	0.006%
89	12.468	3457	3461	3466	rBV2	397	451	0.04%	0.005%
90	12.555	3483	3488	3492	rBV2	245	305	0.03%	0.003%
91	12.600	3499	3502	3506	rVB2	324	255	0.02%	0.003%
92	12.677	3524	3526	3529	rVB	340	201	0.02%	0.002%
93	12.828	3571	3573	3575	rBV	274	161	0.01%	0.002%
94	12.906	3592	3597	3601	rBV2	304	388	0.03%	0.004%
95	12.947	3607	3610	3615	rVB2	288	221	0.02%	0.002%
96	12.980	3615	3620	3626	rBV3	594	733	0.06%	0.008%
97	13.105	3654	3659	3663	rVB3	428	390	0.03%	0.004%
98	13.848	3880	3890	3904	rBV3	10149	16587	1.40%	0.170%
99	14.291	4025	4028	4032	rBV	425	351	0.03%	0.004%
100	15.542	4415	4417	4418	rBV	555	222	0.02%	0.002%

Sum of corrected areas: 9755772




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048039.D
Acq On : 14 Apr 2022 05:17
Operator : SY/MD
Sample : N2386-06 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

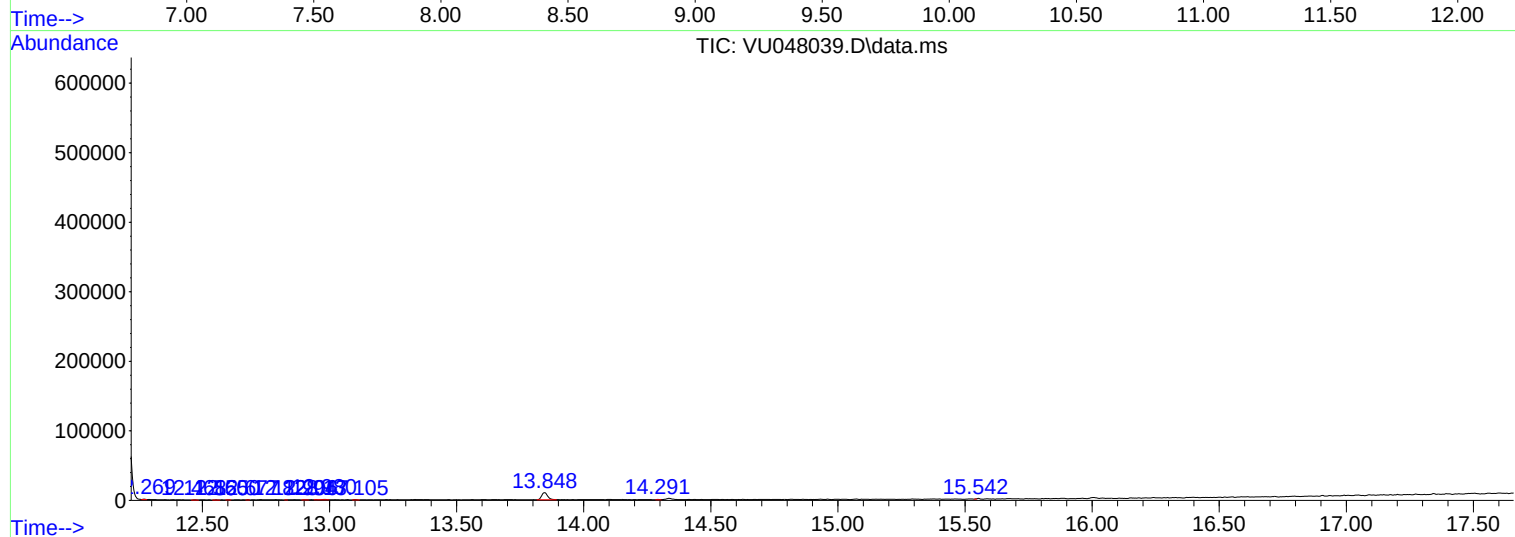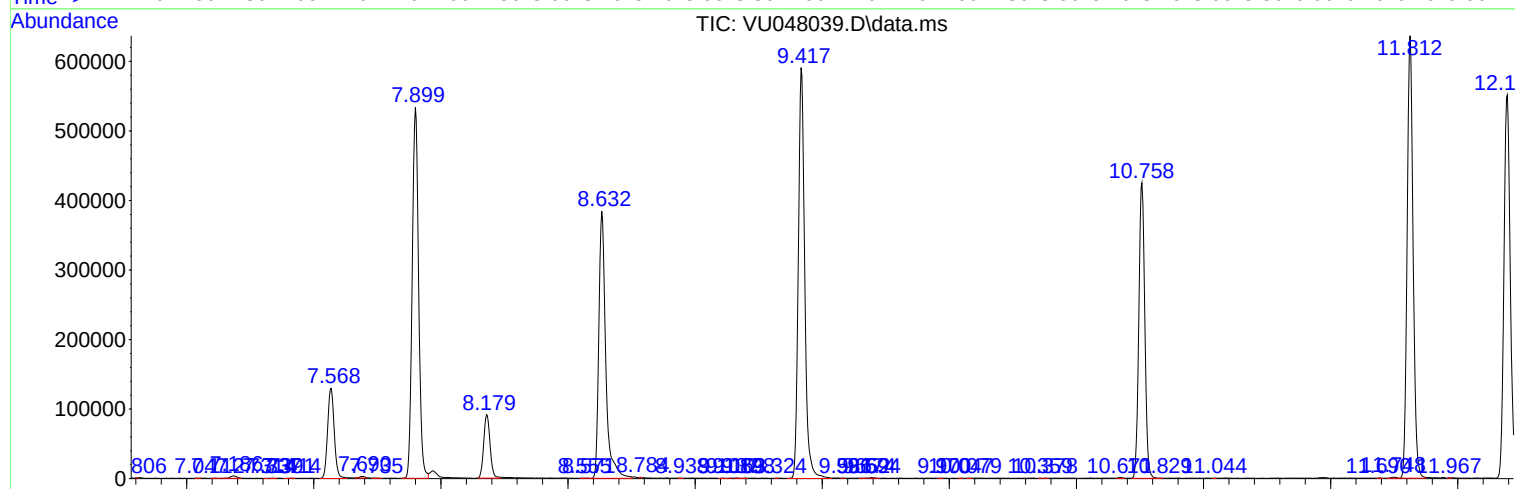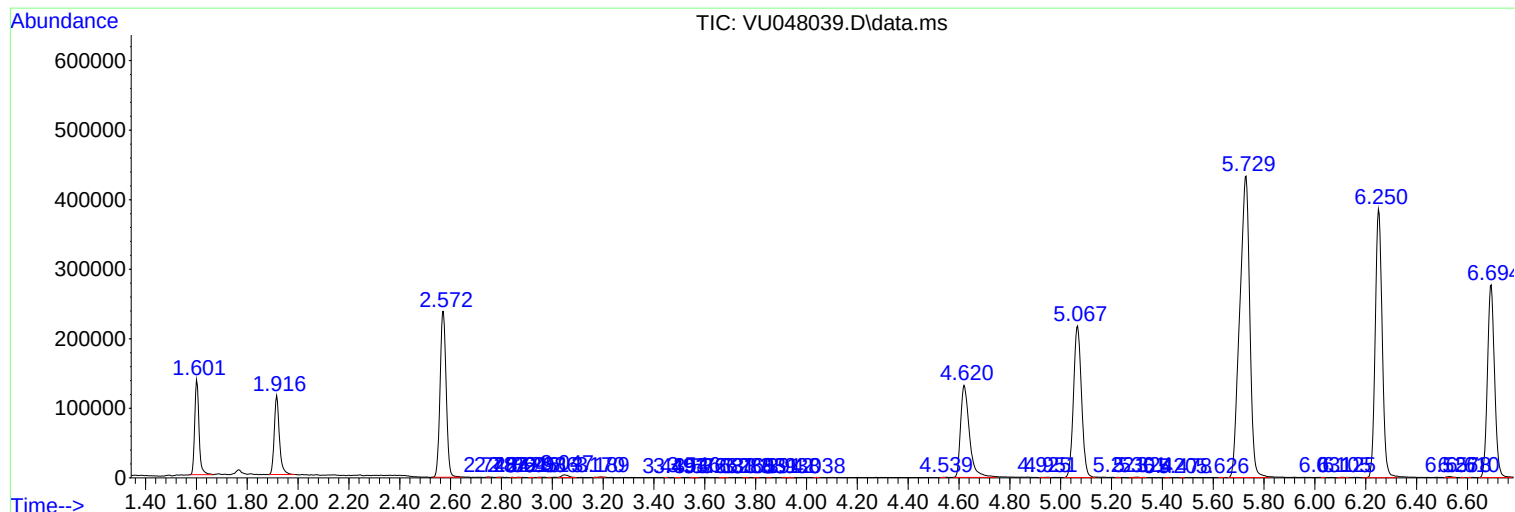

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048039.D
Acq On : 14 Apr 2022 05:17
Operator : SY/MD
Sample : N2386-06 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048039.D
Acq On : 14 Apr 2022 05:17
Operator : SY/MD
Sample : N2386-06 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------