

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048040.D
 Acq On : 14 Apr 2022 05:41
 Operator : SY/MD
 Sample : N2386-16 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rBV	137185	157745	13.22%	1.628%
2	1.916	171	179	203	rVB	115813	162369	13.61%	1.676%
3	2.572	370	383	407	rBV	242276	400033	33.52%	4.129%
4	2.668	411	413	417	rVB3	430	273	0.02%	0.003%
5	2.694	417	421	422	rBV2	295	189	0.02%	0.002%
6	2.752	432	439	449	rBV2	5442	9274	0.78%	0.096%
7	2.838	464	466	469	rBV4	302	227	0.02%	0.002%
8	2.890	480	482	486	rVB2	304	225	0.02%	0.002%
9	3.051	523	532	546	rVB3	3328	6767	0.57%	0.070%
10	3.131	554	557	560	rBV	275	215	0.02%	0.002%
11	3.182	568	573	582	rBV4	710	1336	0.11%	0.014%
12	3.237	586	590	593	rBV2	483	398	0.03%	0.004%
13	3.382	630	635	638	rVB2	419	409	0.03%	0.004%
14	3.408	638	643	645	rBV2	213	207	0.02%	0.002%
15	3.424	645	648	650	rBV	303	209	0.02%	0.002%
16	3.546	682	686	689	rBV2	318	240	0.02%	0.002%
17	3.626	708	711	714	rVV3	280	211	0.02%	0.002%
18	3.694	729	732	738	rBV	280	232	0.02%	0.002%
19	3.752	747	750	754	rBV3	321	296	0.02%	0.003%
20	3.838	770	777	780	rVB2	252	314	0.03%	0.003%
21	3.867	784	786	791	rVB3	313	187	0.02%	0.002%
22	3.973	815	819	823	rVB2	308	295	0.02%	0.003%
23	4.060	843	846	849	rVV2	315	225	0.02%	0.002%
24	4.105	857	860	864	rBV2	204	197	0.02%	0.002%
25	4.137	865	870	874	rBV3	256	268	0.02%	0.003%
26	4.221	894	896	899	rVV	270	210	0.02%	0.002%
27	4.562	999	1002	1007	rVB4	248	203	0.02%	0.002%
28	4.620	1007	1020	1060	rBV	132013	322393	27.01%	3.328%
29	5.067	1141	1159	1183	rBV	216820	475569	39.85%	4.909%
30	5.340	1239	1244	1246	rBV2	236	246	0.02%	0.003%
31	5.729	1340	1365	1396	rBV2	433582	1193395	100.00%	12.318%
32	5.983	1442	1444	1447	rVB2	334	218	0.02%	0.002%
33	6.044	1458	1463	1466	rBV2	317	354	0.03%	0.004%
34	6.063	1466	1469	1472	rVB2	438	290	0.02%	0.003%
35	6.179	1503	1505	1510	rVB3	310	187	0.02%	0.002%
36	6.250	1511	1527	1551	rBV	379147	725211	60.77%	7.485%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048040.D
 Acq On : 14 Apr 2022 05:41
 Operator : SY/MD
 Sample : N2386-16 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.362	1559	1562	1570	rVB3	939	1057	0.09%	0.011%
38	6.401	1570	1574	1578	rBV4	457	422	0.04%	0.004%
39	6.497	1601	1604	1608	rVV2	261	200	0.02%	0.002%
40	6.526	1608	1613	1625	rVB5	1116	1921	0.16%	0.020%
41	6.694	1650	1665	1691	rBV	275680	541851	45.40%	5.593%
42	6.877	1718	1722	1725	rVB2	270	241	0.02%	0.002%
43	6.906	1725	1731	1733	rBV2	225	199	0.02%	0.002%
44	6.925	1734	1737	1742	rVB2	305	263	0.02%	0.003%
45	7.047	1771	1775	1782	rVB2	510	549	0.05%	0.006%
46	7.105	1789	1793	1797	rBV2	277	274	0.02%	0.003%
47	7.186	1809	1818	1827	rBV3	3730	6109	0.51%	0.063%
48	7.250	1836	1838	1843	rVB3	439	333	0.03%	0.003%
49	7.520	1917	1922	1924	rBV3	269	243	0.02%	0.003%
50	7.568	1924	1937	1956	rBV	129770	230693	19.33%	2.381%
51	7.690	1968	1975	1986	rVB5	2695	4925	0.41%	0.051%
52	7.793	2002	2007	2010	rBV3	382	341	0.03%	0.004%
53	7.899	2023	2040	2057	rBV	536856	928914	77.84%	9.588%
54	8.179	2116	2127	2145	rBV	92000	157763	13.22%	1.628%
55	8.578	2247	2251	2254	rBV3	293	204	0.02%	0.002%
56	8.632	2254	2268	2306	rBV	382494	727914	61.00%	7.513%
57	8.819	2321	2326	2330	rBV3	447	571	0.05%	0.006%
58	8.838	2330	2332	2335	rVB2	486	239	0.02%	0.002%
59	8.980	2371	2376	2378	rBV3	262	288	0.02%	0.003%
60	9.086	2406	2409	2414	rBV2	352	313	0.03%	0.003%
61	9.166	2432	2434	2437	rVV2	372	190	0.02%	0.002%
62	9.185	2437	2440	2444	rVB2	352	261	0.02%	0.003%
63	9.275	2463	2468	2471	rBV3	316	345	0.03%	0.004%
64	9.298	2471	2475	2477	rVV	266	249	0.02%	0.003%
65	9.417	2497	2512	2550	rBV	575420	993861	83.28%	10.258%
66	9.697	2592	2599	2603	rVV2	780	1122	0.09%	0.012%
67	9.809	2629	2634	2638	rVB	389	368	0.03%	0.004%
68	9.857	2645	2649	2651	rBV2	247	201	0.02%	0.002%
69	10.076	2713	2717	2721	rBV2	405	299	0.03%	0.003%
70	10.095	2721	2723	2726	rBV	320	241	0.02%	0.002%
71	10.208	2748	2758	2762	rBV2	363	644	0.05%	0.007%
72	10.250	2766	2771	2773	rBV2	256	305	0.03%	0.003%
73	10.330	2790	2796	2798	rVB2	231	210	0.02%	0.002%
74	10.398	2809	2817	2822	rBV2	608	871	0.07%	0.009%
75	10.546	2859	2863	2866	rVB2	393	256	0.02%	0.003%
76	10.648	2889	2895	2897	rBV	251	253	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048040.D
 Acq On : 14 Apr 2022 05:41
 Operator : SY/MD
 Sample : N2386-16 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.668	2897	2901	2908	rVV3	986	1111	0.09%	0.011%
78	10.758	2916	2929	2947	rBV	422326	687886	57.64%	7.100%
79	10.992	2999	3002	3006	rVB3	268	202	0.02%	0.002%
80	11.015	3006	3009	3013	rVB3	483	389	0.03%	0.004%
81	11.047	3013	3019	3020	rBV2	297	288	0.02%	0.003%
82	11.134	3043	3046	3048	rBV2	336	204	0.02%	0.002%
83	11.150	3048	3051	3054	rVB	336	258	0.02%	0.003%
84	11.179	3054	3060	3063	rBV2	432	488	0.04%	0.005%
85	11.455	3141	3146	3148	rBV2	899	791	0.07%	0.008%
86	11.581	3182	3185	3190	rVB	349	252	0.02%	0.003%
87	11.697	3219	3221	3227	rVB2	548	412	0.03%	0.004%
88	11.748	3233	3237	3244	rVB5	641	668	0.06%	0.007%
89	11.812	3244	3257	3279	rBV	617898	996091	83.47%	10.281%
90	11.973	3305	3307	3315	rVB4	931	1009	0.08%	0.010%
91	12.037	3324	3327	3331	rVB2	304	199	0.02%	0.002%
92	12.089	3340	3343	3347	rVB3	470	440	0.04%	0.005%
93	12.195	3362	3376	3396	rBV	552583	921207	77.19%	9.508%
94	12.404	3435	3441	3443	rBV2	362	390	0.03%	0.004%
95	12.806	3562	3566	3569	rBV2	418	429	0.04%	0.004%
96	12.976	3616	3619	3623	rVB2	585	507	0.04%	0.005%
97	13.848	3882	3890	3902	rBV3	4893	7521	0.63%	0.078%
98	14.324	4036	4038	4040	rBV2	420	238	0.02%	0.002%
99	15.600	4431	4435	4437	rBV3	768	658	0.06%	0.007%
100	15.687	4459	4462	4466	rBV3	653	584	0.05%	0.006%


Sum of corrected areas: 9688342

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048040.D
Acq On : 14 Apr 2022 05:41
Operator : SY/MD
Sample : N2386-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

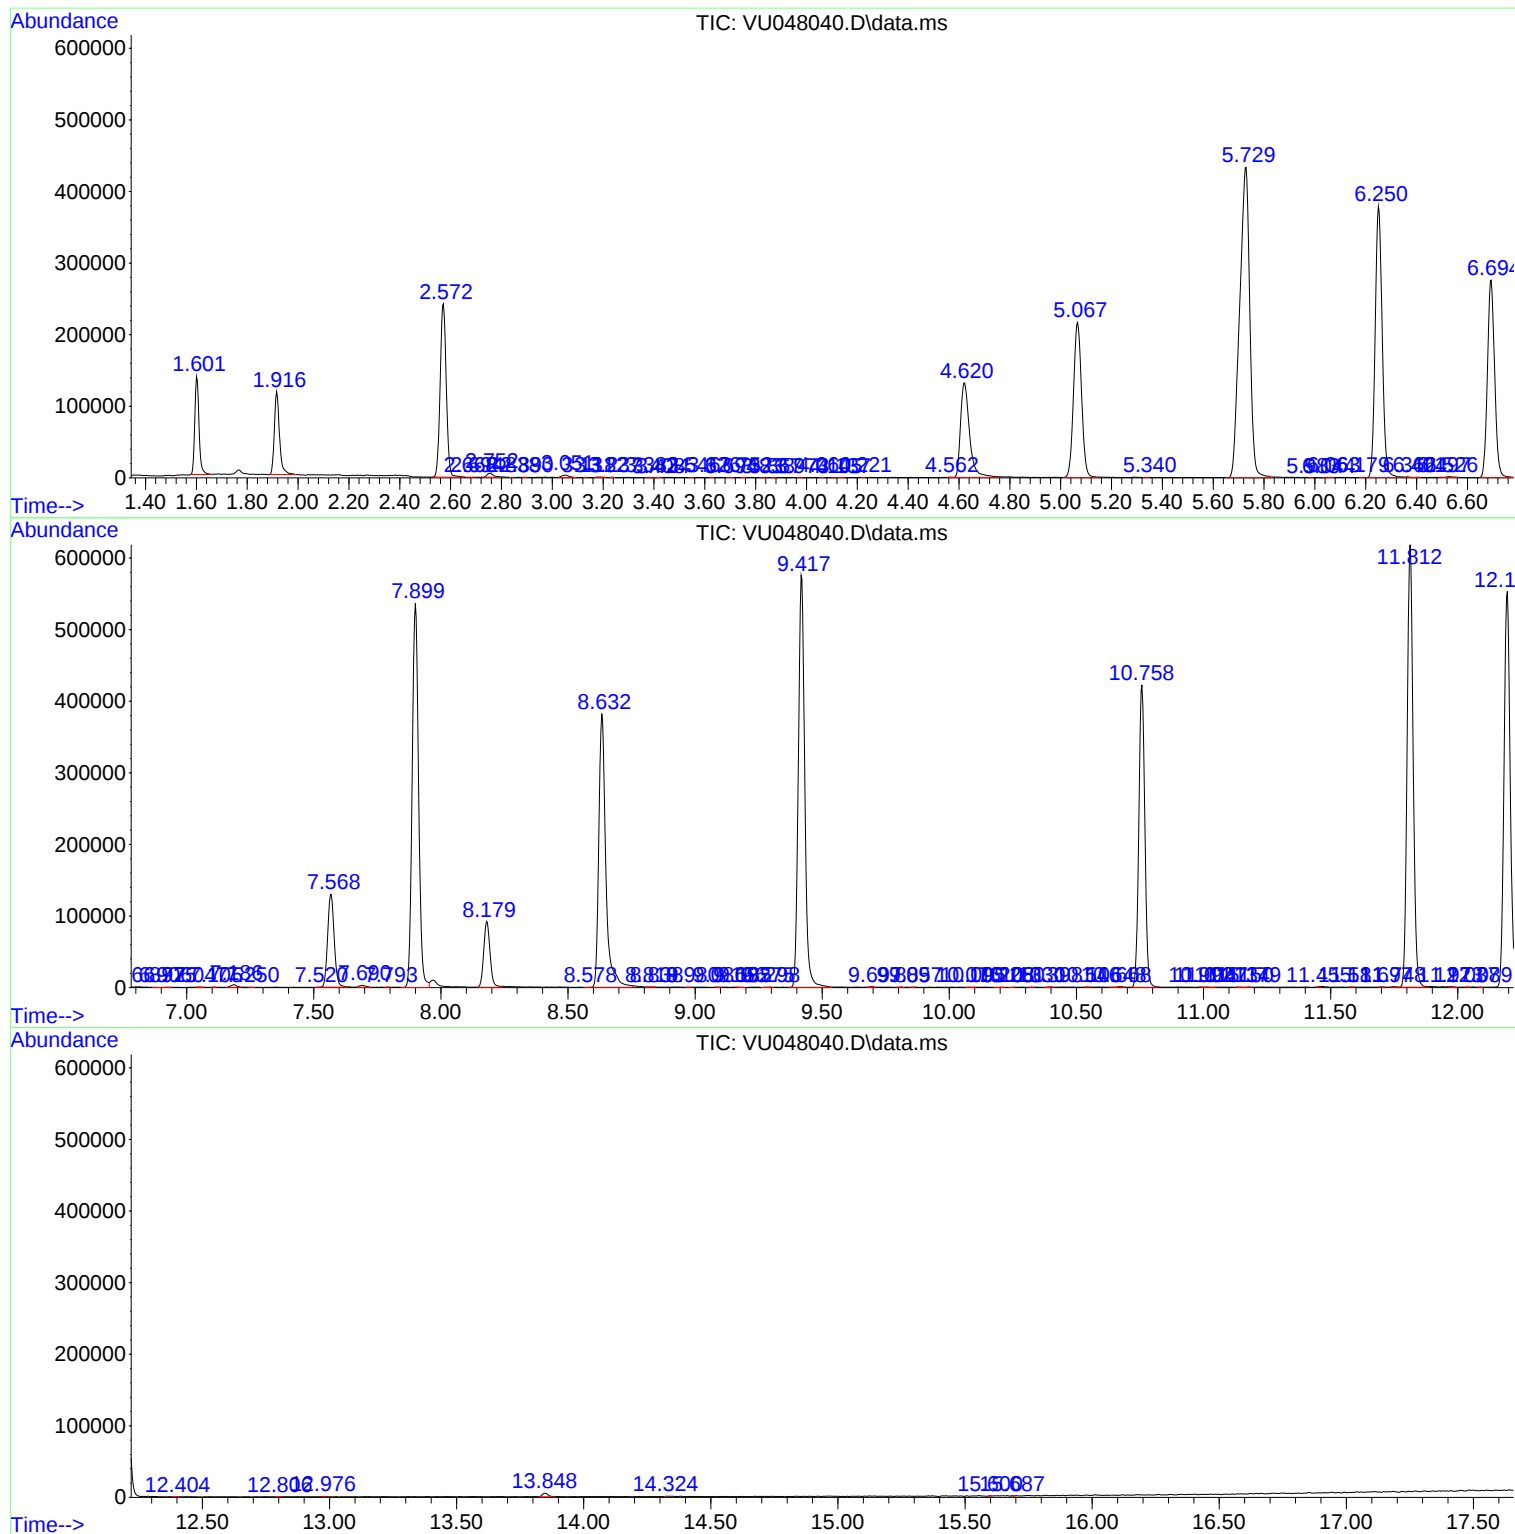

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048040.D
Acq On : 14 Apr 2022 05:41
Operator : SY/MD
Sample : N2386-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048040.D
Acq On : 14 Apr 2022 05:41
Operator : SY/MD
Sample : N2386-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------