

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
 Data File : VU053679.D
 Acq On : 13 Apr 2023 11:48
 Operator : JC/MD
 Sample : VU0413WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	102	rVB	110563	137504	17.11%	2.139%
2	1.890	165	171	189	rVB	77282	109474	13.62%	1.703%
3	2.559	367	379	394	rBV	169604	277929	34.58%	4.323%
4	3.137	556	559	561	rBV2	224	133	0.02%	0.002%
5	3.247	590	593	597	rBV	267	166	0.02%	0.003%
6	3.343	619	623	628	rBV3	488	469	0.06%	0.007%
7	3.459	657	659	661	rVB3	358	118	0.01%	0.002%
8	3.552	687	688	692	rVB	249	91	0.01%	0.001%
9	4.083	851	853	856	rBV	222	155	0.02%	0.002%
10	4.192	882	887	890	rBV2	306	346	0.04%	0.005%
11	4.221	894	896	899	rVB	227	121	0.02%	0.002%
12	4.333	928	931	934	rVB2	277	176	0.02%	0.003%
13	4.613	1007	1018	1041	rBV	65526	156332	19.45%	2.431%
14	4.951	1121	1123	1125	rBV	268	158	0.02%	0.002%
15	5.057	1140	1156	1180	rBV	150389	326421	40.62%	5.077%
16	5.275	1222	1224	1227	rBV2	491	343	0.04%	0.005%
17	5.327	1235	1240	1244	rBV3	586	717	0.09%	0.011%
18	5.365	1250	1252	1254	rBV	321	169	0.02%	0.003%
19	5.410	1263	1266	1268	rBV	176	83	0.01%	0.001%
20	5.632	1332	1335	1341	rBB2	175	142	0.02%	0.002%
21	5.719	1341	1362	1381	rBV3	296730	803627	100.00%	12.499%
22	5.973	1433	1441	1443	rBV2	296	439	0.05%	0.007%
23	6.028	1456	1458	1461	rBV	242	118	0.01%	0.002%
24	6.166	1498	1501	1503	rBV	164	97	0.01%	0.002%
25	6.243	1512	1525	1541	rBV	296132	551450	68.62%	8.577%
26	6.449	1586	1589	1590	rBV2	277	137	0.02%	0.002%
27	6.526	1604	1613	1625	rVB7	3388	6154	0.77%	0.096%
28	6.597	1634	1635	1643	rVB2	352	215	0.03%	0.003%
29	6.636	1643	1647	1648	rBV	188	116	0.01%	0.002%
30	6.684	1648	1662	1683	rBV	182434	357183	44.45%	5.555%
31	6.845	1710	1712	1713	rBV	193	102	0.01%	0.002%
32	6.902	1728	1730	1732	rBV	167	92	0.01%	0.001%
33	6.947	1741	1744	1747	rBV2	216	187	0.02%	0.003%
34	7.005	1761	1762	1763	rBV	237	73	0.01%	0.001%
35	7.150	1804	1807	1809	rBV	186	159	0.02%	0.002%
36	7.176	1812	1815	1817	rVV	601	436	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
 Data File : VU053679.D
 Acq On : 13 Apr 2023 11:48
 Operator : JC/MD
 Sample : VU0413WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.201	1821	1823	1826	rBV2	261	134	0.02%	0.002%
38	7.263	1839	1842	1844	rVB2	340	173	0.02%	0.003%
39	7.282	1846	1848	1852	rVB2	280	168	0.02%	0.003%
40	7.324	1859	1861	1862	rBV	173	68	0.01%	0.001%
41	7.381	1876	1879	1881	rBV	330	235	0.03%	0.004%
42	7.398	1882	1884	1887	rVV	166	89	0.01%	0.001%
43	7.430	1892	1894	1899	rVB	276	156	0.02%	0.002%
44	7.472	1904	1907	1910	rVV	298	159	0.02%	0.002%
45	7.562	1923	1935	1952	rBV	99791	173600	21.60%	2.700%
46	7.841	2019	2022	2025	rBV	194	103	0.01%	0.002%
47	7.893	2025	2038	2069	rBV	374776	650183	80.91%	10.112%
48	8.082	2094	2097	2101	rVB3	374	262	0.03%	0.004%
49	8.176	2115	2126	2147	rBV	70335	118050	14.69%	1.836%
50	8.398	2192	2195	2198	rVB	277	159	0.02%	0.002%
51	8.578	2249	2251	2253	rBV	175	81	0.01%	0.001%
52	8.629	2256	2267	2296	rVV	214035	380178	47.31%	5.913%
53	8.989	2377	2379	2380	rBV	269	80	0.01%	0.001%
54	9.160	2430	2432	2435	rBV2	265	169	0.02%	0.003%
55	9.414	2498	2511	2530	rBV	397486	658709	81.97%	10.245%
56	9.565	2553	2558	2565	rBV3	759	1069	0.13%	0.017%
57	9.825	2636	2639	2644	rBV2	263	294	0.04%	0.005%
58	9.960	2676	2681	2682	rBV	258	214	0.03%	0.003%
59	10.092	2720	2722	2725	rBV2	421	339	0.04%	0.005%
60	10.156	2739	2742	2747	rVB3	400	341	0.04%	0.005%
61	10.295	2782	2785	2786	rBV	203	135	0.02%	0.002%
62	10.751	2916	2927	2942	rBV	279979	447792	55.72%	6.964%
63	11.082	3026	3030	3031	rBV	434	341	0.04%	0.005%
64	11.748	3229	3237	3244	rBV4	2040	2934	0.37%	0.046%
65	11.809	3244	3256	3277	rBV	398705	634936	79.01%	9.875%
66	12.188	3361	3374	3391	rBV	362434	594107	73.93%	9.240%
67	12.838	3574	3576	3578	rBV	228	101	0.01%	0.002%
68	13.224	3689	3696	3705	rBV5	2180	3559	0.44%	0.055%
69	13.262	3705	3708	3712	rBV2	507	382	0.05%	0.006%
70	13.433	3759	3761	3765	rBV2	400	268	0.03%	0.004%
71	13.712	3846	3848	3849	rBV	278	134	0.02%	0.002%
72	13.777	3864	3868	3873	rBV2	448	441	0.05%	0.007%
73	13.841	3881	3888	3897	rBV5	5241	7543	0.94%	0.117%
74	13.921	3911	3913	3917	rBV	422	312	0.04%	0.005%
75	14.089	3958	3965	3975	rBV2	8493	13369	1.66%	0.208%
76	14.259	4015	4018	4019	rBV	244	132	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
Data File : VU053679.D
Acq On : 13 Apr 2023 11:48
Operator : JC/MD
Sample : VU0413WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK078

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	14.330	4034	4040	4050	rVB5	4237	6607	0.82%	0.103%
----	--------	------	------	------	------	------	------	-------	--------




Sum of corrected areas: 6429738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
Data File : VU053679.D
Acq On : 13 Apr 2023 11:48
Operator : JC/MD
Sample : VU0413WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK078

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

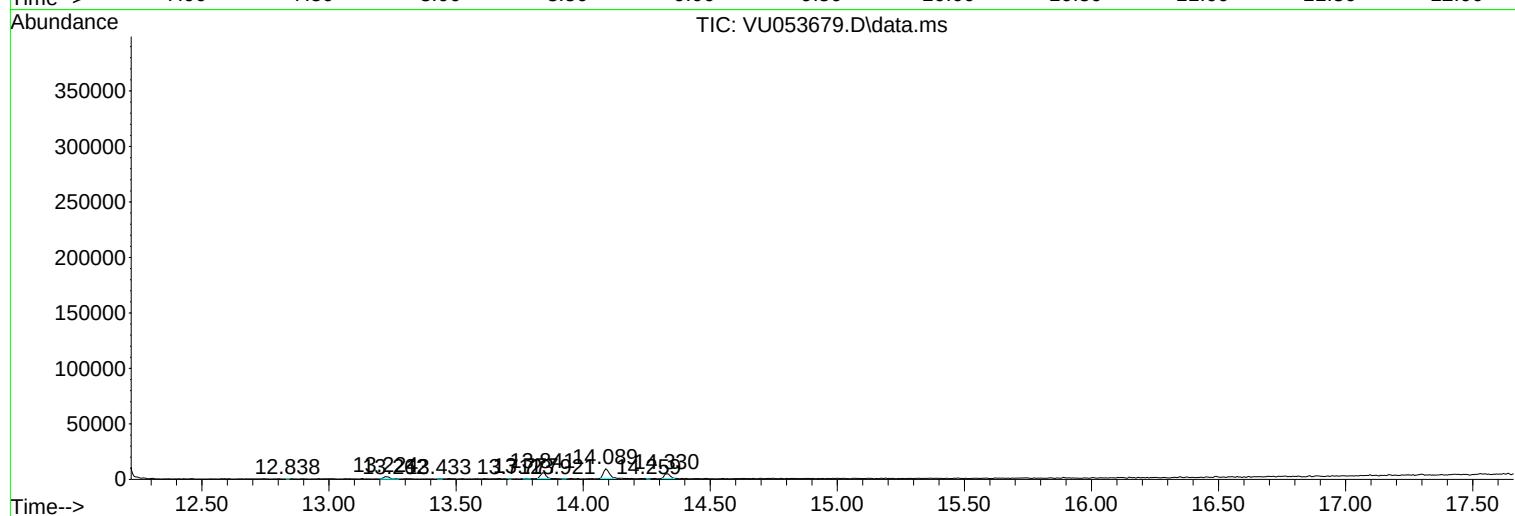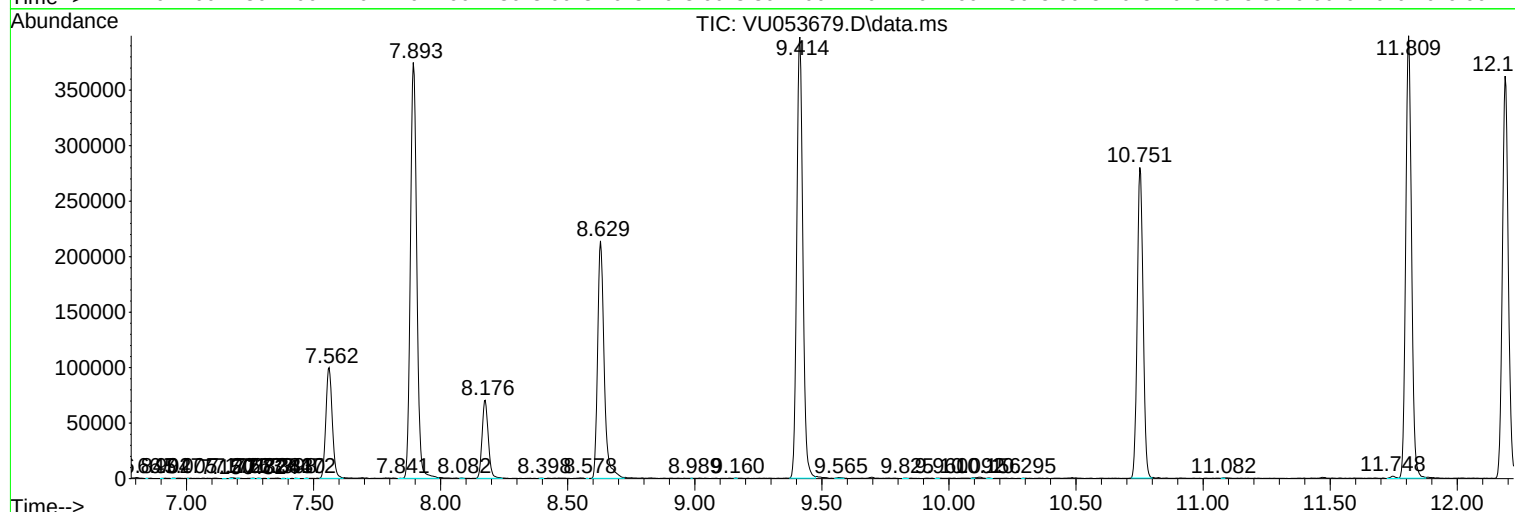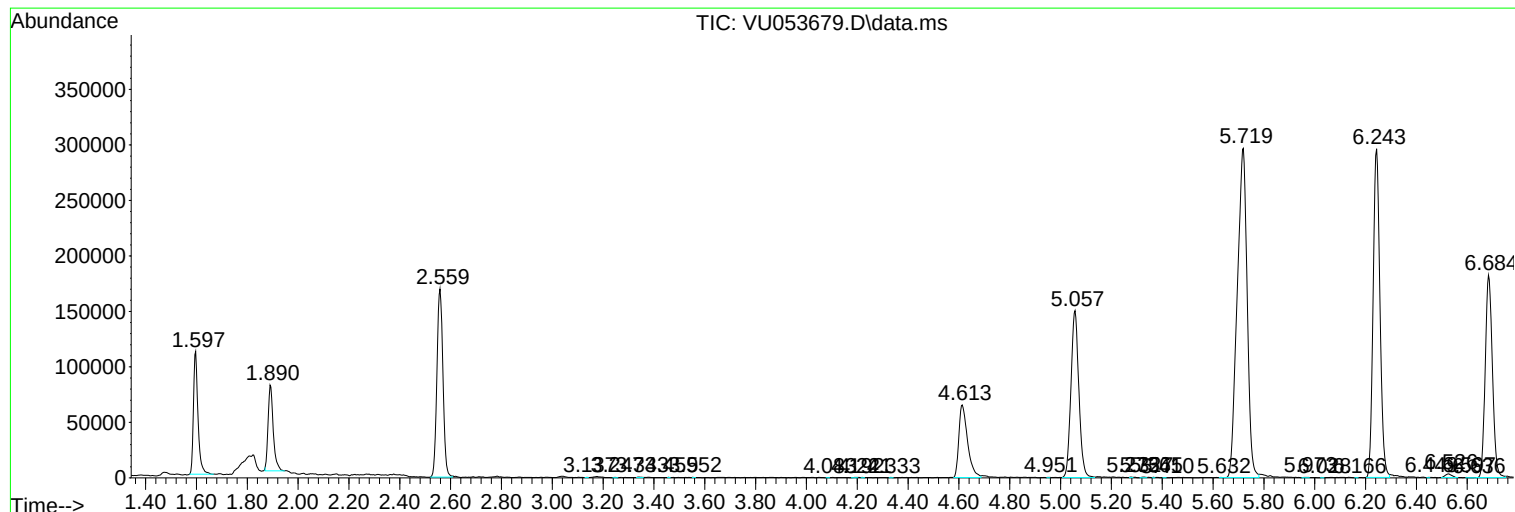

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
Data File : VU053679.D
Acq On : 13 Apr 2023 11:48
Operator : JC/MD
Sample : VU0413WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK078

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
Data File : VU053679.D
Acq On : 13 Apr 2023 11:48
Operator : JC/MD
Sample : VU0413WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK078

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------