

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
 Data File : VU053680.D
 Acq On : 13 Apr 2023 12:16
 Operator : JC/MD
 Sample : 02252-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	105854	127391	13.85%	1.894%
2	1.909	169	177	193	rBV	83774	120225	13.07%	1.787%
3	2.562	368	380	396	rBV	172485	280109	30.45%	4.165%
4	2.887	479	481	486	rBV	232	146	0.02%	0.002%
5	3.028	523	525	526	rBV	344	160	0.02%	0.002%
6	3.044	526	530	539	rVV3	1059	1224	0.13%	0.018%
7	3.080	539	541	545	rVB2	269	170	0.02%	0.003%
8	3.160	563	566	567	rBV	403	218	0.02%	0.003%
9	3.263	596	598	602	rBV	186	157	0.02%	0.002%
10	3.311	610	613	619	rVB	286	213	0.02%	0.003%
11	3.340	619	622	624	rBV	285	195	0.02%	0.003%
12	3.356	625	627	633	rVB	328	240	0.03%	0.004%
13	3.719	734	740	741	rBV	222	209	0.02%	0.003%
14	3.880	787	790	792	rBV2	312	201	0.02%	0.003%
15	4.141	868	871	876	rVB	274	206	0.02%	0.003%
16	4.170	876	880	883	rBV	277	243	0.03%	0.004%
17	4.301	917	921	924	rVB2	278	205	0.02%	0.003%
18	4.346	932	935	941	rBV	163	150	0.02%	0.002%
19	4.514	984	987	990	rVB2	218	161	0.02%	0.002%
20	4.613	1007	1018	1046	rBV2	62689	154393	16.78%	2.295%
21	5.057	1141	1156	1181	rVV	147035	317418	34.50%	4.719%
22	5.269	1219	1222	1225	rBV	315	214	0.02%	0.003%
23	5.324	1237	1239	1245	rVB2	302	209	0.02%	0.003%
24	5.391	1256	1260	1265	rVB2	278	274	0.03%	0.004%
25	5.414	1265	1267	1273	rBV	239	199	0.02%	0.003%
26	5.591	1317	1322	1324	rBV2	294	254	0.03%	0.004%
27	5.719	1341	1362	1374	rBV2	283492	785367	85.37%	11.677%
28	5.957	1433	1436	1439	rVB2	266	196	0.02%	0.003%
29	5.977	1439	1442	1445	rVB	266	164	0.02%	0.002%
30	5.999	1445	1449	1454	rVB2	345	281	0.03%	0.004%
31	6.124	1481	1488	1491	rBV3	462	511	0.06%	0.008%
32	6.243	1512	1525	1548	rBV	297970	568629	61.81%	8.454%
33	6.456	1588	1591	1595	rVB2	431	400	0.04%	0.006%
34	6.478	1595	1598	1604	rBV	493	466	0.05%	0.007%
35	6.530	1606	1614	1622	rVV9	2368	4247	0.46%	0.063%
36	6.687	1648	1663	1681	rBV	178165	344230	37.42%	5.118%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
 Data File : VU053680.D
 Acq On : 13 Apr 2023 12:16
 Operator : JC/MD
 Sample : 02252-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.809	1694	1701	1706	rVB4	940	1122	0.12%	0.017%
38	6.851	1712	1714	1717	rBV2	314	186	0.02%	0.003%
39	6.919	1731	1735	1736	rBV2	171	145	0.02%	0.002%
40	6.980	1751	1754	1757	rVB2	279	205	0.02%	0.003%
41	7.002	1757	1761	1770	rBV	158	246	0.03%	0.004%
42	7.150	1802	1807	1812	rBV	323	293	0.03%	0.004%
43	7.189	1812	1819	1821	rVV	636	717	0.08%	0.011%
44	7.214	1825	1827	1833	rVB2	276	201	0.02%	0.003%
45	7.301	1850	1854	1856	rVV	315	203	0.02%	0.003%
46	7.321	1857	1860	1866	rVB	322	260	0.03%	0.004%
47	7.507	1913	1918	1923	rBV2	190	232	0.03%	0.003%
48	7.562	1923	1935	1958	rBV	100291	174846	19.01%	2.600%
49	7.687	1971	1974	1978	rBV	588	614	0.07%	0.009%
50	7.755	1990	1995	1998	rBV2	231	200	0.02%	0.003%
51	7.790	1998	2006	2016	rBV4	1044	1888	0.21%	0.028%
52	7.893	2025	2038	2060	rBV	367944	645543	70.17%	9.598%
53	8.092	2097	2100	2103	rBV	196	153	0.02%	0.002%
54	8.131	2108	2112	2114	rBV2	204	160	0.02%	0.002%
55	8.176	2115	2126	2141	rBV	67909	115813	12.59%	1.722%
56	8.301	2161	2165	2172	rBV2	370	449	0.05%	0.007%
57	8.433	2201	2206	2210	rVB2	266	301	0.03%	0.004%
58	8.478	2210	2220	2225	rBV3	873	1423	0.15%	0.021%
59	8.504	2225	2228	2233	rVB2	187	149	0.02%	0.002%
60	8.533	2233	2237	2239	rBV	258	211	0.02%	0.003%
61	8.552	2241	2243	2248	rVB	414	268	0.03%	0.004%
62	8.629	2255	2267	2297	rBV	189468	349800	38.02%	5.201%
63	8.771	2309	2311	2315	rBV2	258	163	0.02%	0.002%
64	9.031	2386	2392	2396	rVB2	340	358	0.04%	0.005%
65	9.083	2405	2408	2411	rVB2	246	162	0.02%	0.002%
66	9.279	2466	2469	2473	rBV	253	202	0.02%	0.003%
67	9.414	2493	2511	2538	rBV2	413897	919992	100.00%	13.678%
68	9.610	2570	2572	2577	rVB	336	230	0.03%	0.003%
69	9.687	2594	2596	2597	rBV	682	306	0.03%	0.005%
70	9.761	2616	2619	2620	rBV2	282	185	0.02%	0.003%
71	9.902	2660	2663	2666	rBV2	275	238	0.03%	0.004%
72	10.099	2720	2724	2727	rBV2	252	257	0.03%	0.004%
73	10.301	2784	2787	2791	rBV	151	158	0.02%	0.002%
74	10.369	2806	2808	2812	rVB2	236	155	0.02%	0.002%
75	10.751	2915	2927	2944	rBV	252000	404739	43.99%	6.018%
76	10.854	2956	2959	2960	rBV	278	145	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
 Data File : VU053680.D
 Acq On : 13 Apr 2023 12:16
 Operator : JC/MD
 Sample : 02252-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.877	2963	2966	2967	rBV	588	336	0.04%	0.005%
78	10.980	2993	2998	3000	rBV2	236	228	0.02%	0.003%
79	11.311	3099	3101	3104	rBV2	271	180	0.02%	0.003%
80	11.471	3146	3151	3158	rBV4	622	824	0.09%	0.012%
81	11.529	3162	3169	3179	rBV6	4964	7524	0.82%	0.112%
82	11.626	3196	3199	3202	rBV2	310	225	0.02%	0.003%
83	11.745	3230	3236	3243	rVB2	2477	3123	0.34%	0.046%
84	11.809	3243	3256	3282	rBV	414384	728337	79.17%	10.829%
85	11.973	3305	3307	3311	rVB2	362	245	0.03%	0.004%
86	12.076	3337	3339	3341	rBV	250	171	0.02%	0.003%
87	12.189	3362	3374	3404	rBV	370486	636586	69.19%	9.465%
88	12.401	3438	3440	3444	rBV2	266	173	0.02%	0.003%
89	12.571	3490	3493	3495	rBV	234	170	0.02%	0.003%
90	12.938	3604	3607	3609	rBV3	350	200	0.02%	0.003%
91	13.044	3636	3640	3644	rBV	334	297	0.03%	0.004%
92	13.137	3666	3669	3671	rBV	398	178	0.02%	0.003%
93	13.475	3772	3774	3778	rBV2	288	231	0.03%	0.003%
94	13.706	3842	3846	3850	rBV2	512	423	0.05%	0.006%
95	13.754	3858	3861	3865	rBV2	348	276	0.03%	0.004%
96	13.841	3884	3888	3900	rVB7	2876	4197	0.46%	0.062%
97	14.034	3944	3948	3949	rBV	251	177	0.02%	0.003%
98	14.092	3960	3966	3976	rBV2	3876	5003	0.54%	0.074%
99	14.253	4014	4016	4020	rBV2	379	318	0.03%	0.005%
100	14.330	4033	4040	4052	rBV5	2909	4363	0.47%	0.065%




Sum of corrected areas: 6725978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
Data File : VU053680.D
Acq On : 13 Apr 2023 12:16
Operator : JC/MD
Sample : 02252-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

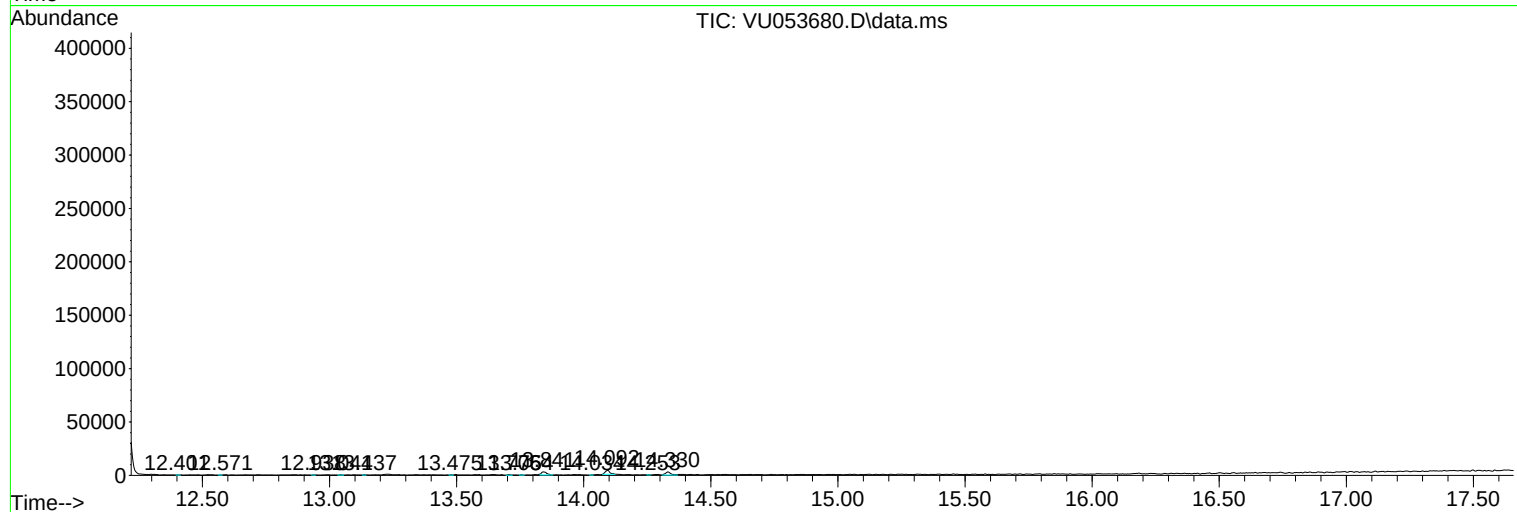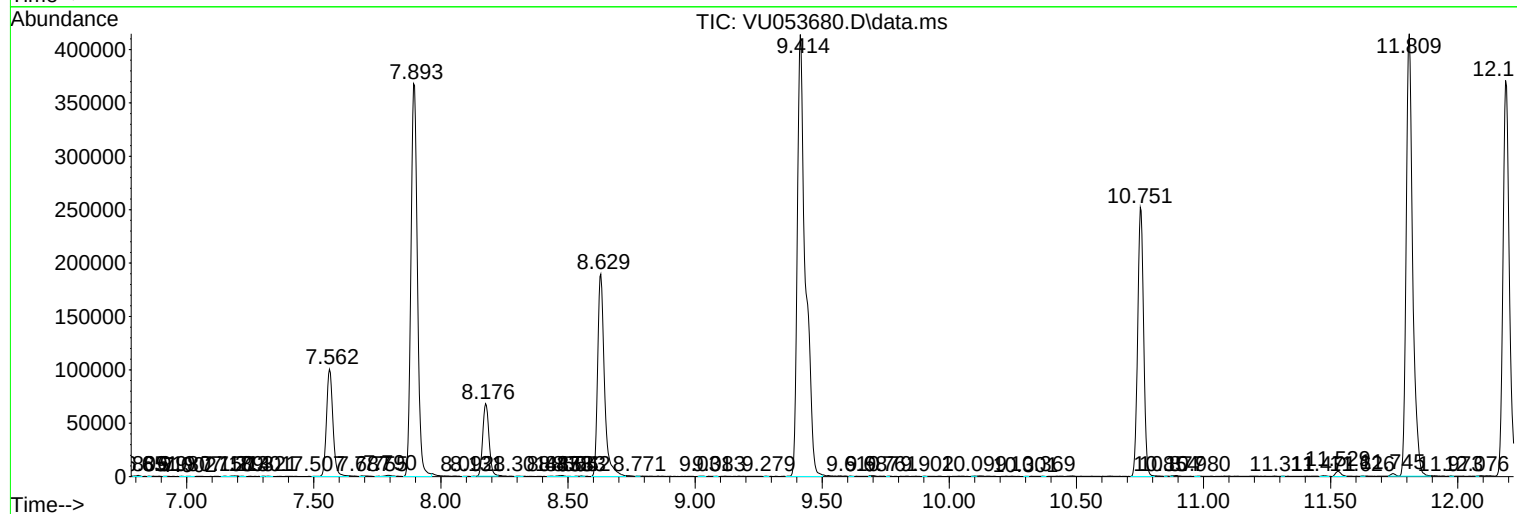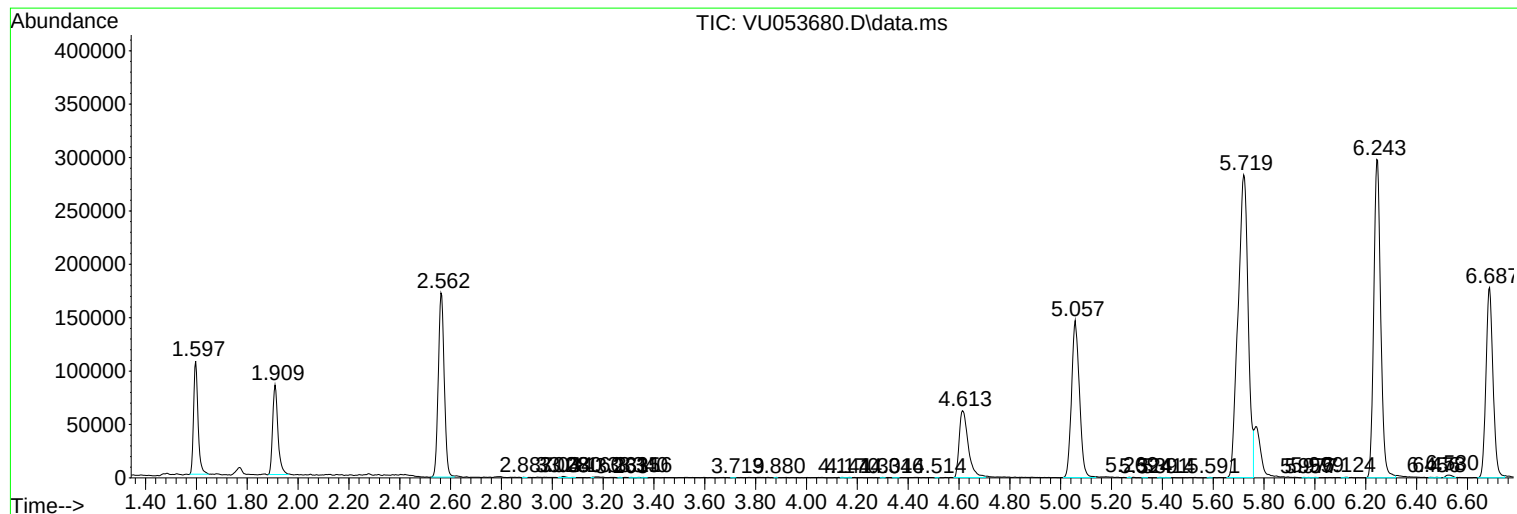

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
Data File : VU053680.D
Acq On : 13 Apr 2023 12:16
Operator : JC/MD
Sample : 02252-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
Data File : VU053680.D
Acq On : 13 Apr 2023 12:16
Operator : JC/MD
Sample : 02252-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------