


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041323\
Data File : VU053676.D
Acq On : 13 Apr 2023 08:59
Operator : JC/MD
Sample : BFB180
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB180

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis
Last Update : Fri Apr 14 01:54:10 2023

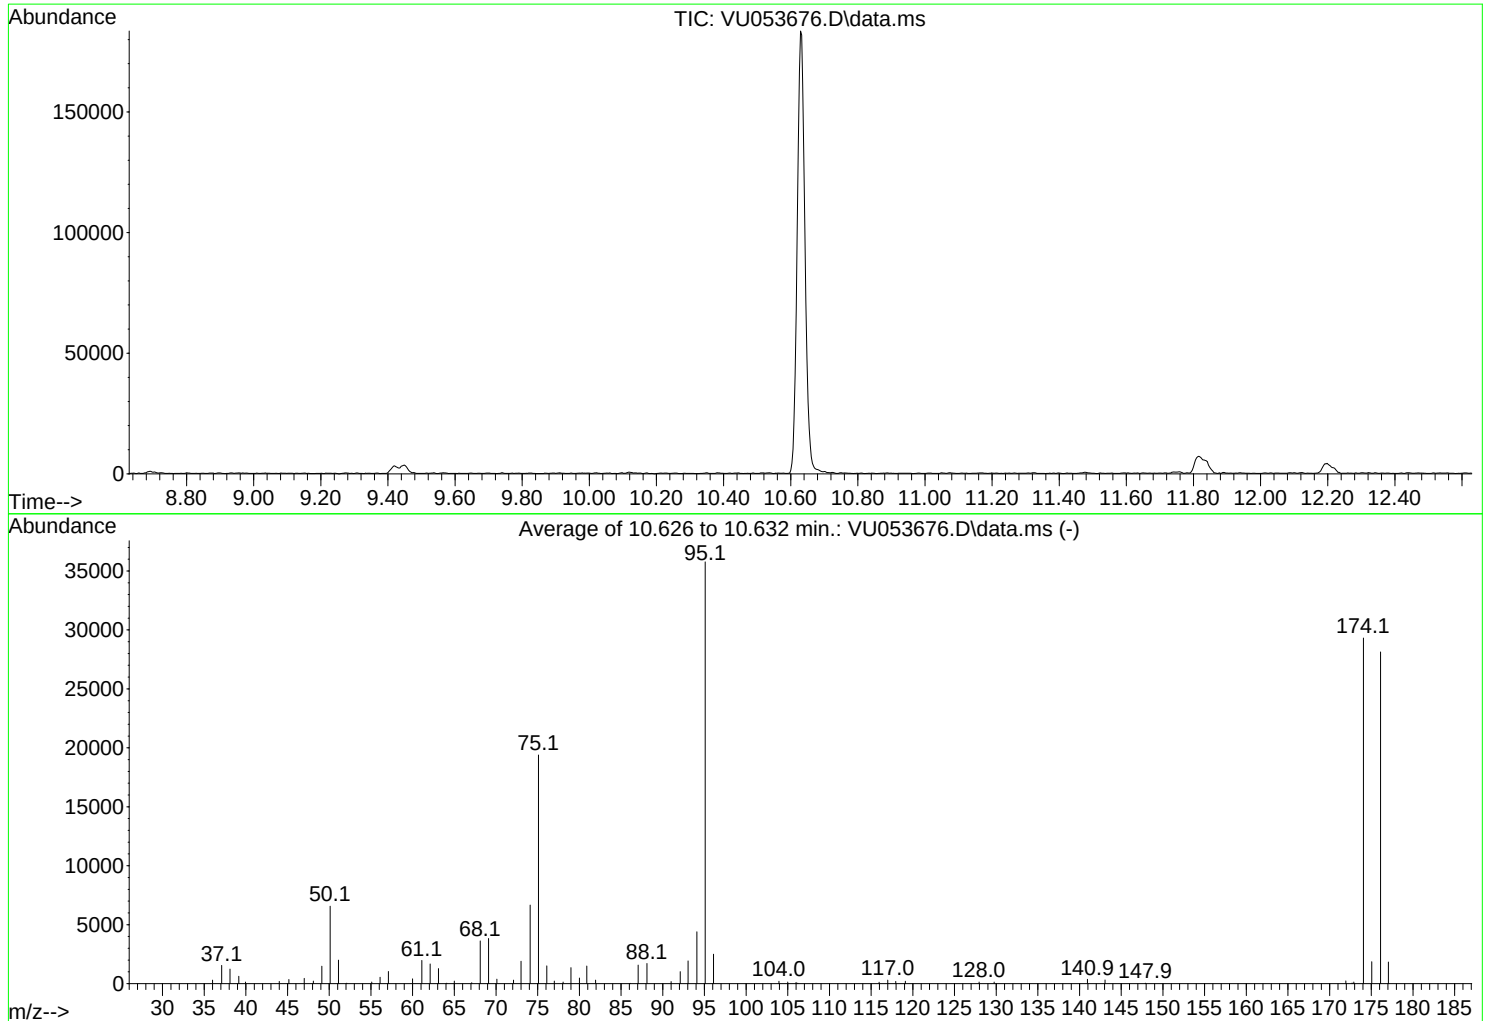

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	6562	PASS
75	95	30	80	54.2	19397	PASS
95	95	100	100	100.0	35776	PASS
96	95	5	9	7.0	2503	PASS
173	174	0.00	2	0.5	140	PASS
174	95	50	120	81.9	29312	PASS
175	174	5	9	6.4	1863	PASS
176	174	95	101	96.0	28131	PASS
177	176	5	9	6.5	1826	PASS

m/z	Abundance
44.00	263.0

Instrument :
MSVOA_U
ClientSampleId :
BFB180

m/z	Abundance
36.00	299.0
37.10	1493.0
38.10	1139.0
39.20	606.0
40.00	130.0
44.10	417.0
45.10	336.0
47.00	398.0
48.10	218.0
49.10	1316.0
50.10	6295.0
51.10	2091.0
55.10	116.0
56.10	528.0
57.10	948.0
59.90	406.0
61.10	1765.0
62.10	1561.0
63.10	1198.0
65.00	207.0
67.10	144.0
68.10	3438.0
69.10	3740.0
70.10	352.0
72.10	257.0
73.00	1782.0
74.10	6126.0
75.10	18368.0
76.10	1419.0
77.00	230.0
78.10	122.0
79.00	1377.0
80.00	418.0
80.90	1500.0
82.00	267.0
87.00	1567.0
88.10	1565.0
91.00	164.0
92.10	846.0
93.10	1763.0
94.10	4194.0
95.10	33976.0
96.10	2465.0
103.90	227.0
105.00	101.0
106.00	178.0
115.90	109.0
117.00	294.0
117.90	189.0
119.10	176.0
128.00	160.0
129.80	152.0
140.90	281.0
143.10	292.0
147.90	110.0
172.00	239.0
172.70	173.0
174.00	26888.0
175.00	1810.0
176.10	25952.0
177.00	1743.0

Instrument :
MSVOA_U
ClientSampleId :
BFB180

m/z	Abundance
36.00	326.0
37.10	1602.0
38.10	1287.0
39.20	655.0
39.90	144.0
44.00	456.0
45.20	374.0
47.00	490.0
48.10	208.0
49.10	1585.0
50.10	6815.0
51.10	2117.0
55.10	152.0
56.10	542.0
57.10	1049.0
60.00	412.0
61.10	2055.0
62.10	1699.0
63.10	1312.0
65.00	234.0
67.10	122.0
68.10	3793.0
69.10	3919.0
70.10	375.0
72.10	317.0
73.00	2009.0
74.10	6921.0
75.10	20264.0
76.10	1525.0
77.00	237.0
78.00	141.0
79.00	1384.0
80.00	505.0
80.90	1559.0
82.00	313.0
86.10	103.0
87.10	1621.0
88.10	1800.0
91.00	202.0
92.10	1033.0
93.10	2056.0
94.10	4573.0
95.10	36720.0
96.10	2619.0
103.90	208.0
105.00	156.0
106.00	148.0
115.90	131.0
117.00	311.0
117.90	196.0
119.10	218.0
127.90	156.0
129.70	132.0
141.00	364.0
143.00	300.0
171.90	251.0
172.90	175.0
174.00	30288.0
175.10	1902.0
176.10	29072.0
177.00	1876.0

Instrument :
MSVOA_U
ClientSampleId :
BFB180

m/z	Abundance
36.00	288.0
37.10	1533.0
38.10	1298.0
39.10	616.0
39.90	149.0
44.00	482.0
45.20	354.0
47.00	451.0
48.10	212.0
49.10	1534.0
50.10	6576.0
51.10	1770.0
52.10	114.0
55.10	161.0
56.10	554.0
57.10	1091.0
60.10	412.0
61.10	2079.0
62.10	1751.0
63.10	1302.0
64.10	132.0
65.00	205.0
68.10	3663.0
69.10	3819.0
70.10	403.0
72.10	309.0
73.00	1908.0
74.10	6938.0
75.10	19560.0
76.10	1590.0
77.00	178.0
78.00	156.0
79.00	1320.0
80.00	520.0
80.90	1408.0
81.90	314.0
87.10	1530.0
88.10	1757.0
91.00	183.0
92.10	1173.0
93.00	1974.0
94.10	4411.0
95.10	36632.0
96.10	2426.0
104.00	174.0
105.00	137.0
106.20	108.0
116.00	132.0
117.00	278.0
118.00	204.0
119.10	220.0
127.90	105.0
129.70	114.0
141.00	447.0
143.00	337.0
172.00	209.0
172.90	245.0
174.10	30760.0
175.10	1878.0
176.10	29368.0
177.10	1860.0

Instrument :
MSVOA_U
ClientSampleId :
BFB180