


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041421\
 Data File : VU043082.D
 Acq On : 14 Apr 2021 09:15
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
 Title : SW846 8260
 Last Update : Mon Apr 12 13:17:29 2021

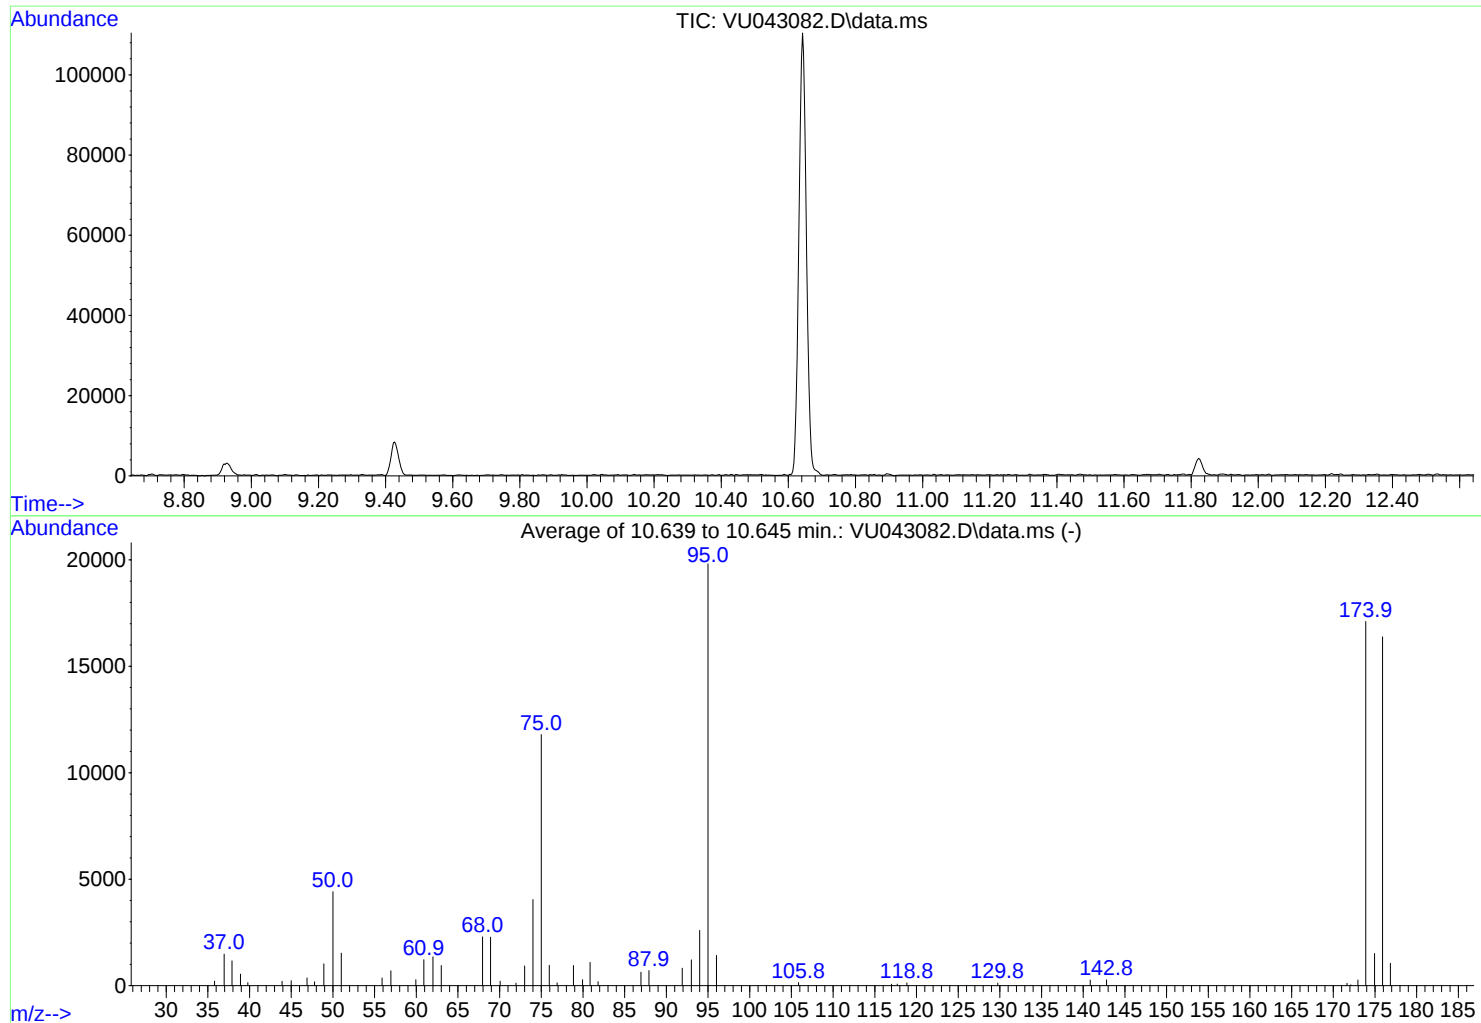

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	4415	PASS
75	95	30	60	59.5	11792	PASS
95	95	100	100	100.0	19813	PASS
96	95	5	9	7.2	1418	PASS
173	174	0.00	2	1.5	260	PASS
174	95	50	100	86.3	17107	PASS
175	174	5	9	8.8	1509	PASS
176	174	95	101	95.8	16383	PASS
177	176	5	9	6.4	1049	PASS