

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048073.D
 Acq On : 14 Apr 2022 21:07
 Operator : SY/MD
 Sample : N2345-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Apr 15 05:27:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 15 05:02:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	294192	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	316754	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	153628	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	87997	41.248	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.500%
7) Chloroethane-d5	1.916	69	82351	48.955	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.920%
11) 1,1-Dichloroethene-d2	2.568	63	119458	30.605	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.220%
21) 2-Butanone-d5	4.623	46	192508	105.131	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.130%
24) Chloroform-d	5.067	84	193730	49.630	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.260%
26) 1,2-Dichloroethane-d4	5.703	65	127012	53.052	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.100%
32) Benzene-d6	5.729	84	377557	47.370	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.740%
36) 1,2-Dichloropropane-d6	6.694	67	128073	52.322	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.640%
41) Toluene-d8	7.899	98	326981	42.107	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.220%
43) trans-1,3-Dichloroprop...	8.179	79	51721	41.707	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.420%
47) 2-Hexanone-d5	8.632	63	129887	90.644	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.640%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	206478	49.152	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.300%
66) 1,2-Dichlorobenzene-d4	12.195	152	145392	53.195	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.380%
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	5532	3.246	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048073.D
Acq On : 14 Apr 2022 21:07
Operator : SY/MD
Sample : N2345-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Apr 15 05:27:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 15 05:02:53 2022
Response via : Initial Calibration

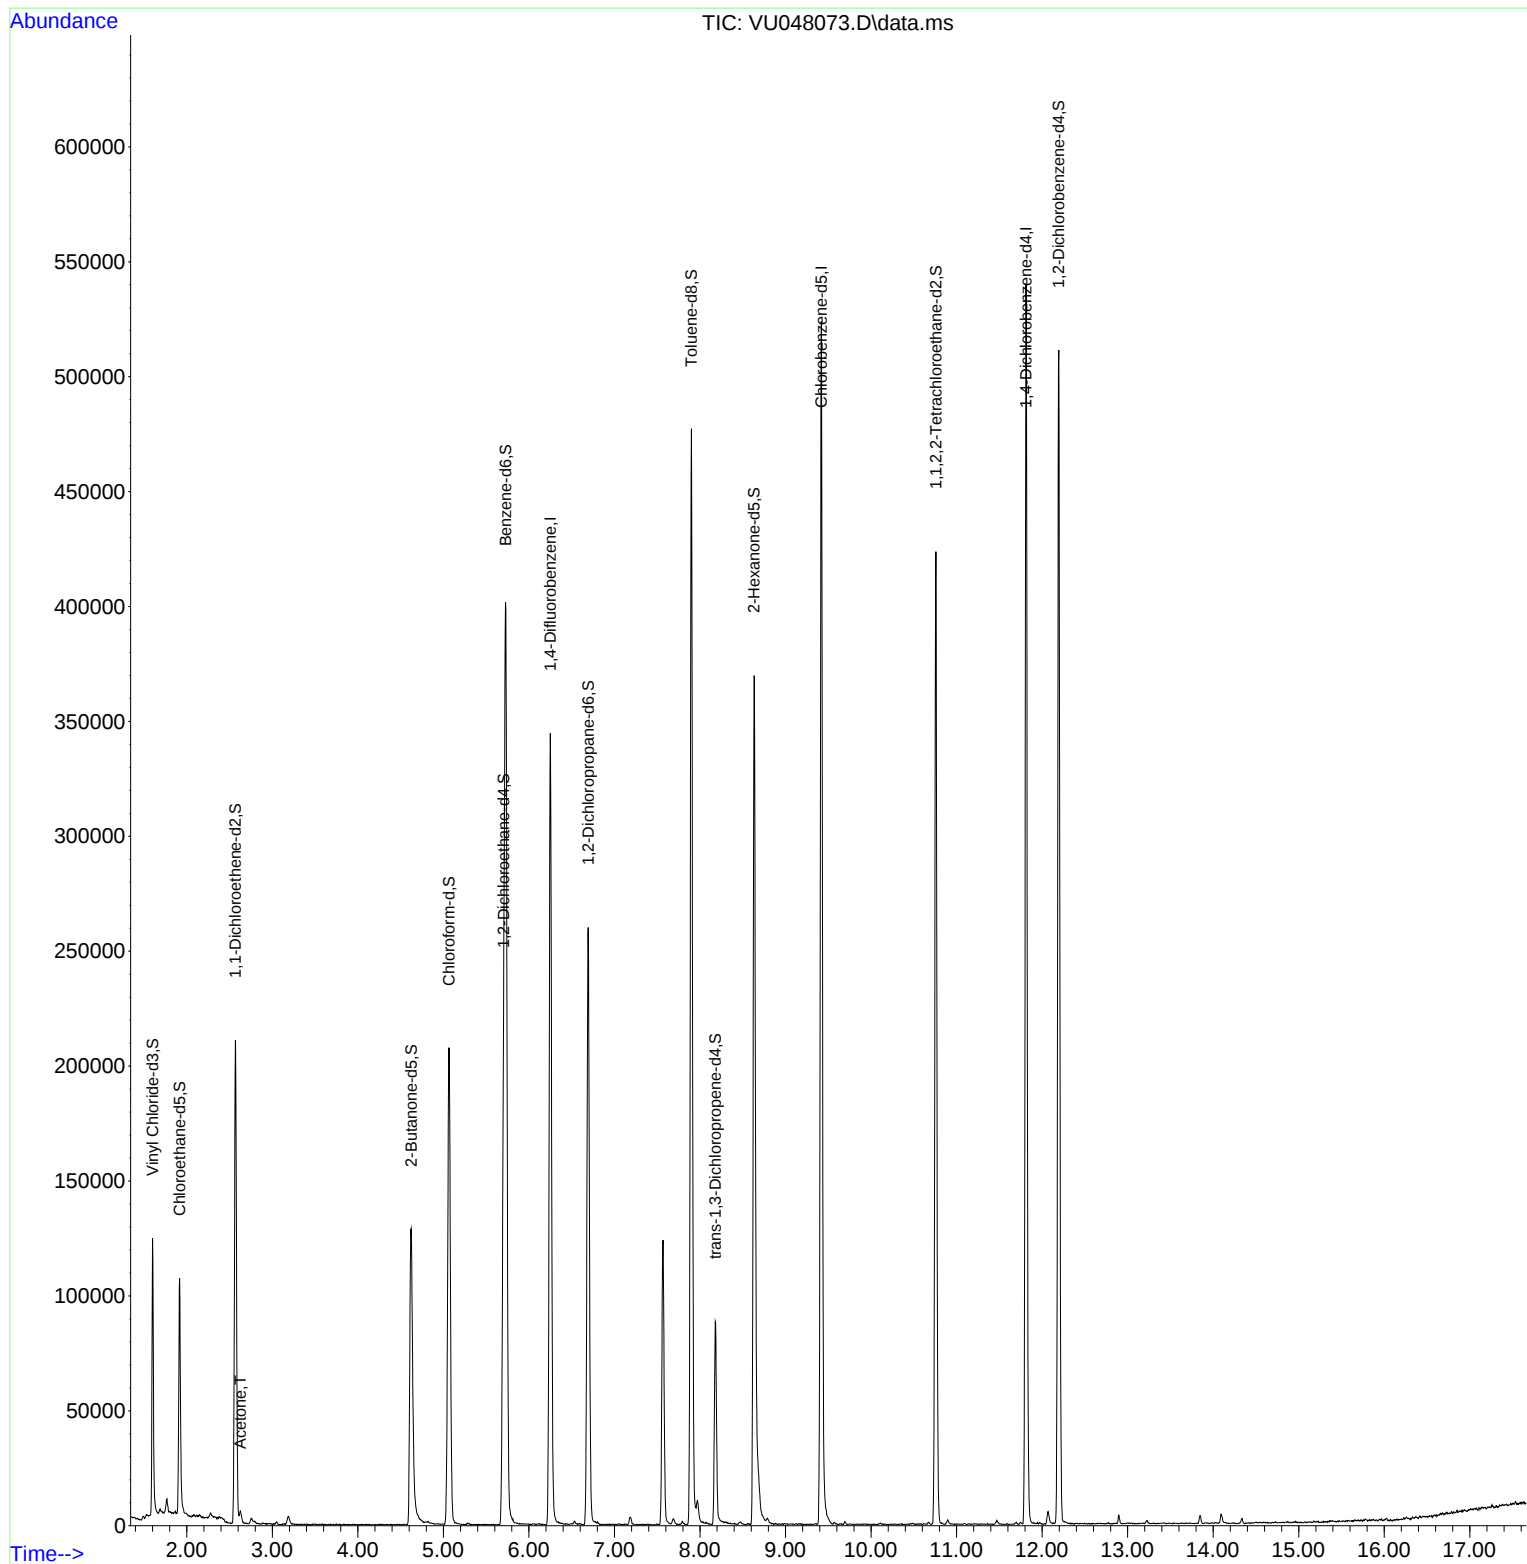

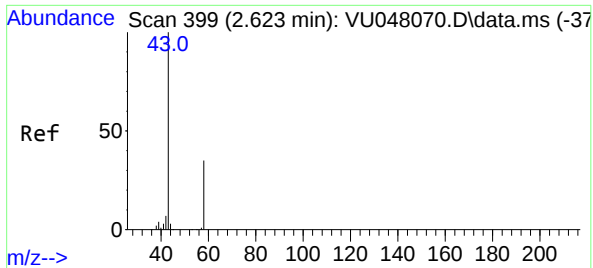

#13
Acetone
Concen: 3.246 ug/L
RT: 2.626 min Scan# 40
Delta R.T. 0.003 min
Lab File: VU048073.D
Acq: 14 Apr 2022 21:07

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

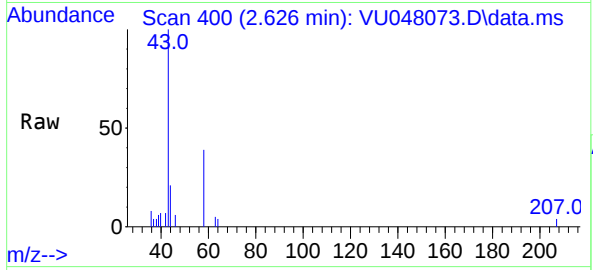

Tgt Ion: 43 Resp: 5532
Ion Ratio Lower Upper
43 100
58 33.8 0.0 70.0

