

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048045.D
 Acq On : 14 Apr 2022 10:15
 Operator : SY/MD
 Sample : VU0414WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	95	rBV	154424	180737	14.38%	1.810%
2	1.765	125	132	140	rBV4	7036	10715	0.85%	0.107%
3	1.916	170	179	201	rVB	124193	175346	13.95%	1.756%
4	2.491	356	358	362	rVB3	396	224	0.02%	0.002%
5	2.568	370	382	402	rBV	264819	435092	34.61%	4.358%
6	2.787	445	450	451	rBV2	560	374	0.03%	0.004%
7	2.867	472	475	479	rBV2	317	197	0.02%	0.002%
8	2.948	496	500	503	rBV2	486	345	0.03%	0.003%
9	3.044	522	530	540	rBV6	1306	2385	0.19%	0.024%
10	3.147	558	562	565	rBV	259	228	0.02%	0.002%
11	3.366	624	630	633	rBV2	207	266	0.02%	0.003%
12	3.491	665	669	674	rBV2	238	234	0.02%	0.002%
13	3.536	679	683	687	rVB2	214	203	0.02%	0.002%
14	3.584	696	698	703	rVB2	359	214	0.02%	0.002%
15	3.617	703	708	710	rBV2	242	258	0.02%	0.003%
16	3.813	762	769	774	rBV2	220	359	0.03%	0.004%
17	3.993	822	825	830	rVB2	325	263	0.02%	0.003%
18	4.086	848	854	859	rBV2	356	454	0.04%	0.005%
19	4.131	859	868	873	rVB2	250	372	0.03%	0.004%
20	4.166	876	879	885	rBV2	196	240	0.02%	0.002%
21	4.311	919	924	927	rBV2	280	338	0.03%	0.003%
22	4.411	949	955	958	rBV2	266	331	0.03%	0.003%
23	4.620	1008	1020	1050	rBV	134256	326540	25.98%	3.270%
24	4.835	1084	1087	1089	rBV2	293	199	0.02%	0.002%
25	5.067	1142	1159	1183	rBV	228413	504700	40.15%	5.055%
26	5.227	1205	1209	1211	rBV2	335	254	0.02%	0.003%
27	5.559	1306	1312	1319	rVB3	434	548	0.04%	0.005%
28	5.729	1343	1365	1399	rVV2	461279	1257071	100.00%	12.590%
29	6.038	1456	1461	1463	rBV2	418	367	0.03%	0.004%
30	6.054	1464	1466	1470	rVB2	429	200	0.02%	0.002%
31	6.076	1470	1473	1478	rBV3	369	301	0.02%	0.003%
32	6.108	1478	1483	1489	rBV2	423	502	0.04%	0.005%
33	6.250	1513	1527	1549	rBV	359956	690872	54.96%	6.919%
34	6.488	1598	1601	1604	rBV3	261	196	0.02%	0.002%
35	6.530	1608	1614	1623	rBV5	1766	2813	0.22%	0.028%
36	6.584	1627	1631	1636	rVB3	497	534	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048045.D
 Acq On : 14 Apr 2022 10:15
 Operator : SY/MD
 Sample : VU0414WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1650	1665	1688	rBV	288867	571192	45.44%	5.721%
38	6.800	1696	1698	1701	rBV3	369	292	0.02%	0.003%
39	7.034	1768	1771	1773	rBV2	505	252	0.02%	0.003%
40	7.102	1789	1792	1796	rVB	245	200	0.02%	0.002%
41	7.186	1807	1818	1828	rBV5	3381	6400	0.51%	0.064%
42	7.227	1829	1831	1837	rVB3	279	236	0.02%	0.002%
43	7.568	1922	1937	1959	rBV	149763	263038	20.92%	2.634%
44	7.665	1964	1967	1968	rVV2	549	359	0.03%	0.004%
45	7.690	1968	1975	1984	rVV3	2672	4581	0.36%	0.046%
46	7.726	1984	1986	1992	rVB3	429	302	0.02%	0.003%
47	7.796	2000	2008	2015	rBV3	1667	2170	0.17%	0.022%
48	7.899	2026	2040	2056	rBV	566930	984114	78.29%	9.856%
49	8.115	2104	2107	2111	rVB2	447	301	0.02%	0.003%
50	8.182	2116	2128	2141	rBV	103262	177202	14.10%	1.775%
51	8.269	2152	2155	2159	rBV3	820	655	0.05%	0.007%
52	8.372	2183	2187	2190	rBV4	476	419	0.03%	0.004%
53	8.462	2210	2215	2218	rBV3	373	487	0.04%	0.005%
54	8.507	2227	2229	2233	rVB2	400	240	0.02%	0.002%
55	8.632	2256	2268	2300	rBV	395553	739464	58.82%	7.406%
56	9.131	2420	2423	2426	rBV2	274	199	0.02%	0.002%
57	9.163	2429	2433	2436	rVV2	477	439	0.03%	0.004%
58	9.420	2497	2513	2551	rBV	554908	942757	75.00%	9.442%
59	9.555	2551	2555	2558	rVV4	424	366	0.03%	0.004%
60	9.578	2558	2562	2565	rVB2	610	483	0.04%	0.005%
61	9.620	2571	2575	2578	rBV	356	287	0.02%	0.003%
62	9.639	2578	2581	2582	rBV	345	214	0.02%	0.002%
63	9.687	2590	2596	2597	rBV	786	569	0.05%	0.006%
64	9.964	2679	2682	2684	rBV2	376	249	0.02%	0.002%
65	10.021	2695	2700	2704	rBV3	321	366	0.03%	0.004%
66	10.102	2720	2725	2726	rBV2	621	417	0.03%	0.004%
67	10.304	2785	2788	2790	rBV	391	306	0.02%	0.003%
68	10.349	2797	2802	2807	rBV2	237	310	0.02%	0.003%
69	10.378	2807	2811	2815	rVB3	268	231	0.02%	0.002%
70	10.533	2858	2859	2865	rVB2	353	263	0.02%	0.003%
71	10.562	2865	2868	2870	rBV	280	233	0.02%	0.002%
72	10.674	2896	2903	2911	rBV4	1454	2275	0.18%	0.023%
73	10.758	2915	2929	2955	rVB	437407	714563	56.84%	7.157%
74	11.034	3012	3015	3018	rBV	317	248	0.02%	0.002%
75	11.089	3027	3032	3036	rBV2	506	581	0.05%	0.006%
76	11.137	3042	3047	3050	rBV3	266	248	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048045.D
 Acq On : 14 Apr 2022 10:15
 Operator : SY/MD
 Sample : VU0414WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.398	3122	3128	3130	rBV2	420	390	0.03%	0.004%
78	11.462	3140	3148	3149	rBV3	1840	1534	0.12%	0.015%
79	11.693	3213	3220	3221	rBV2	710	608	0.05%	0.006%
80	11.748	3231	3237	3244	rVB4	1394	2030	0.16%	0.020%
81	11.812	3244	3257	3274	rBV	595117	961777	76.51%	9.632%
82	11.906	3283	3286	3290	rBV3	487	349	0.03%	0.003%
83	11.941	3294	3297	3301	rBV3	459	387	0.03%	0.004%
84	11.976	3306	3308	3314	rVB3	1531	974	0.08%	0.010%
85	12.047	3327	3330	3334	rVV2	298	216	0.02%	0.002%
86	12.144	3354	3360	3362	rBV2	473	502	0.04%	0.005%
87	12.195	3362	3376	3401	rVV	589209	967110	76.93%	9.686%
88	12.539	3479	3483	3487	rBV2	393	367	0.03%	0.004%
89	12.980	3617	3620	3624	rBV2	450	338	0.03%	0.003%
90	13.005	3624	3628	3630	rBV	555	437	0.03%	0.004%
91	13.224	3692	3696	3704	rVB4	1716	2156	0.17%	0.022%
92	13.520	3785	3788	3790	rBV	303	216	0.02%	0.002%
93	13.793	3870	3873	3877	rVB3	354	230	0.02%	0.002%
94	13.848	3881	3890	3900	rVB4	4314	6550	0.52%	0.066%
95	14.031	3945	3947	3950	rBV2	331	221	0.02%	0.002%
96	14.092	3956	3966	3977	rBV	11237	18244	1.45%	0.183%
97	14.333	4032	4041	4054	rVB4	4408	7435	0.59%	0.074%
98	14.436	4071	4073	4077	rBV2	448	330	0.03%	0.003%
99	14.555	4107	4110	4111	rBV	416	243	0.02%	0.002%
100	14.629	4131	4133	4139	rBV4	374	363	0.03%	0.004%



Sum of corrected areas: 9984787

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048045.D
Acq On : 14 Apr 2022 10:15
Operator : SY/MD
Sample : VU0414WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK092

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

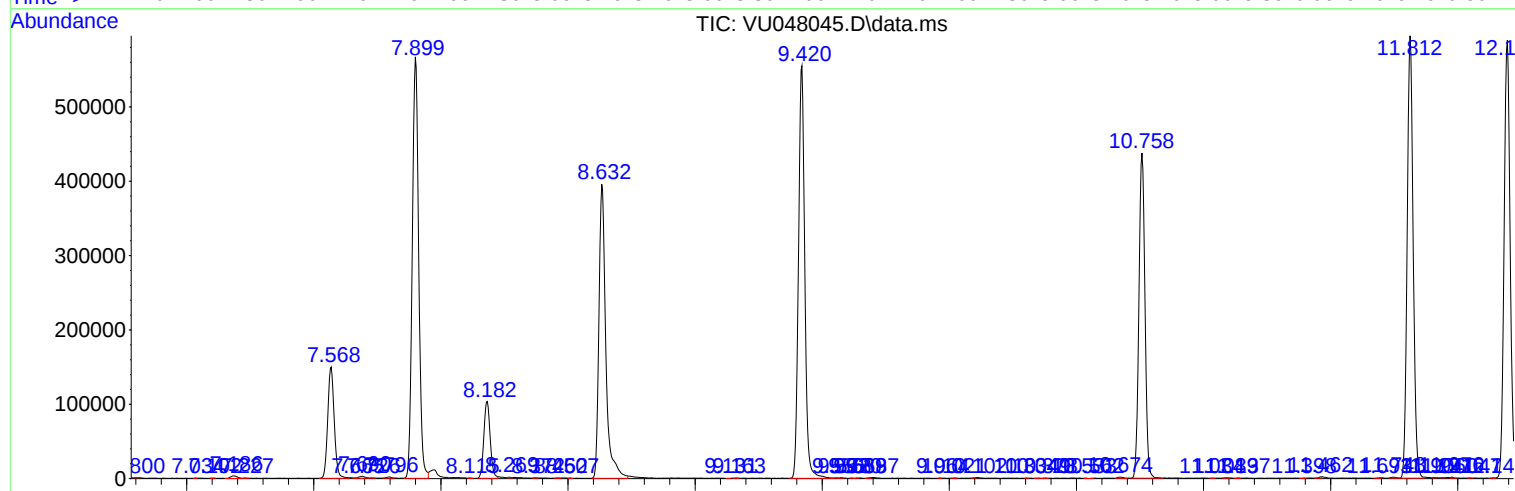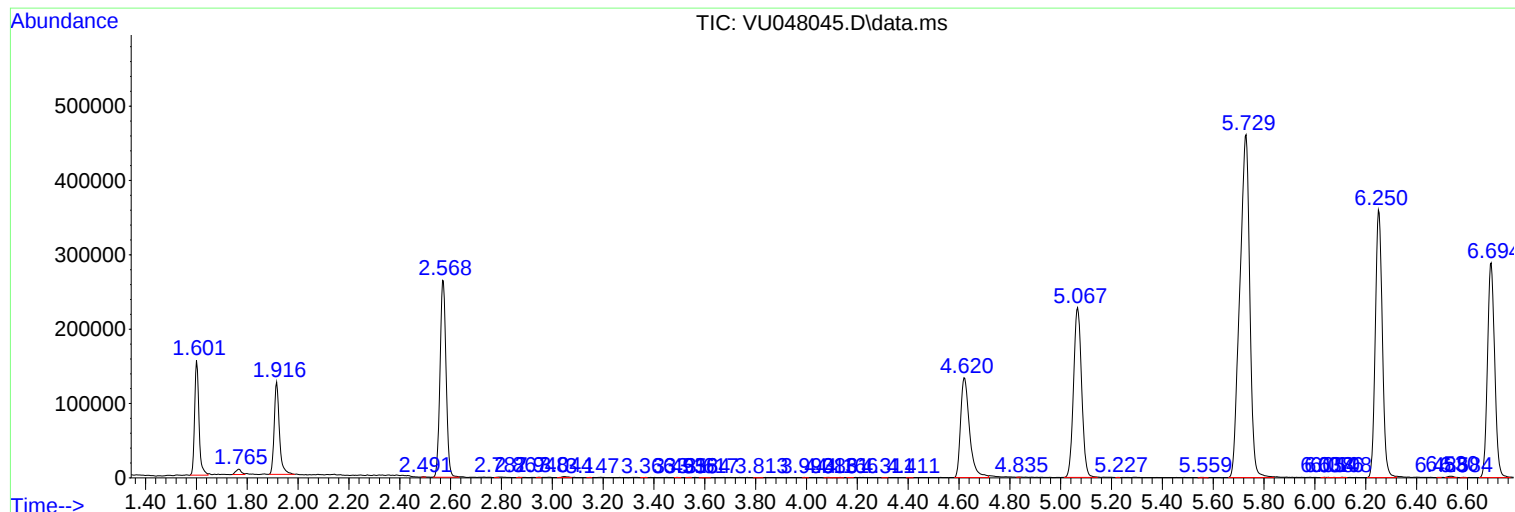

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048045.D
Acq On : 14 Apr 2022 10:15
Operator : SY/MD
Sample : VU0414WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK092

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048045.D
Acq On : 14 Apr 2022 10:15
Operator : SY/MD
Sample : VU0414WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK092

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------