

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048049.D
 Acq On : 14 Apr 2022 11:48
 Operator : SY/MD
 Sample : N2345-14DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rBV	136857	159508	3.39%	0.942%
2	1.915	170	179	203	rVB	114300	166377	3.53%	0.983%
3	2.571	369	383	402	rVV	243834	399088	8.48%	2.357%
4	2.780	444	448	449	rBV2	305	232	0.00%	0.001%
5	2.925	488	493	497	rVB3	392	378	0.01%	0.002%
6	3.050	520	532	544	rBV4	2532	4656	0.10%	0.028%
7	3.124	553	555	560	rVB2	307	231	0.00%	0.001%
8	3.173	566	570	571	rVV3	341	224	0.00%	0.001%
9	3.195	575	577	583	rVB2	481	455	0.01%	0.003%
10	3.263	595	598	601	rVB2	341	244	0.01%	0.001%
11	3.292	601	607	609	rBV2	352	329	0.01%	0.002%
12	3.330	613	619	622	rVB3	366	367	0.01%	0.002%
13	3.353	622	626	630	rBV3	292	335	0.01%	0.002%
14	3.542	681	685	690	rBV2	294	235	0.00%	0.001%
15	3.690	728	731	734	rVB	377	212	0.00%	0.001%
16	3.706	734	736	741	rVB	344	221	0.00%	0.001%
17	3.790	760	762	767	rVB2	269	216	0.00%	0.001%
18	3.841	775	778	782	rVB3	266	240	0.01%	0.001%
19	3.976	817	820	825	rBV2	355	330	0.01%	0.002%
20	4.089	852	855	859	rBV2	315	226	0.00%	0.001%
21	4.243	898	903	910	rVB2	261	303	0.01%	0.002%
22	4.620	1007	1020	1056	rBV	133249	324762	6.90%	1.918%
23	4.902	1105	1108	1114	rVB2	398	288	0.01%	0.002%
24	4.931	1114	1117	1122	rBV2	303	255	0.01%	0.002%
25	5.066	1142	1159	1187	rBV	217981	479846	10.19%	2.834%
26	5.198	1198	1200	1207	rVB3	338	251	0.01%	0.001%
27	5.292	1224	1229	1233	rBV3	382	477	0.01%	0.003%
28	5.333	1238	1242	1247	rVV2	351	291	0.01%	0.002%
29	5.517	1297	1299	1309	rVB3	273	285	0.01%	0.002%
30	5.729	1341	1365	1370	rBV2	448324	1143998	24.30%	6.757%
31	5.777	1372	1380	1416	rVB	1431071	2833454	60.18%	16.737%
32	6.044	1460	1463	1467	rVB3	575	396	0.01%	0.002%
33	6.063	1467	1469	1474	rVB2	335	218	0.00%	0.001%
34	6.111	1480	1484	1486	rBV4	723	542	0.01%	0.003%
35	6.163	1497	1500	1503	rVB	357	211	0.00%	0.001%
36	6.250	1512	1527	1554	rBV	398955	757511	16.09%	4.474%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048049.D
 Acq On : 14 Apr 2022 11:48
 Operator : SY/MD
 Sample : N2345-14DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.529	1608	1614	1616	rBV5	1277	1420	0.03%	0.008%
38	6.693	1650	1665	1683	rBV	282401	549343	11.67%	3.245%
39	6.800	1695	1698	1707	rVB5	894	979	0.02%	0.006%
40	6.877	1718	1722	1726	rVB2	300	224	0.00%	0.001%
41	6.992	1751	1758	1761	rBV2	231	331	0.01%	0.002%
42	7.050	1774	1776	1781	rVB3	463	345	0.01%	0.002%
43	7.134	1800	1802	1806	rVB	447	289	0.01%	0.002%
44	7.182	1806	1817	1828	rBV4	3522	6728	0.14%	0.040%
45	7.568	1923	1937	1959	rBV	140678	249648	5.30%	1.475%
46	7.664	1964	1967	1968	rBV3	406	226	0.00%	0.001%
47	7.684	1968	1973	1975	rBV2	1663	1546	0.03%	0.009%
48	7.787	2001	2005	2009	rBV3	388	372	0.01%	0.002%
49	7.809	2009	2012	2014	rVB2	383	221	0.00%	0.001%
50	7.899	2019	2040	2056	rBV	550034	946660	20.11%	5.592%
51	8.179	2116	2127	2146	rBV	98465	169126	3.59%	0.999%
52	8.426	2200	2204	2210	rVB3	422	480	0.01%	0.003%
53	8.455	2210	2213	2216	rBV2	394	380	0.01%	0.002%
54	8.632	2253	2268	2298	rBV	390422	714387	15.17%	4.220%
55	8.857	2334	2338	2342	rBV2	460	563	0.01%	0.003%
56	9.137	2423	2425	2432	rBV2	366	472	0.01%	0.003%
57	9.169	2432	2435	2438	rVB2	442	283	0.01%	0.002%
58	9.192	2438	2442	2446	rBV2	327	348	0.01%	0.002%
59	9.446	2498	2521	2566	rBV2	2258630	4707966	100.00%	27.809%
60	9.684	2592	2595	2596	rBV	905	516	0.01%	0.003%
61	9.758	2613	2618	2623	rVB3	533	644	0.01%	0.004%
62	9.803	2629	2632	2634	rVV	293	236	0.01%	0.001%
63	9.880	2651	2656	2660	rVB2	390	416	0.01%	0.002%
64	9.906	2660	2664	2665	rBV	305	210	0.00%	0.001%
65	9.931	2665	2672	2677	rVV2	268	333	0.01%	0.002%
66	9.989	2686	2690	2695	rBV3	332	309	0.01%	0.002%
67	10.057	2707	2711	2714	rBV2	393	307	0.01%	0.002%
68	10.095	2720	2723	2725	rBV2	387	260	0.01%	0.002%
69	10.176	2745	2748	2753	rVB2	313	268	0.01%	0.002%
70	10.266	2772	2776	2779	rBV3	324	302	0.01%	0.002%
71	10.552	2861	2865	2870	rBV3	257	267	0.01%	0.002%
72	10.610	2880	2883	2889	rBV	322	354	0.01%	0.002%
73	10.671	2897	2902	2908	rVB4	1276	1601	0.03%	0.009%
74	10.758	2916	2929	2948	rBV	424982	688277	14.62%	4.065%
75	10.854	2957	2959	2961	rBV	382	237	0.01%	0.001%
76	10.867	2961	2963	2966	rVV2	313	249	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048049.D
 Acq On : 14 Apr 2022 11:48
 Operator : SY/MD
 Sample : N2345-14DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.031	3011	3014	3017	rVB	329	215	0.00%	0.001%
78	11.066	3021	3025	3029	rBV3	302	280	0.01%	0.002%
79	11.092	3029	3033	3038	rVB2	473	414	0.01%	0.002%
80	11.114	3038	3040	3044	rBV2	388	303	0.01%	0.002%
81	11.185	3055	3062	3066	rVB2	347	469	0.01%	0.003%
82	11.465	3141	3149	3158	rVV8	1408	2564	0.05%	0.015%
83	11.584	3182	3186	3187	rBV	392	214	0.00%	0.001%
84	11.626	3196	3199	3201	rBV	362	224	0.00%	0.001%
85	11.690	3212	3219	3227	rBV3	730	1039	0.02%	0.006%
86	11.748	3227	3237	3245	rBV3	21037	34582	0.73%	0.204%
87	11.815	3245	3258	3261	rBV	687325	1075995	22.85%	6.356%
88	11.915	3287	3289	3293	rBV4	525	318	0.01%	0.002%
89	12.005	3314	3317	3322	rVB4	433	335	0.01%	0.002%
90	12.079	3336	3340	3342	rBV3	284	225	0.00%	0.001%
91	12.198	3362	3377	3398	rBV3	638094	1448986	30.78%	8.559%
92	12.307	3408	3411	3415	rVB2	663	483	0.01%	0.003%
93	12.561	3485	3490	3496	rBV4	526	663	0.01%	0.004%
94	12.732	3540	3543	3547	rBV2	441	317	0.01%	0.002%
95	13.044	3637	3640	3642	rBV	519	379	0.01%	0.002%
96	13.060	3642	3645	3647	rVV2	517	361	0.01%	0.002%
97	13.844	3879	3889	3905	rBV2	19607	32053	0.68%	0.189%
98	14.098	3964	3968	3980	rVB3	1037	1756	0.04%	0.010%
99	14.333	4035	4041	4052	rVB5	1919	2507	0.05%	0.015%
100	15.648	4448	4450	4455	rVB3	929	741	0.02%	0.004%




Sum of corrected areas: 16929738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048049.D
Acq On : 14 Apr 2022 11:48
Operator : SY/MD
Sample : N2345-14DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J94DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

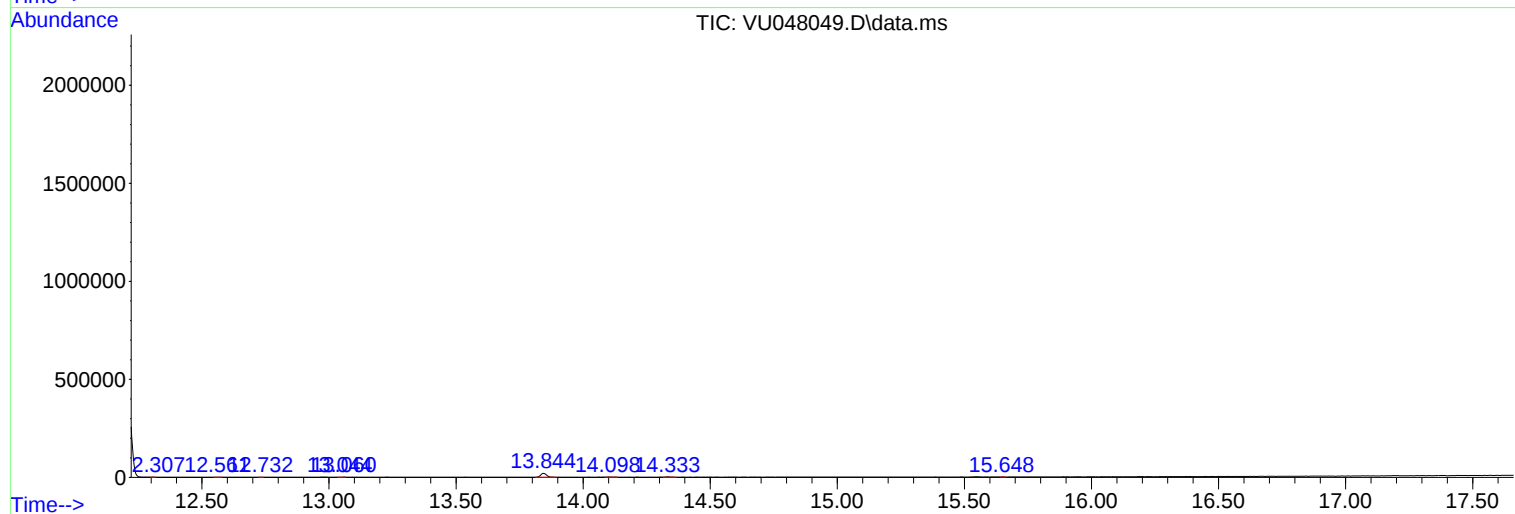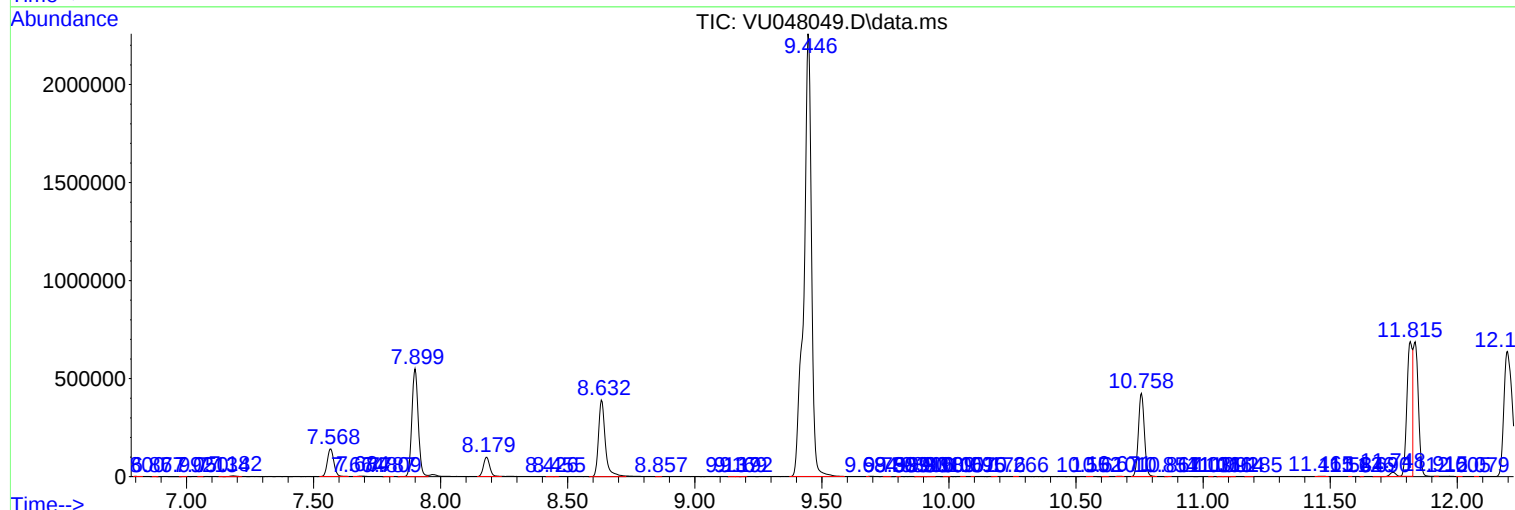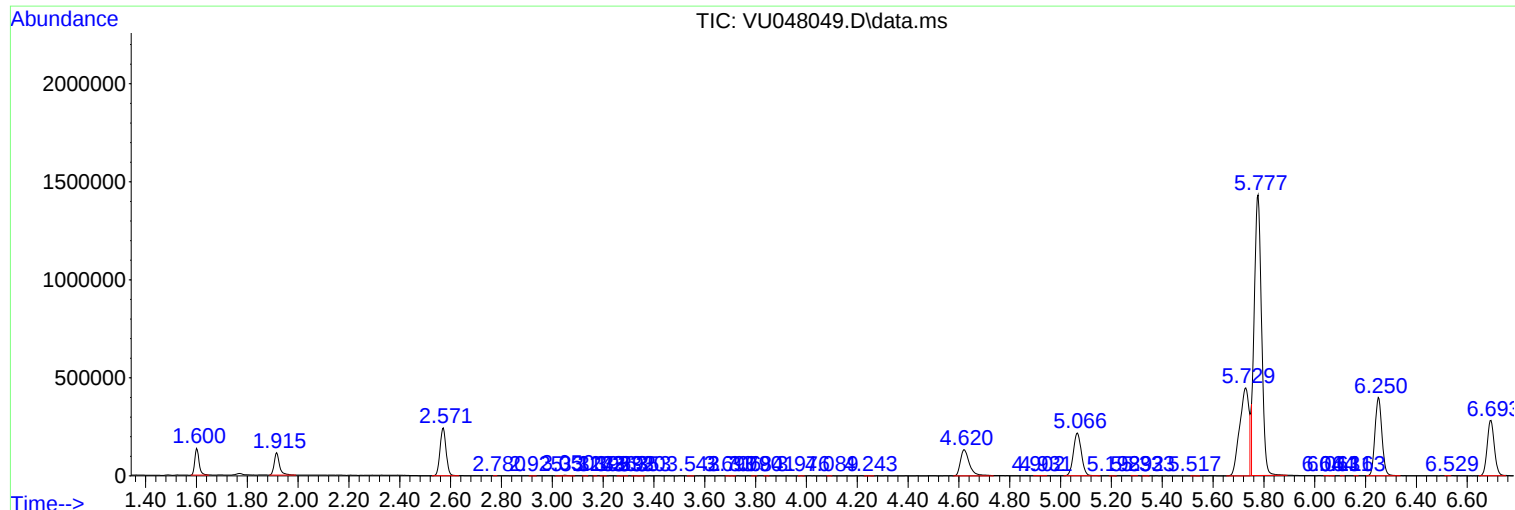

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048049.D
Acq On : 14 Apr 2022 11:48
Operator : SY/MD
Sample : N2345-14DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J94DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048049.D
Acq On : 14 Apr 2022 11:48
Operator : SY/MD
Sample : N2345-14DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J94DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc