

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048054.D
 Acq On : 14 Apr 2022 13:39
 Operator : SY/MD
 Sample : N2386-15DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J39DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rVB	138998	159912	11.94%	1.500%
2	1.916	170	179	202	rBV	117628	165986	12.39%	1.557%
3	2.568	370	382	397	rBV	245385	400100	29.88%	3.752%
4	2.691	417	420	425	rVV4	318	314	0.02%	0.003%
5	2.793	447	452	459	rVB4	847	932	0.07%	0.009%
6	2.835	463	465	473	rVB3	343	348	0.03%	0.003%
7	2.961	497	504	505	rBV2	355	432	0.03%	0.004%
8	3.051	521	532	544	rBV2	3154	5720	0.43%	0.054%
9	3.182	567	573	574	rBV3	777	685	0.05%	0.006%
10	3.285	601	605	610	rBV2	251	283	0.02%	0.003%
11	3.314	610	614	617	rVV3	385	299	0.02%	0.003%
12	3.359	624	628	629	rVV	364	225	0.02%	0.002%
13	3.398	638	640	647	rVB2	207	241	0.02%	0.002%
14	3.465	658	661	665	rBV	331	289	0.02%	0.003%
15	3.517	674	677	681	rVB	322	248	0.02%	0.002%
16	3.674	721	726	731	rVB3	234	217	0.02%	0.002%
17	3.768	751	755	760	rBV2	283	284	0.02%	0.003%
18	3.806	764	767	771	rVB3	327	259	0.02%	0.002%
19	3.835	771	776	780	rBV2	222	211	0.02%	0.002%
20	4.086	849	854	857	rBV2	290	326	0.02%	0.003%
21	4.166	873	879	881	rBV2	228	295	0.02%	0.003%
22	4.263	906	909	913	rVB	366	241	0.02%	0.002%
23	4.330	925	930	935	rBV3	357	398	0.03%	0.004%
24	4.430	957	961	966	rBV2	366	382	0.03%	0.004%
25	4.465	966	972	975	rBV2	160	222	0.02%	0.002%
26	4.514	984	987	992	rVB2	269	244	0.02%	0.002%
27	4.562	995	1002	1006	rBV2	312	481	0.04%	0.005%
28	4.623	1007	1021	1062	rBV	138242	341875	25.53%	3.206%
29	5.067	1142	1159	1190	rVV	228788	500199	37.35%	4.691%
30	5.282	1222	1226	1229	rBV3	581	604	0.05%	0.006%
31	5.346	1241	1246	1250	rBV3	344	337	0.03%	0.003%
32	5.391	1256	1260	1263	rBV	408	307	0.02%	0.003%
33	5.456	1276	1280	1283	rBV	223	211	0.02%	0.002%
34	5.530	1299	1303	1309	rVB	513	445	0.03%	0.004%
35	5.562	1309	1313	1317	rBV2	244	219	0.02%	0.002%
36	5.729	1343	1365	1397	rBV2	459423	1253700	93.62%	11.758%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048054.D
 Acq On : 14 Apr 2022 13:39
 Operator : SY/MD
 Sample : N2386-15DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J39DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.845	1397	1401	1402	rBV2	558	388	0.03%	0.004%
38	5.909	1418	1421	1424	rBV3	369	252	0.02%	0.002%
39	6.005	1449	1451	1457	rBV3	420	383	0.03%	0.004%
40	6.038	1457	1461	1462	rBV3	474	354	0.03%	0.003%
41	6.147	1492	1495	1497	rBV	419	289	0.02%	0.003%
42	6.173	1497	1503	1506	rVV2	250	292	0.02%	0.003%
43	6.250	1511	1527	1560	rBV	392179	752152	56.16%	7.054%
44	6.530	1607	1614	1623	rBV8	1617	2640	0.20%	0.025%
45	6.587	1629	1632	1635	rVB4	361	214	0.02%	0.002%
46	6.600	1635	1636	1645	rVB2	388	401	0.03%	0.004%
47	6.636	1645	1647	1650	rBV2	294	214	0.02%	0.002%
48	6.694	1650	1665	1683	rBV	292673	571306	42.66%	5.358%
49	6.793	1693	1696	1699	rBV4	593	475	0.04%	0.004%
50	6.813	1699	1702	1709	rVB4	1141	1107	0.08%	0.010%
51	6.848	1709	1713	1718	rBV3	376	318	0.02%	0.003%
52	7.044	1770	1774	1776	rBV2	535	428	0.03%	0.004%
53	7.186	1807	1818	1829	rBV3	3759	7196	0.54%	0.067%
54	7.272	1842	1845	1848	rVB2	378	221	0.02%	0.002%
55	7.568	1924	1937	1956	rBV	143677	256271	19.14%	2.403%
56	7.652	1961	1963	1966	rVV2	372	213	0.02%	0.002%
57	7.684	1967	1973	1987	rVV4	2379	4681	0.35%	0.044%
58	7.784	2001	2004	2007	rBV2	443	272	0.02%	0.003%
59	7.899	2025	2040	2055	rBV	559127	962963	71.91%	9.031%
60	8.179	2115	2127	2142	rBV	102178	175497	13.10%	1.646%
61	8.472	2210	2218	2225	rBV4	760	1233	0.09%	0.012%
62	8.552	2240	2243	2245	rBV2	456	232	0.02%	0.002%
63	8.632	2255	2268	2308	rBV	406043	768186	57.36%	7.204%
64	8.793	2316	2318	2321	rVB2	480	267	0.02%	0.003%
65	9.044	2393	2396	2402	rVB3	288	281	0.02%	0.003%
66	9.083	2404	2408	2410	rBV	251	212	0.02%	0.002%
67	9.166	2431	2434	2436	rVB3	529	283	0.02%	0.003%
68	9.230	2450	2454	2457	rVV2	333	239	0.02%	0.002%
69	9.420	2499	2513	2518	rBV	618613	1073226	80.14%	10.065%
70	9.648	2579	2584	2589	rBV4	441	522	0.04%	0.005%
71	9.690	2593	2597	2606	rVB3	1119	1451	0.11%	0.014%
72	9.774	2620	2623	2627	rBV2	308	214	0.02%	0.002%
73	9.893	2655	2660	2664	rVB2	300	264	0.02%	0.002%
74	10.041	2704	2706	2709	rVB2	372	223	0.02%	0.002%
75	10.102	2719	2725	2729	rBV2	342	470	0.04%	0.004%
76	10.201	2751	2756	2758	rBV2	328	259	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048054.D
 Acq On : 14 Apr 2022 13:39
 Operator : SY/MD
 Sample : N2386-15DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J39DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.398	2813	2817	2821	rBV	239	215	0.02%	0.002%
78	10.671	2896	2902	2913	rVB5	1525	2035	0.15%	0.019%
79	10.758	2916	2929	2948	rBV	448512	724622	54.11%	6.796%
80	10.864	2958	2962	2966	rBV3	570	470	0.04%	0.004%
81	10.893	2966	2971	2976	rVV3	1132	1343	0.10%	0.013%
82	11.086	3028	3031	3038	rVB2	309	287	0.02%	0.003%
83	11.195	3061	3065	3068	rBV2	324	269	0.02%	0.003%
84	11.462	3144	3148	3149	rBV2	826	549	0.04%	0.005%
85	11.558	3175	3178	3185	rBV	501	484	0.04%	0.005%
86	11.700	3219	3222	3225	rVB	786	501	0.04%	0.005%
87	11.748	3228	3237	3244	rBV2	9399	13823	1.03%	0.130%
88	11.812	3244	3257	3280	rVV	654959	1097320	81.94%	10.291%
89	12.034	3321	3326	3330	rBV2	366	463	0.03%	0.004%
90	12.195	3362	3376	3398	rBV3	642302	1339207	100.00%	12.560%
91	12.459	3456	3458	3466	rVB2	471	555	0.04%	0.005%
92	12.780	3551	3558	3560	rBV3	507	495	0.04%	0.005%
93	12.941	3605	3608	3610	rBV	268	211	0.02%	0.002%
94	12.973	3615	3618	3623	rVV3	1139	1059	0.08%	0.010%
95	12.996	3623	3625	3629	rVB3	507	241	0.02%	0.002%
96	13.279	3709	3713	3716	rBV2	315	314	0.02%	0.003%
97	13.844	3879	3889	3904	rVB3	28840	46331	3.46%	0.435%
98	14.089	3962	3965	3967	rBV	894	610	0.05%	0.006%
99	14.333	4034	4041	4050	rVB2	5182	7500	0.56%	0.070%
100	15.282	4334	4336	4339	rBV2	525	255	0.02%	0.002%




Sum of corrected areas: 10662719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048054.D
Acq On : 14 Apr 2022 13:39
Operator : SY/MD
Sample : N2386-15DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

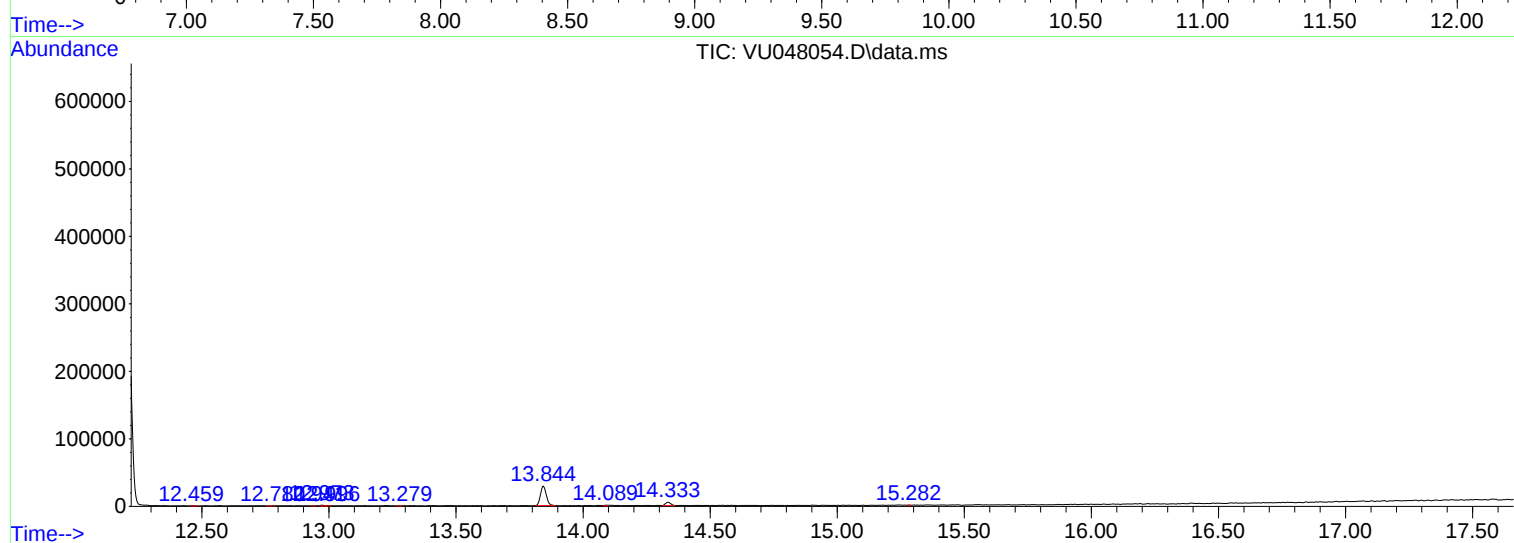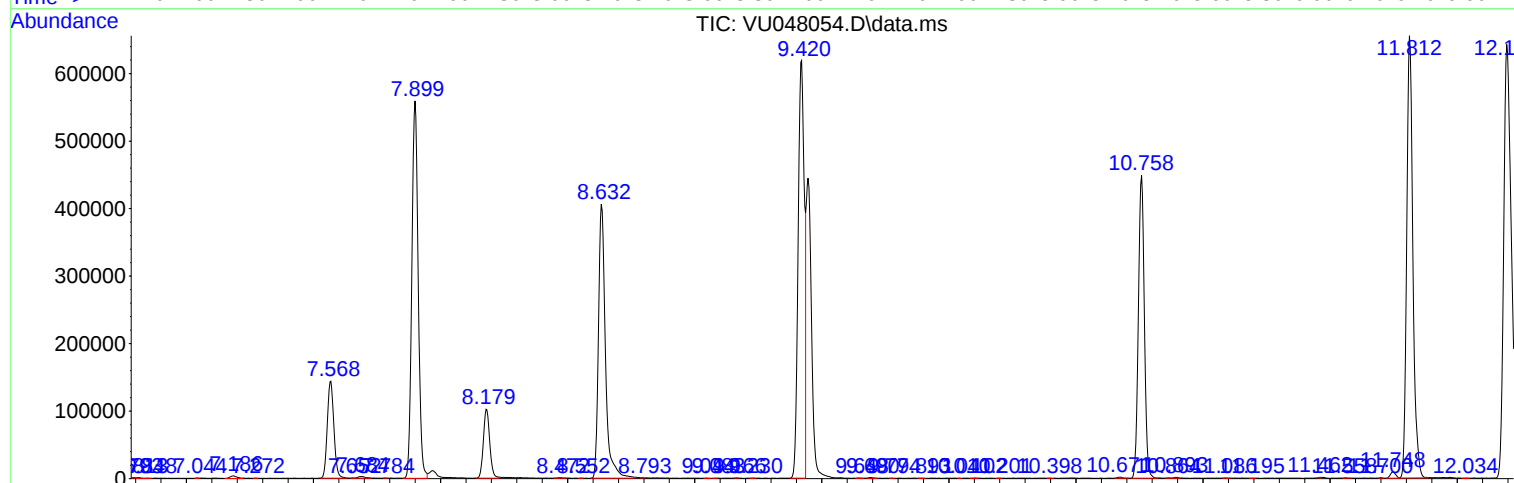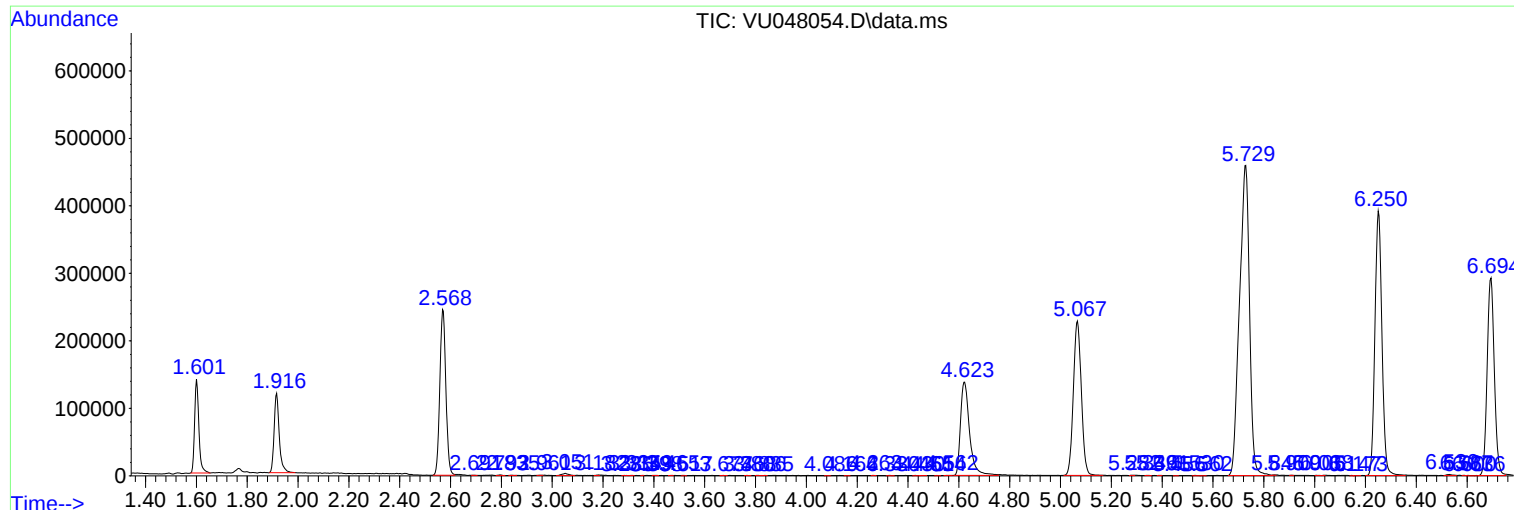

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048054.D
Acq On : 14 Apr 2022 13:39
Operator : SY/MD
Sample : N2386-15DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048054.D
Acq On : 14 Apr 2022 13:39
Operator : SY/MD
Sample : N2386-15DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------