

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048059.D
 Acq On : 14 Apr 2022 15:35
 Operator : SY/MD
 Sample : N2387-01 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rBV	129770	149289	4.42%	1.131%
2	1.916	171	179	198	rVB	110907	153833	4.55%	1.166%
3	2.568	369	382	398	rBV	230099	380157	11.25%	2.881%
4	2.755	429	440	459	rBV	8118	16770	0.50%	0.127%
5	2.867	473	475	477	rBV	308	183	0.01%	0.001%
6	2.948	497	500	501	rBV	417	219	0.01%	0.002%
7	3.051	520	532	543	rBV3	6180	12507	0.37%	0.095%
8	3.189	564	575	579	rBV2	2246	3770	0.11%	0.029%
9	3.247	591	593	596	rVB3	269	162	0.00%	0.001%
10	3.333	614	620	626	rBV2	294	524	0.02%	0.004%
11	3.446	653	655	659	rVB2	301	200	0.01%	0.002%
12	3.481	662	666	670	rBV	212	212	0.01%	0.002%
13	3.504	670	673	676	rVB	359	188	0.01%	0.001%
14	3.674	722	726	730	rBV2	232	175	0.01%	0.001%
15	3.948	808	811	815	rVB2	245	169	0.01%	0.001%
16	4.025	830	835	837	rBV2	247	271	0.01%	0.002%
17	4.044	837	841	844	rVV2	245	225	0.01%	0.002%
18	4.063	844	847	852	rVB2	172	173	0.01%	0.001%
19	4.182	881	884	886	rBV	228	179	0.01%	0.001%
20	4.263	902	909	911	rBV2	159	165	0.00%	0.001%
21	4.623	1008	1021	1056	rBV	128651	319730	9.46%	2.423%
22	4.919	1109	1113	1116	rBV2	335	274	0.01%	0.002%
23	5.067	1142	1159	1180	rBV	216905	472989	14.00%	3.585%
24	5.218	1204	1206	1209	rVV3	318	211	0.01%	0.002%
25	5.288	1223	1228	1229	rBV	708	588	0.02%	0.004%
26	5.346	1243	1246	1250	rVB2	334	232	0.01%	0.002%
27	5.729	1342	1365	1397	rBV2	430589	1201667	35.56%	9.107%
28	5.874	1408	1410	1413	rVB3	391	180	0.01%	0.001%
29	5.980	1438	1443	1446	rBV3	306	330	0.01%	0.003%
30	6.079	1470	1474	1477	rBV3	234	249	0.01%	0.002%
31	6.111	1481	1484	1490	rBV4	459	489	0.01%	0.004%
32	6.250	1512	1527	1556	rBV	374661	716030	21.19%	5.427%
33	6.529	1608	1614	1628	rVB4	1414	2318	0.07%	0.018%
34	6.693	1649	1665	1686	rBV	275531	540271	15.99%	4.095%
35	6.809	1696	1701	1704	rBV3	909	832	0.02%	0.006%
36	6.886	1722	1725	1731	rVB2	316	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048059.D
 Acq On : 14 Apr 2022 15:35
 Operator : SY/MD
 Sample : N2387-01 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.931	1735	1739	1741	rBV2	274	206	0.01%	0.002%
38	6.944	1741	1743	1746	rVV2	268	170	0.01%	0.001%
39	7.047	1771	1775	1780	rBV2	260	292	0.01%	0.002%
40	7.182	1809	1817	1833	rVB2	3463	6334	0.19%	0.048%
41	7.398	1878	1884	1886	rBV	382	331	0.01%	0.003%
42	7.568	1924	1937	1955	rBV	137279	242739	7.18%	1.840%
43	7.652	1961	1963	1966	rBV4	341	203	0.01%	0.002%
44	7.690	1967	1975	1983	rVB7	2022	3316	0.10%	0.025%
45	7.793	2004	2007	2010	rBV2	310	244	0.01%	0.002%
46	7.899	2026	2040	2056	rBV	521997	907592	26.86%	6.879%
47	8.082	2095	2097	2104	rVB4	547	404	0.01%	0.003%
48	8.179	2115	2127	2145	rBV	96514	167636	4.96%	1.270%
49	8.336	2173	2176	2179	rVB2	387	195	0.01%	0.001%
50	8.475	2210	2219	2228	rVB3	1005	1911	0.06%	0.014%
51	8.552	2239	2243	2245	rBV	396	203	0.01%	0.002%
52	8.632	2252	2268	2302	rBV	387896	728261	21.55%	5.519%
53	9.005	2382	2384	2387	rBV3	269	178	0.01%	0.001%
54	9.140	2423	2426	2428	rBV2	352	258	0.01%	0.002%
55	9.160	2428	2432	2435	rVV2	406	330	0.01%	0.003%
56	9.301	2473	2476	2480	rVB2	387	289	0.01%	0.002%
57	9.330	2480	2485	2488	rVB3	268	243	0.01%	0.002%
58	9.353	2488	2492	2497	rBV	356	313	0.01%	0.002%
59	9.417	2497	2512	2550	rBV2	571003	1113223	32.95%	8.437%
60	9.571	2557	2560	2566	rVB2	1022	898	0.03%	0.007%
61	9.693	2590	2598	2600	rBV3	944	1100	0.03%	0.008%
62	9.838	2641	2643	2646	rVB2	298	168	0.00%	0.001%
63	9.857	2646	2649	2652	rBV2	285	254	0.01%	0.002%
64	9.925	2667	2670	2674	rBV2	254	255	0.01%	0.002%
65	10.018	2696	2699	2707	rBV3	222	247	0.01%	0.002%
66	10.098	2718	2724	2735	rBV4	1356	2309	0.07%	0.017%
67	10.160	2738	2743	2747	rVB2	290	304	0.01%	0.002%
68	10.192	2749	2753	2755	rBV2	279	213	0.01%	0.002%
69	10.446	2826	2832	2834	rBV2	221	219	0.01%	0.002%
70	10.484	2842	2844	2853	rVB	276	396	0.01%	0.003%
71	10.613	2881	2884	2886	rBV	349	215	0.01%	0.002%
72	10.671	2893	2902	2909	rBV5	1420	1982	0.06%	0.015%
73	10.758	2916	2929	2948	rVB	427095	691705	20.47%	5.242%
74	10.825	2948	2950	2957	rVB	437	280	0.01%	0.002%
75	10.870	2961	2964	2967	rBV3	426	370	0.01%	0.003%
76	10.899	2967	2973	2976	rBV3	976	1198	0.04%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048059.D
 Acq On : 14 Apr 2022 15:35
 Operator : SY/MD
 Sample : N2387-01 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.047	3016	3019	3022	rVB	282	172	0.01%	0.001%
78	11.298	3093	3097	3102	rBV3	441	425	0.01%	0.003%
79	11.327	3102	3106	3110	rBV3	247	247	0.01%	0.002%
80	11.369	3115	3119	3121	rBV2	204	164	0.00%	0.001%
81	11.436	3136	3140	3141	rBV	333	225	0.01%	0.002%
82	11.465	3141	3149	3161	rVB7	1445	2635	0.08%	0.020%
83	11.668	3208	3212	3214	rBV2	193	171	0.01%	0.001%
84	11.748	3225	3237	3246	rBV	88324	142866	4.23%	1.083%
85	11.835	3246	3264	3288	rVB2	1540985	3379032	100.00%	25.609%
86	12.057	3329	3333	3334	rBV2	502	363	0.01%	0.003%
87	12.069	3334	3337	3341	rVV5	1033	937	0.03%	0.007%
88	12.198	3362	3377	3401	rBV2	683241	1591305	47.09%	12.060%
89	12.323	3414	3416	3423	rVB3	542	464	0.01%	0.004%
90	12.394	3434	3438	3440	rBV3	508	457	0.01%	0.003%
91	12.430	3447	3449	3451	rBV2	403	235	0.01%	0.002%
92	12.783	3556	3559	3564	rBV4	387	341	0.01%	0.003%
93	12.857	3578	3582	3583	rBV	462	299	0.01%	0.002%
94	12.873	3585	3587	3589	rBV	275	178	0.01%	0.001%
95	12.976	3616	3619	3622	rBV3	593	421	0.01%	0.003%
96	13.841	3877	3888	3905	rBV	99840	158805	4.70%	1.204%
97	14.333	4031	4041	4059	rBV2	19234	31305	0.93%	0.237%
98	15.330	4346	4351	4353	rBV3	726	742	0.02%	0.006%
99	15.420	4370	4379	4390	rVB3	12347	19313	0.57%	0.146%
100	16.002	4554	4560	4573	rVB5	7391	10514	0.31%	0.080%




Sum of corrected areas: 13194588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048059.D
Acq On : 14 Apr 2022 15:35
Operator : SY/MD
Sample : N2387-01 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

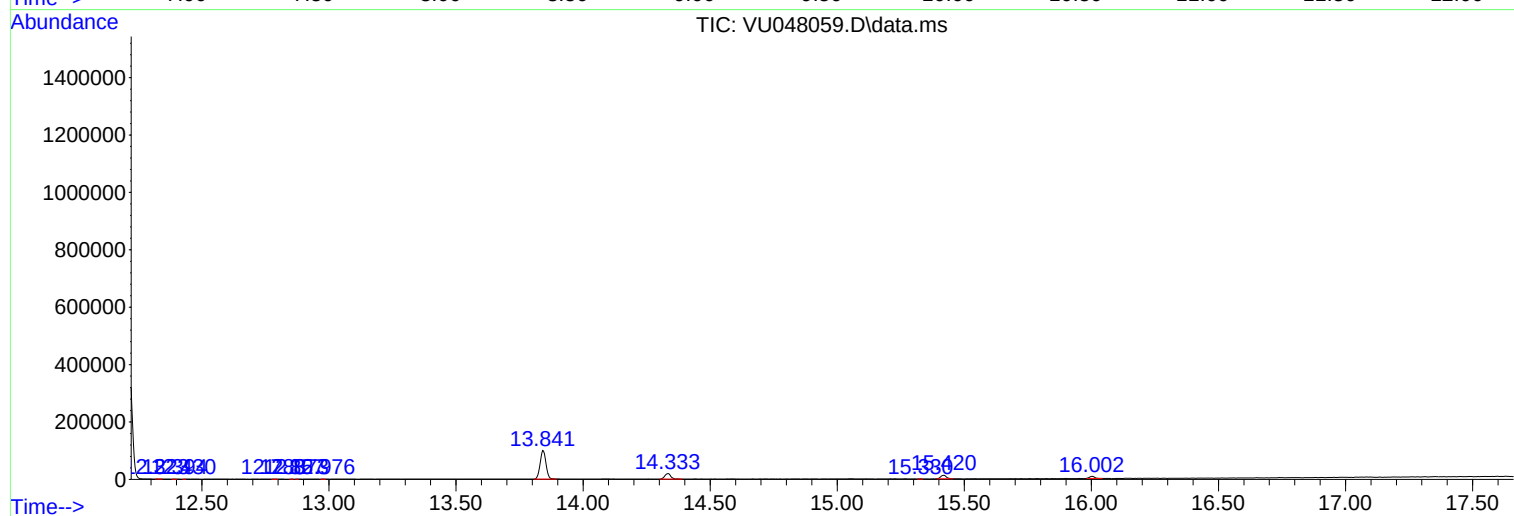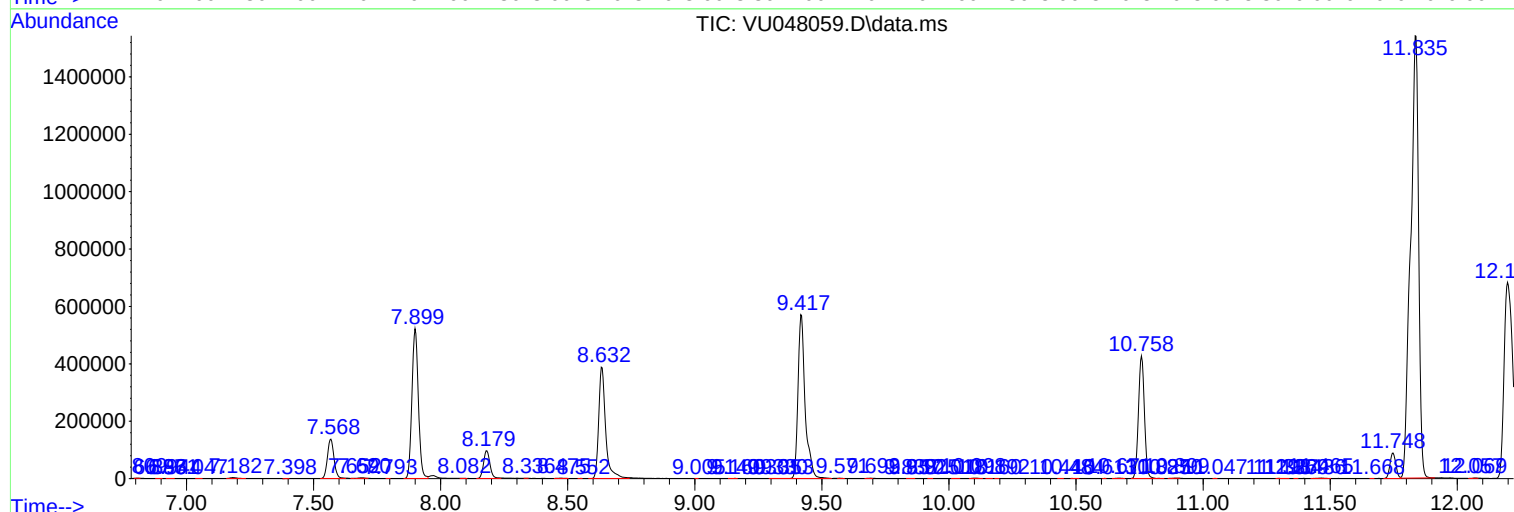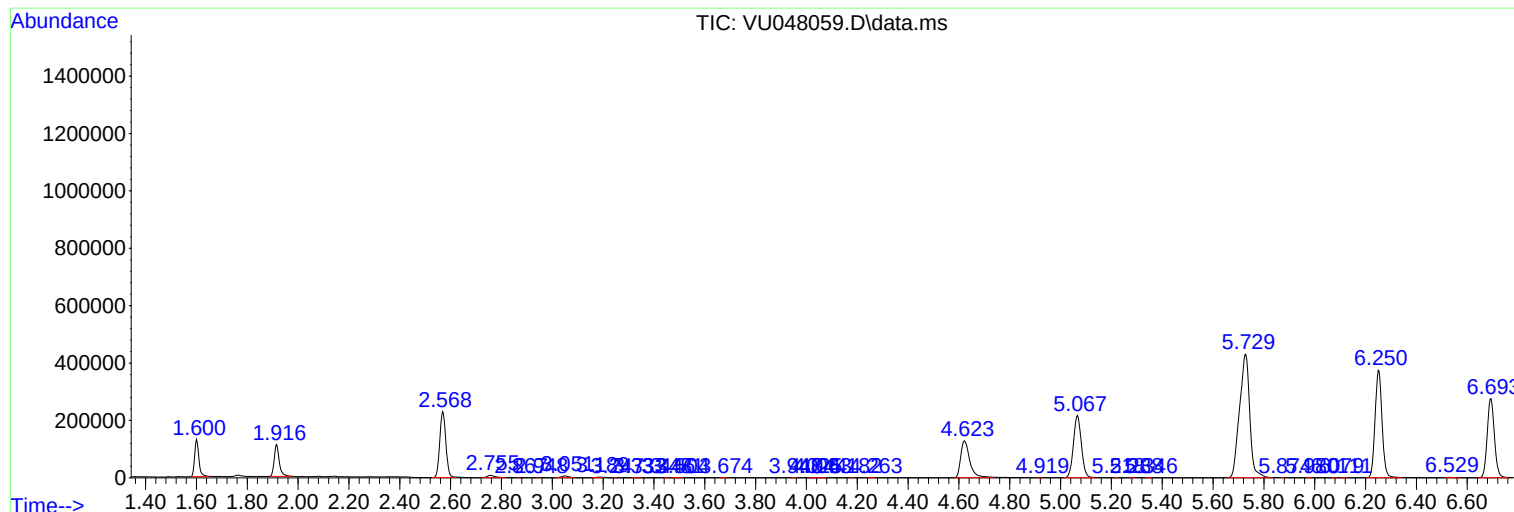

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048059.D
Acq On : 14 Apr 2022 15:35
Operator : SY/MD
Sample : N2387-01 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048059.D
Acq On : 14 Apr 2022 15:35
Operator : SY/MD
Sample : N2387-01 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------