

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048060.D
 Acq On : 14 Apr 2022 15:58
 Operator : SY/MD
 Sample : N2387-02DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J48DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	100	rBV	126573	149730	9.85%	1.436%
2	1.916	170	179	200	rBV	106800	150888	9.93%	1.447%
3	2.568	370	382	399	rBV	226700	372411	24.50%	3.572%
4	2.697	419	422	424	rBV2	361	257	0.02%	0.002%
5	2.851	468	470	474	rVB2	385	244	0.02%	0.002%
6	2.912	483	489	493	rBV2	360	405	0.03%	0.004%
7	2.945	493	499	500	rBV2	312	297	0.02%	0.003%
8	3.051	522	532	543	rVB2	5201	8778	0.58%	0.084%
9	3.192	564	576	586	rVV5	2025	4176	0.27%	0.040%
10	3.237	588	590	594	rVB2	203	153	0.01%	0.001%
11	3.401	638	641	647	rVB3	297	308	0.02%	0.003%
12	3.527	677	680	684	rBV2	267	231	0.02%	0.002%
13	3.565	689	692	694	rBV2	201	151	0.01%	0.001%
14	3.655	717	720	727	rBV2	223	288	0.02%	0.003%
15	3.713	732	738	741	rBV2	259	330	0.02%	0.003%
16	3.787	758	761	762	rBV	344	223	0.01%	0.002%
17	4.295	915	919	922	rBV	185	157	0.01%	0.002%
18	4.420	954	958	962	rBV	138	172	0.01%	0.002%
19	4.520	985	989	991	rBV	210	164	0.01%	0.002%
20	4.623	1007	1021	1050	rBV	130642	317922	20.92%	3.049%
21	5.006	1137	1140	1142	rBV2	256	157	0.01%	0.002%
22	5.067	1142	1159	1182	rVV	215446	467586	30.77%	4.485%
23	5.260	1217	1219	1222	rVB2	329	171	0.01%	0.002%
24	5.295	1222	1230	1238	rBV3	799	1442	0.09%	0.014%
25	5.330	1238	1241	1244	rVV2	300	206	0.01%	0.002%
26	5.350	1244	1247	1252	rVV2	228	209	0.01%	0.002%
27	5.375	1252	1255	1260	rVV	459	368	0.02%	0.004%
28	5.414	1262	1267	1272	rVB3	327	243	0.02%	0.002%
29	5.523	1297	1301	1303	rBV2	391	337	0.02%	0.003%
30	5.584	1317	1320	1323	rVB	365	190	0.01%	0.002%
31	5.729	1342	1365	1373	rBV2	421416	1170209	77.00%	11.224%
32	5.919	1422	1424	1428	rVB2	573	290	0.02%	0.003%
33	6.163	1498	1500	1503	rBV2	462	284	0.02%	0.003%
34	6.250	1512	1527	1558	rBV	367470	701438	46.15%	6.728%
35	6.459	1589	1592	1597	rVB3	598	579	0.04%	0.006%
36	6.485	1597	1600	1602	rBV	435	328	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048060.D
 Acq On : 14 Apr 2022 15:58
 Operator : SY/MD
 Sample : N2387-02DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J48DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.533	1607	1615	1617	rBV5	1107	1363	0.09%	0.013%
38	6.694	1650	1665	1691	rBV	271411	534527	35.17%	5.127%
39	6.806	1694	1700	1701	rBV2	427	413	0.03%	0.004%
40	6.851	1711	1714	1716	rBV2	369	184	0.01%	0.002%
41	6.973	1750	1752	1758	rVB	212	186	0.01%	0.002%
42	7.012	1758	1764	1766	rBV2	214	240	0.02%	0.002%
43	7.054	1770	1777	1780	rBV2	372	491	0.03%	0.005%
44	7.182	1807	1817	1828	rBV3	3029	5295	0.35%	0.051%
45	7.349	1867	1869	1876	rVB2	284	171	0.01%	0.002%
46	7.382	1877	1879	1885	rVB2	235	178	0.01%	0.002%
47	7.478	1906	1909	1911	rBV2	287	168	0.01%	0.002%
48	7.568	1923	1937	1957	rBV	136038	239020	15.73%	2.293%
49	7.690	1962	1975	1983	rVV7	2372	4409	0.29%	0.042%
50	7.764	1993	1998	2001	rBV2	295	330	0.02%	0.003%
51	7.800	2007	2009	2014	rVB3	433	283	0.02%	0.003%
52	7.899	2025	2040	2056	rBV	507955	881804	58.02%	8.458%
53	8.179	2116	2127	2144	rBV	96303	163488	10.76%	1.568%
54	8.401	2194	2196	2201	rVB2	458	312	0.02%	0.003%
55	8.430	2202	2205	2209	rVB4	356	263	0.02%	0.003%
56	8.542	2236	2240	2241	rBV	221	189	0.01%	0.002%
57	8.581	2249	2252	2256	rVB3	320	222	0.01%	0.002%
58	8.632	2256	2268	2298	rBV	383668	728810	47.95%	6.991%
59	9.034	2390	2393	2395	rBV2	301	178	0.01%	0.002%
60	9.166	2430	2434	2436	rBV	403	319	0.02%	0.003%
61	9.221	2449	2451	2453	rBV2	248	152	0.01%	0.001%
62	9.420	2499	2513	2516	rBV	578037	881468	58.00%	8.455%
63	9.610	2569	2572	2574	rBV	279	183	0.01%	0.002%
64	9.697	2592	2599	2605	rBV3	954	1300	0.09%	0.012%
65	9.986	2687	2689	2692	rBV2	231	161	0.01%	0.002%
66	10.076	2714	2717	2719	rBV	362	242	0.02%	0.002%
67	10.105	2722	2726	2728	rVB	388	276	0.02%	0.003%
68	10.346	2799	2801	2806	rVB2	247	181	0.01%	0.002%
69	10.414	2818	2822	2825	rBV	325	251	0.02%	0.002%
70	10.472	2836	2840	2842	rBV2	282	201	0.01%	0.002%
71	10.491	2842	2846	2850	rVV3	444	382	0.03%	0.004%
72	10.510	2850	2852	2861	rVB	276	212	0.01%	0.002%
73	10.671	2895	2902	2911	rVV4	1141	1623	0.11%	0.016%
74	10.758	2916	2929	2948	rBV	427559	694094	45.67%	6.658%
75	10.870	2960	2964	2966	rVB2	604	457	0.03%	0.004%
76	10.890	2966	2970	2972	rBV	884	631	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048060.D
 Acq On : 14 Apr 2022 15:58
 Operator : SY/MD
 Sample : N2387-02DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J48DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.999	3001	3004	3010	rVB4	404	337	0.02%	0.003%
78	11.105	3035	3037	3044	rVB2	321	249	0.02%	0.002%
79	11.173	3054	3058	3063	rVB3	296	298	0.02%	0.003%
80	11.372	3117	3120	3127	rVB2	286	243	0.02%	0.002%
81	11.417	3130	3134	3136	rBV2	275	193	0.01%	0.002%
82	11.455	3143	3146	3147	rBV2	522	275	0.02%	0.003%
83	11.690	3218	3219	3221	rBV2	468	242	0.02%	0.002%
84	11.748	3227	3237	3245	rBV3	19196	29245	1.92%	0.281%
85	11.812	3245	3257	3281	rVB2	636067	1519816	100.00%	14.578%
86	11.947	3294	3299	3302	rBV6	694	693	0.05%	0.007%
87	12.047	3326	3330	3333	rBV	377	330	0.02%	0.003%
88	12.195	3362	3376	3402	rBV3	609895	1304041	85.80%	12.508%
89	12.410	3441	3443	3445	rBV	355	158	0.01%	0.002%
90	12.449	3452	3455	3458	rBV2	416	264	0.02%	0.003%
91	12.597	3498	3501	3504	rBV	296	209	0.01%	0.002%
92	12.835	3571	3575	3578	rBV2	329	260	0.02%	0.002%
93	12.980	3617	3620	3625	rBV2	536	396	0.03%	0.004%
94	13.221	3692	3695	3705	rVB5	856	1028	0.07%	0.010%
95	13.648	3825	3828	3833	rBV2	506	375	0.02%	0.004%
96	13.841	3879	3888	3903	rBV	36618	57917	3.81%	0.556%
97	14.336	4034	4042	4051	rVB4	4313	7008	0.46%	0.067%
98	14.655	4139	4141	4142	rBV4	438	171	0.01%	0.002%
99	15.417	4375	4378	4387	rVB6	1944	2476	0.16%	0.024%
100	16.002	4556	4560	4572	rVB10	2276	3507	0.23%	0.034%




Sum of corrected areas: 10425710

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048060.D
Acq On : 14 Apr 2022 15:58
Operator : SY/MD
Sample : N2387-02DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J48DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

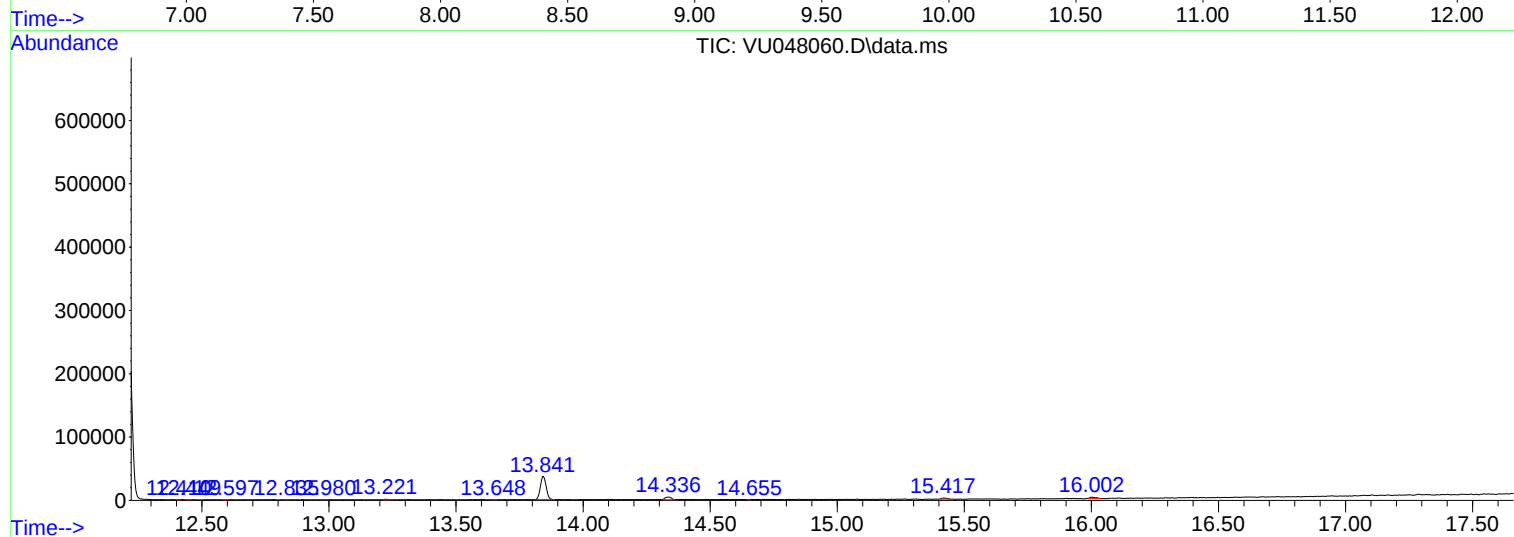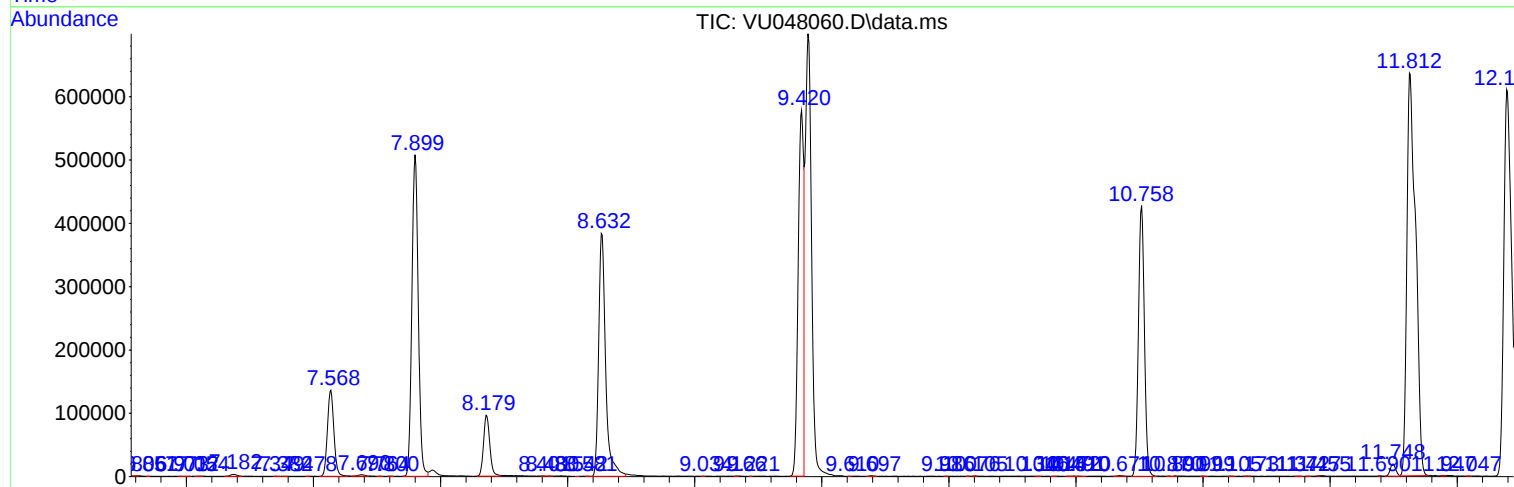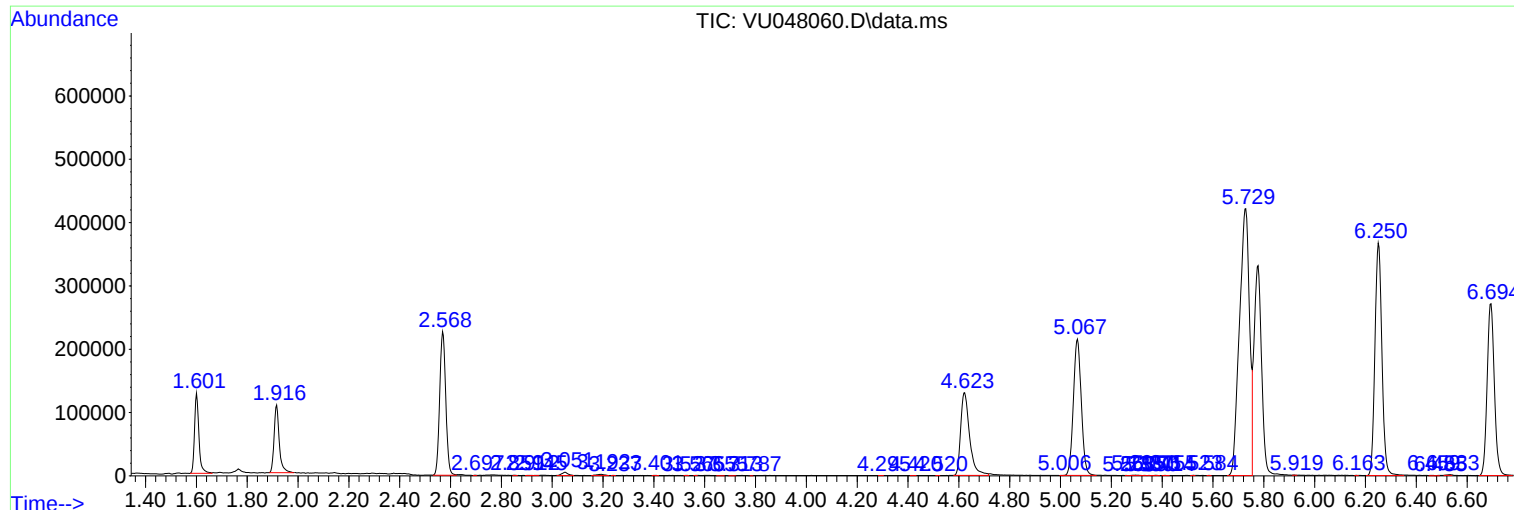

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048060.D
Acq On : 14 Apr 2022 15:58
Operator : SY/MD
Sample : N2387-02DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J48DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048060.D
Acq On : 14 Apr 2022 15:58
Operator : SY/MD
Sample : N2387-02DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J48DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------