

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048081.D
 Acq On : 15 Apr 2022 00:12
 Operator : SY/MD
 Sample : N2387-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rBV	110930	131449	12.34%	1.526%
2	1.916	171	179	196	rVB	96267	135396	12.71%	1.572%
3	2.472	350	352	356	rBV3	430	245	0.02%	0.003%
4	2.568	370	382	399	rBV	200181	329355	30.91%	3.824%
5	2.703	421	424	427	rBV3	302	220	0.02%	0.003%
6	2.793	448	452	463	rVB3	988	1330	0.12%	0.015%
7	2.842	463	467	468	rBV3	430	279	0.03%	0.003%
8	2.967	503	506	510	rBV2	239	225	0.02%	0.003%
9	3.051	526	532	537	rBV3	604	648	0.06%	0.008%
10	3.186	562	574	589	rVB2	5820	13144	1.23%	0.153%
11	3.295	605	608	612	rVV3	344	252	0.02%	0.003%
12	3.337	616	621	624	rBV2	404	393	0.04%	0.005%
13	3.392	634	638	641	rVV3	234	206	0.02%	0.002%
14	3.449	653	656	661	rVB2	303	273	0.03%	0.003%
15	3.572	690	694	699	rBV3	303	229	0.02%	0.003%
16	3.732	739	744	750	rVV3	246	371	0.03%	0.004%
17	3.861	780	784	789	rVB2	534	389	0.04%	0.005%
18	3.977	814	820	824	rBV2	250	220	0.02%	0.003%
19	4.150	870	874	877	rVB2	318	209	0.02%	0.002%
20	4.620	1007	1020	1042	rBV	130411	308339	28.94%	3.580%
21	4.973	1127	1130	1137	rBV3	268	259	0.02%	0.003%
22	5.067	1140	1159	1182	rBV	197410	434987	40.83%	5.051%
23	5.176	1190	1193	1195	rBV2	344	201	0.02%	0.002%
24	5.215	1203	1205	1209	rBV	328	301	0.03%	0.003%
25	5.256	1213	1218	1222	rVB2	396	415	0.04%	0.005%
26	5.289	1222	1228	1230	rBV2	754	823	0.08%	0.010%
27	5.629	1329	1334	1337	rBV2	218	236	0.02%	0.003%
28	5.726	1342	1364	1394	rBV2	387615	1065447	100.00%	12.371%
29	6.079	1471	1474	1480	rVB3	262	219	0.02%	0.003%
30	6.118	1480	1486	1488	rBV3	575	422	0.04%	0.005%
31	6.250	1512	1527	1554	rBV	351642	673228	63.19%	7.817%
32	6.424	1577	1581	1585	rBV3	305	272	0.03%	0.003%
33	6.523	1608	1612	1615	rBV4	807	729	0.07%	0.008%
34	6.575	1626	1628	1631	rBV	423	313	0.03%	0.004%
35	6.616	1638	1641	1649	rBV	216	251	0.02%	0.003%
36	6.694	1649	1665	1685	rBV	252789	497576	46.70%	5.777%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048081.D
 Acq On : 15 Apr 2022 00:12
 Operator : SY/MD
 Sample : N2387-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.887	1721	1725	1732	rVB2	179	212	0.02%	0.002%
38	7.044	1768	1774	1777	rBV3	248	295	0.03%	0.003%
39	7.182	1808	1817	1827	rBV4	3292	5593	0.52%	0.065%
40	7.366	1864	1874	1877	rBV	343	365	0.03%	0.004%
41	7.465	1903	1905	1911	rVB2	304	196	0.02%	0.002%
42	7.568	1925	1937	1951	rBV	110678	195925	18.39%	2.275%
43	7.694	1967	1976	1986	rVB6	1811	3181	0.30%	0.037%
44	7.732	1986	1988	1990	rVB	491	203	0.02%	0.002%
45	7.751	1990	1994	1998	rVB3	394	339	0.03%	0.004%
46	7.796	2004	2008	2010	rBV3	393	328	0.03%	0.004%
47	7.899	2027	2040	2056	rBV	443253	777547	72.98%	9.028%
48	8.099	2099	2102	2106	rVB3	542	394	0.04%	0.005%
49	8.121	2106	2109	2114	rVB3	385	264	0.02%	0.003%
50	8.182	2114	2128	2142	rBV	81700	140490	13.19%	1.631%
51	8.375	2186	2188	2191	rVB	461	267	0.03%	0.003%
52	8.395	2191	2194	2195	rBV	360	205	0.02%	0.002%
53	8.472	2212	2218	2226	rVB2	1344	1848	0.17%	0.021%
54	8.536	2235	2238	2244	rVB4	295	319	0.03%	0.004%
55	8.587	2249	2254	2255	rBV	225	196	0.02%	0.002%
56	8.632	2255	2268	2306	rBV	352013	674431	63.30%	7.831%
57	8.877	2340	2344	2345	rBV2	547	364	0.03%	0.004%
58	8.919	2352	2357	2359	rBV2	366	275	0.03%	0.003%
59	8.967	2369	2372	2376	rBV2	330	299	0.03%	0.003%
60	9.163	2431	2433	2437	rVB	362	286	0.03%	0.003%
61	9.195	2438	2443	2448	rVB2	266	287	0.03%	0.003%
62	9.221	2448	2451	2453	rBV	260	220	0.02%	0.003%
63	9.269	2461	2466	2472	rBV	404	460	0.04%	0.005%
64	9.417	2499	2512	2550	rBV	529846	914616	85.84%	10.620%
65	9.613	2570	2573	2576	rBV3	282	237	0.02%	0.003%
66	9.822	2633	2638	2641	rVB2	251	237	0.02%	0.003%
67	9.980	2681	2687	2690	rBV2	189	218	0.02%	0.003%
68	10.015	2694	2698	2701	rVB	310	226	0.02%	0.003%
69	10.102	2721	2725	2728	rVV2	257	313	0.03%	0.004%
70	10.182	2743	2750	2753	rVV2	149	213	0.02%	0.002%
71	10.385	2811	2813	2819	rVB2	288	270	0.03%	0.003%
72	10.420	2819	2824	2831	rVB2	369	437	0.04%	0.005%
73	10.481	2841	2843	2850	rVB3	254	246	0.02%	0.003%
74	10.558	2861	2867	2869	rBV2	188	214	0.02%	0.002%
75	10.632	2883	2890	2891	rBV	304	320	0.03%	0.004%
76	10.671	2896	2902	2904	rBV2	945	751	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048081.D
 Acq On : 15 Apr 2022 00:12
 Operator : SY/MD
 Sample : N2387-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.700	2908	2911	2915	rBV2	225	212	0.02%	0.002%
78	10.758	2915	2929	2949	rVB	364858	592844	55.64%	6.883%
79	10.893	2966	2971	2980	rVB6	2084	3349	0.31%	0.039%
80	11.099	3031	3035	3040	rVB	273	252	0.02%	0.003%
81	11.285	3089	3093	3097	rVB3	300	299	0.03%	0.003%
82	11.365	3113	3118	3120	rBV2	208	220	0.02%	0.003%
83	11.391	3121	3126	3131	rVV3	304	419	0.04%	0.005%
84	11.578	3182	3184	3188	rVB	356	198	0.02%	0.002%
85	11.709	3221	3225	3229	rBV	348	246	0.02%	0.003%
86	11.812	3244	3257	3274	rBV	560334	891212	83.65%	10.348%
87	11.912	3285	3288	3292	rBV2	544	388	0.04%	0.005%
88	12.066	3330	3336	3348	rBV7	2908	5193	0.49%	0.060%
89	12.195	3363	3376	3393	rBV	482395	791651	74.30%	9.192%
90	12.385	3431	3435	3437	rBV2	299	274	0.03%	0.003%
91	12.484	3464	3466	3471	rVB	436	226	0.02%	0.003%
92	12.513	3471	3475	3478	rBV2	349	345	0.03%	0.004%
93	12.729	3540	3542	3547	rVB2	375	231	0.02%	0.003%
94	13.086	3650	3653	3656	rBV	351	212	0.02%	0.002%
95	13.398	3747	3750	3753	rBV3	378	345	0.03%	0.004%
96	13.703	3842	3845	3848	rBV	309	248	0.02%	0.003%
97	13.848	3885	3890	3894	rBV3	893	1021	0.10%	0.012%
98	14.870	4205	4208	4211	rBV	592	405	0.04%	0.005%
99	15.192	4305	4308	4311	rBV	685	486	0.05%	0.006%
100	15.520	4408	4410	4412	rBV2	644	393	0.04%	0.005%

Sum of corrected areas: 8612607




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048081.D
Acq On : 15 Apr 2022 00:12
Operator : SY/MD
Sample : N2387-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

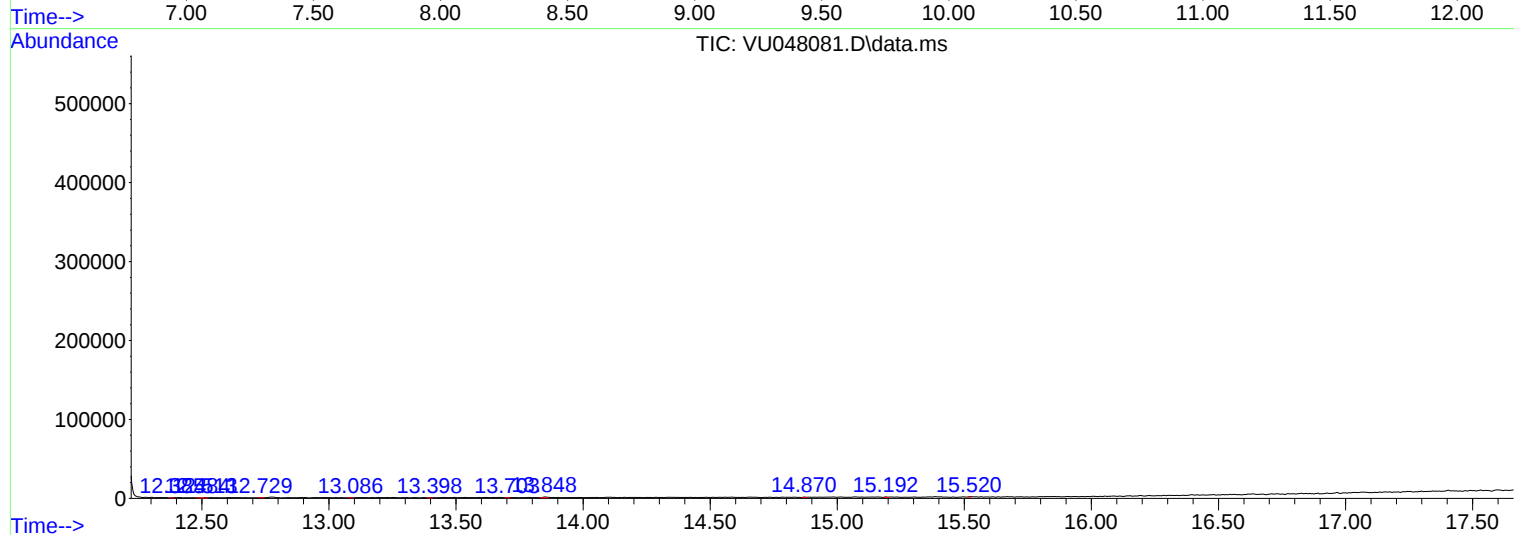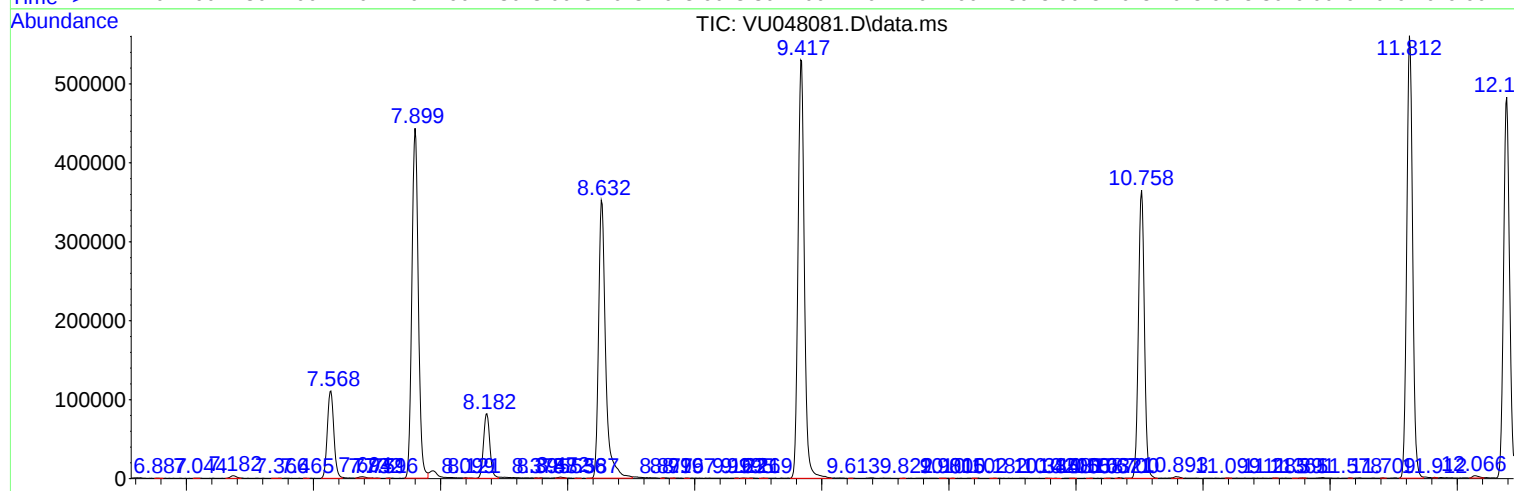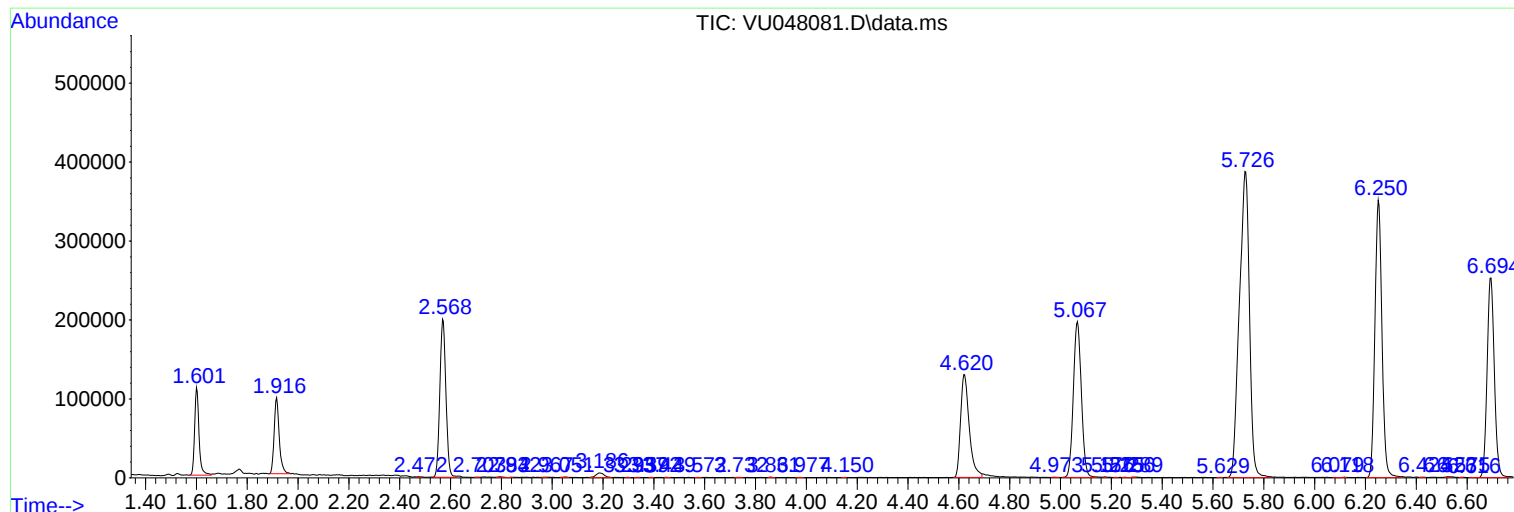

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048081.D
Acq On : 15 Apr 2022 00:12
Operator : SY/MD
Sample : N2387-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048081.D
Acq On : 15 Apr 2022 00:12
Operator : SY/MD
Sample : N2387-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------