

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048085.D
 Acq On : 15 Apr 2022 01:44
 Operator : SY/MD
 Sample : N2419-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	50	rBV2	4308	5202	0.51%	0.062%
2	1.601	73	81	97	rBV	101688	121002	11.75%	1.433%
3	1.916	170	179	196	rBV	94658	131132	12.73%	1.553%
4	2.568	370	382	395	rBV	192904	315133	30.60%	3.731%
5	2.626	395	400	413	rVB	7977	13291	1.29%	0.157%
6	2.739	433	435	436	rBV	551	242	0.02%	0.003%
7	2.758	437	441	448	rVB3	1006	1360	0.13%	0.016%
8	2.906	483	487	490	rVB2	328	259	0.03%	0.003%
9	3.138	553	559	562	rVB	242	282	0.03%	0.003%
10	3.189	564	575	586	rVV2	2300	5506	0.53%	0.065%
11	3.311	609	613	617	rBV3	235	243	0.02%	0.003%
12	3.359	626	628	633	rVB2	405	288	0.03%	0.003%
13	3.465	658	661	665	rBV3	353	303	0.03%	0.004%
14	3.488	665	668	672	rVB	317	225	0.02%	0.003%
15	3.514	672	676	679	rBV	270	243	0.02%	0.003%
16	3.536	679	683	687	rVB2	392	356	0.03%	0.004%
17	3.572	687	694	697	rBV2	489	543	0.05%	0.006%
18	3.636	710	714	719	rVB	321	341	0.03%	0.004%
19	3.729	741	743	750	rVB2	351	220	0.02%	0.003%
20	3.835	768	776	779	rBV3	360	491	0.05%	0.006%
21	3.877	785	789	792	rBV2	337	253	0.02%	0.003%
22	3.916	798	801	805	rBV	237	240	0.02%	0.003%
23	4.009	824	830	837	rBV2	274	388	0.04%	0.005%
24	4.163	873	878	881	rBV2	344	307	0.03%	0.004%
25	4.189	881	886	889	rVV3	223	262	0.03%	0.003%
26	4.453	964	968	972	rBV	216	208	0.02%	0.002%
27	4.623	1008	1021	1052	rBV	124297	312157	30.31%	3.696%
28	5.067	1142	1159	1177	rBV	196954	429089	41.67%	5.080%
29	5.208	1197	1203	1204	rBV3	454	382	0.04%	0.005%
30	5.285	1223	1227	1230	rBV2	529	528	0.05%	0.006%
31	5.408	1260	1265	1268	rBV	210	232	0.02%	0.003%
32	5.517	1294	1299	1302	rBV2	171	197	0.02%	0.002%
33	5.726	1341	1364	1385	rBV2	369675	1029790	100.00%	12.192%
34	5.899	1417	1418	1423	rVB3	480	227	0.02%	0.003%
35	5.925	1423	1426	1428	rBV3	294	190	0.02%	0.002%
36	6.031	1455	1459	1461	rBV3	369	351	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048085.D
 Acq On : 15 Apr 2022 01:44
 Operator : SY/MD
 Sample : N2419-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.153	1494	1497	1500	rBV2	307	201	0.02%	0.002%
38	6.250	1513	1527	1552	rBV	333029	643073	62.45%	7.614%
39	6.385	1567	1569	1574	rVB2	370	238	0.02%	0.003%
40	6.411	1574	1577	1582	rVB3	355	249	0.02%	0.003%
41	6.443	1585	1587	1593	rVB2	588	497	0.05%	0.006%
42	6.472	1593	1596	1600	rBV2	377	305	0.03%	0.004%
43	6.533	1607	1615	1619	rBV4	1197	1781	0.17%	0.021%
44	6.633	1643	1646	1648	rBV	364	211	0.02%	0.002%
45	6.694	1650	1665	1685	rBV	245403	483179	46.92%	5.721%
46	6.806	1696	1700	1709	rVB3	929	1127	0.11%	0.013%
47	7.041	1765	1773	1780	rBV2	524	1071	0.10%	0.013%
48	7.182	1810	1817	1832	rVB4	3347	6015	0.58%	0.071%
49	7.568	1923	1937	1956	rBV	111571	199385	19.36%	2.361%
50	7.690	1966	1975	1988	rVB5	2210	4065	0.39%	0.048%
51	7.758	1993	1996	2000	rBV	245	196	0.02%	0.002%
52	7.793	2004	2007	2011	rVB3	381	358	0.03%	0.004%
53	7.899	2026	2040	2056	rBV	434735	751232	72.95%	8.894%
54	8.179	2111	2127	2145	rBV	82240	140173	13.61%	1.660%
55	8.475	2212	2219	2228	rVB3	2665	3991	0.39%	0.047%
56	8.539	2235	2239	2247	rVB4	443	476	0.05%	0.006%
57	8.632	2256	2268	2301	rBV	323926	603360	58.59%	7.143%
58	8.787	2310	2316	2328	rVB5	5119	8222	0.80%	0.097%
59	8.909	2351	2354	2359	rBV3	277	341	0.03%	0.004%
60	9.105	2410	2415	2417	rVB2	313	260	0.03%	0.003%
61	9.131	2417	2423	2425	rBV2	339	317	0.03%	0.004%
62	9.189	2437	2441	2444	rBV2	279	259	0.03%	0.003%
63	9.340	2485	2488	2493	rVB3	305	215	0.02%	0.003%
64	9.372	2493	2498	2499	rBV	246	217	0.02%	0.003%
65	9.417	2499	2512	2548	rBV	516244	878384	85.30%	10.400%
66	9.571	2555	2560	2567	rVB3	856	982	0.10%	0.012%
67	9.649	2581	2584	2589	rVV3	489	400	0.04%	0.005%
68	9.694	2593	2598	2608	rVB3	954	1346	0.13%	0.016%
69	9.761	2616	2619	2622	rBV2	214	197	0.02%	0.002%
70	9.784	2624	2626	2628	rVV	381	213	0.02%	0.003%
71	9.796	2628	2630	2634	rVV2	457	323	0.03%	0.004%
72	9.825	2637	2639	2644	rVV	333	281	0.03%	0.003%
73	10.025	2697	2701	2704	rBV2	234	209	0.02%	0.002%
74	10.079	2716	2718	2722	rBV	323	243	0.02%	0.003%
75	10.128	2730	2733	2739	rVB2	442	349	0.03%	0.004%
76	10.240	2764	2768	2773	rBV3	473	474	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048085.D
 Acq On : 15 Apr 2022 01:44
 Operator : SY/MD
 Sample : N2419-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.562	2865	2868	2869	rBV2	728	469	0.05%	0.006%
78	10.665	2896	2900	2901	rBV2	756	409	0.04%	0.005%
79	10.758	2915	2929	2950	rVB	400249	647962	62.92%	7.672%
80	10.896	2958	2972	2984	rVB2	5098	9073	0.88%	0.107%
81	10.967	2989	2994	2999	rBV2	345	417	0.04%	0.005%
82	11.279	3089	3091	3097	rVB2	462	396	0.04%	0.005%
83	11.343	3108	3111	3114	rVB	393	261	0.03%	0.003%
84	11.362	3114	3117	3120	rBV2	323	300	0.03%	0.004%
85	11.697	3214	3221	3226	rBV4	1378	1589	0.15%	0.019%
86	11.751	3236	3238	3241	rVB3	543	283	0.03%	0.003%
87	11.812	3244	3257	3275	rVV	541212	867427	84.23%	10.270%
88	11.970	3302	3306	3307	rBV	578	391	0.04%	0.005%
89	12.066	3327	3336	3345	rBV3	7784	13650	1.33%	0.162%
90	12.192	3362	3375	3402	rVV	486394	788669	76.59%	9.337%
91	12.324	3412	3416	3418	rVB3	531	334	0.03%	0.004%
92	12.362	3425	3428	3432	rBV2	370	274	0.03%	0.003%
93	12.404	3438	3441	3443	rBV	544	270	0.03%	0.003%
94	12.465	3457	3460	3463	rBV2	261	217	0.02%	0.003%
95	12.700	3530	3533	3537	rBV2	390	359	0.03%	0.004%
96	12.771	3550	3555	3564	rVB3	2020	2822	0.27%	0.033%
97	12.893	3587	3593	3602	rVB6	2869	3870	0.38%	0.046%
98	13.443	3761	3764	3768	rBV3	347	330	0.03%	0.004%
99	14.092	3963	3966	3968	rBV	364	290	0.03%	0.003%
100	15.449	4386	4388	4392	rBV2	597	381	0.04%	0.005%


Sum of corrected areas: 8446321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048085.D
Acq On : 15 Apr 2022 01:44
Operator : SY/MD
Sample : N2419-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

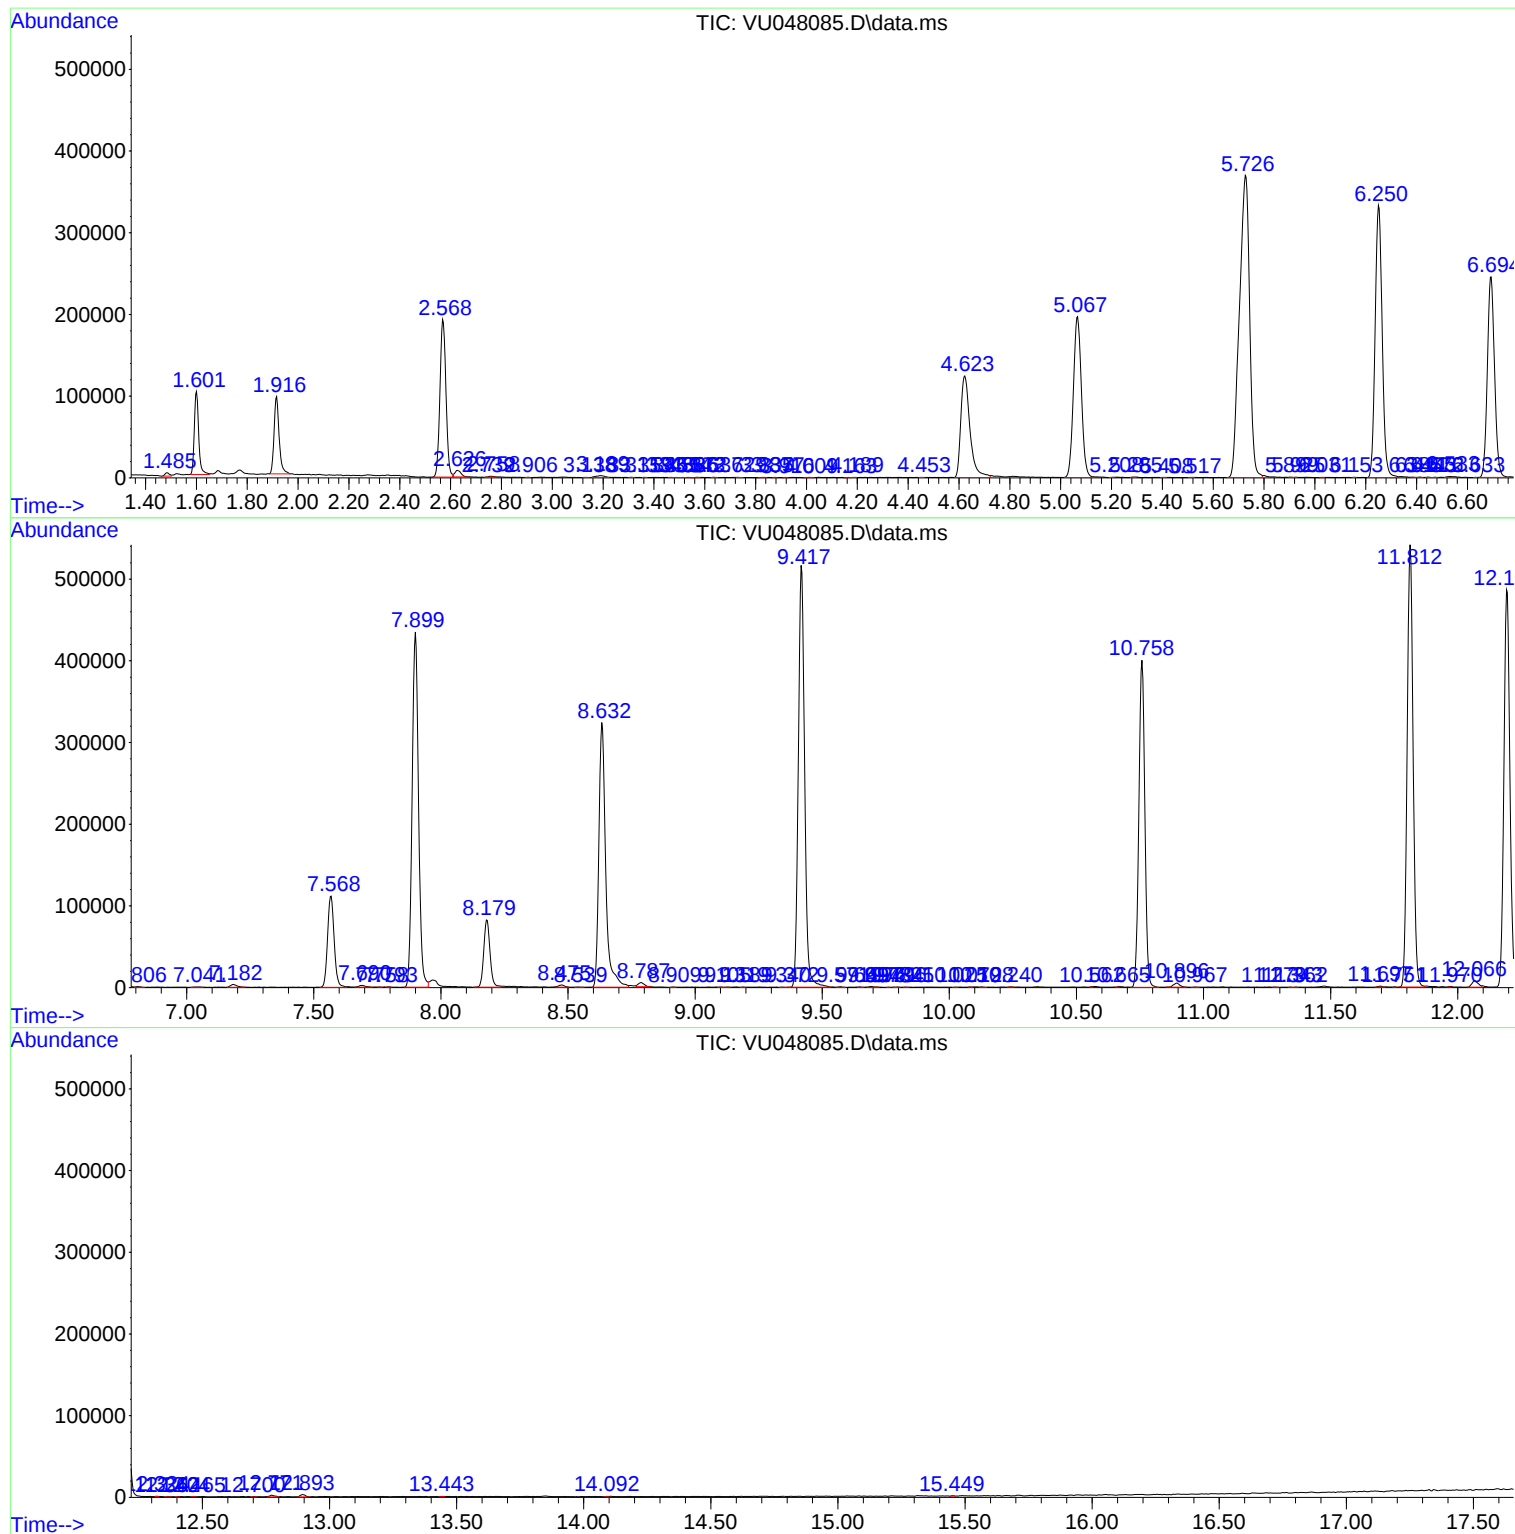

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048085.D
Acq On : 15 Apr 2022 01:44
Operator : SY/MD
Sample : N2419-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048085.D
Acq On : 15 Apr 2022 01:44
Operator : SY/MD
Sample : N2419-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------