

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048086.D
 Acq On : 15 Apr 2022 02:07
 Operator : SY/MD
 Sample : N2419-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	15	rVB2	6247	6187	0.59%	0.072%
2	1.600	73	81	96	rBV	105614	126144	12.12%	1.477%
3	1.916	170	179	198	rBV	94584	132881	12.77%	1.556%
4	2.568	370	382	398	rBV	193116	318165	30.58%	3.726%
5	2.761	437	442	446	rBV2	527	625	0.06%	0.007%
6	2.867	472	475	479	rVB2	402	292	0.03%	0.003%
7	2.890	479	482	488	rBV	402	444	0.04%	0.005%
8	2.951	495	501	503	rBV3	369	320	0.03%	0.004%
9	2.996	512	515	519	rBV	338	259	0.02%	0.003%
10	3.051	526	532	538	rVB3	648	878	0.08%	0.010%
11	3.083	538	542	545	rBV3	395	278	0.03%	0.003%
12	3.121	550	554	559	rVB3	298	257	0.02%	0.003%
13	3.189	565	575	583	rBV2	1822	3267	0.31%	0.038%
14	3.366	614	630	651	rVB2	13812	31290	3.01%	0.366%
15	3.440	651	653	658	rBV3	317	327	0.03%	0.004%
16	3.491	665	669	671	rBV2	241	206	0.02%	0.002%
17	3.578	692	696	697	rBV	419	226	0.02%	0.003%
18	3.620	706	709	716	rVV2	226	245	0.02%	0.003%
19	3.864	781	785	787	rBV	306	279	0.03%	0.003%
20	3.928	803	805	808	rVV	336	253	0.02%	0.003%
21	3.957	811	814	817	rVV2	300	215	0.02%	0.003%
22	4.057	841	845	849	rBV2	237	272	0.03%	0.003%
23	4.131	865	868	873	rBV	378	196	0.02%	0.002%
24	4.369	939	942	947	rVB3	349	319	0.03%	0.004%
25	4.404	947	953	955	rBV2	240	241	0.02%	0.003%
26	4.555	997	1000	1004	rVB	302	191	0.02%	0.002%
27	4.623	1007	1021	1060	rBV	129899	320510	30.80%	3.753%
28	4.861	1092	1095	1096	rBV2	311	185	0.02%	0.002%
29	4.909	1107	1110	1113	rBV2	287	276	0.03%	0.003%
30	4.973	1127	1130	1138	rVB3	271	283	0.03%	0.003%
31	5.067	1141	1159	1182	rBV	195121	428317	41.16%	5.016%
32	5.243	1211	1214	1217	rBV2	208	193	0.02%	0.002%
33	5.285	1223	1227	1232	rBV5	448	470	0.05%	0.006%
34	5.459	1277	1281	1285	rVB	292	241	0.02%	0.003%
35	5.504	1292	1295	1298	rVB2	338	271	0.03%	0.003%
36	5.571	1310	1316	1319	rBV2	194	215	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048086.D
 Acq On : 15 Apr 2022 02:07
 Operator : SY/MD
 Sample : N2419-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.594	1319	1323	1327	rBV2	194	167	0.02%	0.002%
38	5.726	1340	1364	1395	rBV2	376158	1040599	100.00%	12.186%
39	5.944	1423	1432	1433	rBV7	1398	1780	0.17%	0.021%
40	6.063	1465	1469	1473	rVB2	390	298	0.03%	0.003%
41	6.150	1493	1496	1504	rVB	419	526	0.05%	0.006%
42	6.250	1513	1527	1559	rBV	342585	647536	62.23%	7.583%
43	6.526	1607	1613	1622	rVV5	1110	2226	0.21%	0.026%
44	6.694	1649	1665	1695	rVV	250748	492042	47.28%	5.762%
45	6.803	1697	1699	1706	rVV5	762	822	0.08%	0.010%
46	7.105	1789	1793	1795	rBV	204	191	0.02%	0.002%
47	7.144	1801	1805	1808	rBV	215	226	0.02%	0.003%
48	7.182	1810	1817	1830	rVB2	3273	5398	0.52%	0.063%
49	7.269	1839	1844	1851	rBV3	293	361	0.03%	0.004%
50	7.330	1857	1863	1868	rBV2	176	213	0.02%	0.002%
51	7.568	1924	1937	1954	rBV	114665	203903	19.59%	2.388%
52	7.690	1967	1975	1985	rVV3	2218	3759	0.36%	0.044%
53	7.732	1986	1988	1992	rVB3	427	321	0.03%	0.004%
54	7.899	2026	2040	2056	rBV	428488	746380	71.73%	8.741%
55	8.179	2115	2127	2143	rVV	80140	139131	13.37%	1.629%
56	8.256	2149	2151	2153	rBV2	539	289	0.03%	0.003%
57	8.433	2203	2206	2209	rBV3	376	270	0.03%	0.003%
58	8.475	2211	2219	2231	rVB2	2922	5303	0.51%	0.062%
59	8.552	2239	2243	2245	rBV2	402	274	0.03%	0.003%
60	8.632	2256	2268	2301	rBV	367103	681120	65.45%	7.976%
61	8.909	2350	2354	2355	rBV	360	250	0.02%	0.003%
62	8.992	2376	2380	2382	rBV	244	177	0.02%	0.002%
63	9.021	2385	2389	2393	rVB3	276	293	0.03%	0.003%
64	9.160	2430	2432	2437	rVB2	446	292	0.03%	0.003%
65	9.189	2437	2441	2444	rBV2	270	202	0.02%	0.002%
66	9.337	2484	2487	2490	rBV	292	229	0.02%	0.003%
67	9.359	2490	2494	2496	rBV2	261	198	0.02%	0.002%
68	9.417	2499	2512	2531	rBV	490959	827858	79.56%	9.695%
69	9.639	2577	2581	2582	rBV2	345	228	0.02%	0.003%
70	9.697	2593	2599	2607	rBV4	953	1494	0.14%	0.017%
71	9.819	2629	2637	2640	rBV2	379	625	0.06%	0.007%
72	9.877	2650	2655	2656	rBV	194	177	0.02%	0.002%
73	9.909	2662	2665	2669	rVB2	303	232	0.02%	0.003%
74	9.931	2669	2672	2674	rBV2	279	229	0.02%	0.003%
75	9.992	2687	2691	2694	rBV3	227	195	0.02%	0.002%
76	10.115	2726	2729	2734	rVB2	304	218	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048086.D
 Acq On : 15 Apr 2022 02:07
 Operator : SY/MD
 Sample : N2419-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.259	2769	2774	2781	rVB2	188	265	0.03%	0.003%
78	10.645	2891	2894	2898	rBV	313	240	0.02%	0.003%
79	10.671	2900	2902	2907	rVB	434	302	0.03%	0.004%
80	10.758	2916	2929	2948	rBV	405067	651563	62.61%	7.630%
81	10.844	2953	2956	2961	rVV2	256	259	0.02%	0.003%
82	10.896	2961	2972	2987	rVB3	5322	9359	0.90%	0.110%
83	11.012	3005	3008	3013	rVB2	282	248	0.02%	0.003%
84	11.195	3062	3065	3068	rBV2	259	178	0.02%	0.002%
85	11.356	3109	3115	3116	rBV2	259	248	0.02%	0.003%
86	11.468	3145	3150	3154	rBV3	686	801	0.08%	0.009%
87	11.693	3218	3220	3225	rVB3	450	338	0.03%	0.004%
88	11.812	3244	3257	3276	rBV	552387	870958	83.70%	10.200%
89	11.915	3287	3289	3293	rBV2	503	284	0.03%	0.003%
90	12.066	3328	3336	3348	rBV3	9277	15947	1.53%	0.187%
91	12.195	3361	3376	3394	rBV	492610	800326	76.91%	9.372%
92	12.298	3406	3408	3411	rVB2	374	214	0.02%	0.003%
93	12.317	3411	3414	3420	rBV3	465	370	0.04%	0.004%
94	12.774	3549	3556	3565	rVB2	2109	3343	0.32%	0.039%
95	13.053	3641	3643	3646	rBV2	260	187	0.02%	0.002%
96	13.799	3869	3875	3877	rBV3	341	379	0.04%	0.004%
97	13.844	3884	3889	3901	rVB4	942	1292	0.12%	0.015%
98	14.060	3954	3956	3959	rBV3	274	186	0.02%	0.002%
99	14.102	3965	3969	3971	rBV3	391	367	0.04%	0.004%
100	14.545	4104	4107	4110	rBV2	397	275	0.03%	0.003%




Sum of corrected areas: 8539179

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048086.D
Acq On : 15 Apr 2022 02:07
Operator : SY/MD
Sample : N2419-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

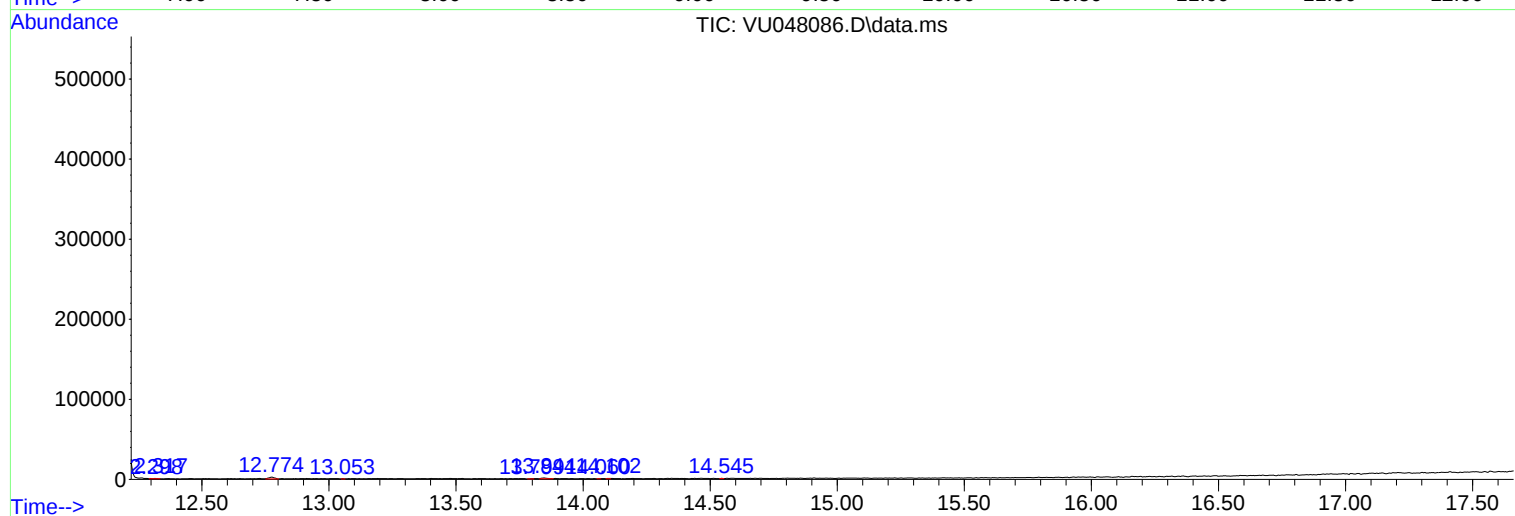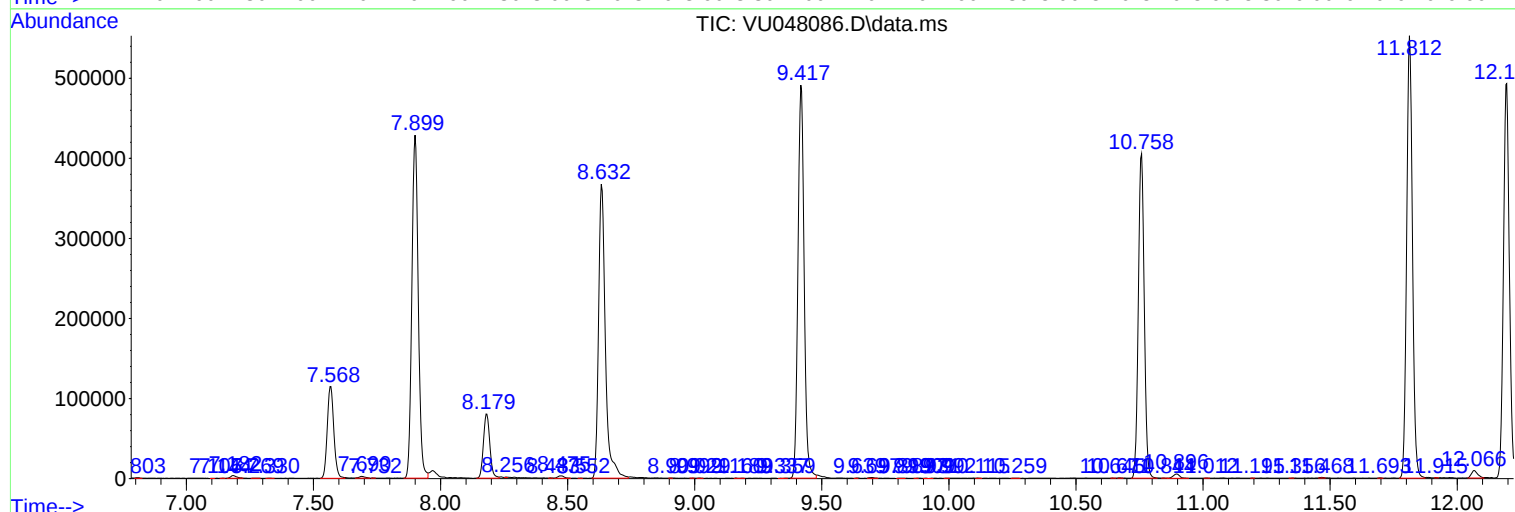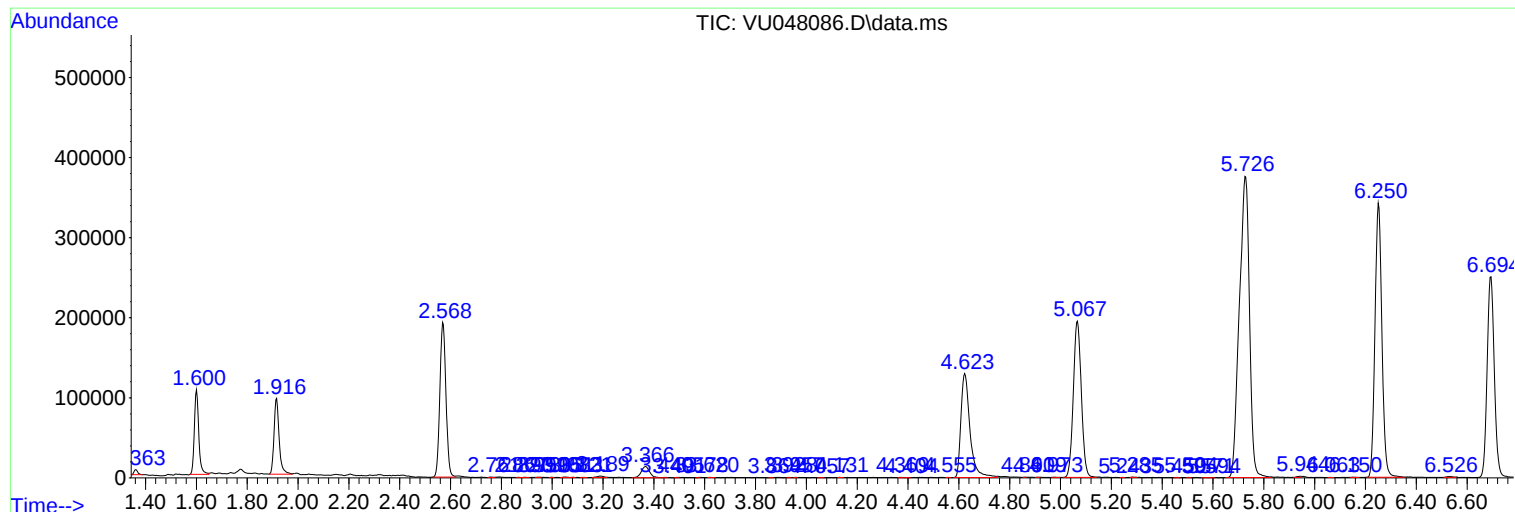

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048086.D
Acq On : 15 Apr 2022 02:07
Operator : SY/MD
Sample : N2419-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048086.D
Acq On : 15 Apr 2022 02:07
Operator : SY/MD
Sample : N2419-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
