

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048087.D
 Acq On : 15 Apr 2022 02:30
 Operator : SY/MD
 Sample : N2419-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rBV	101381	117613	11.47%	1.389%
2	1.916	171	179	195	rVB	92059	125335	12.23%	1.480%
3	2.571	370	383	399	rBV	190317	315270	30.75%	3.724%
4	2.729	429	432	433	rBV2	294	167	0.02%	0.002%
5	2.752	433	439	440	rVV3	358	357	0.03%	0.004%
6	2.806	452	456	458	rBV3	396	282	0.03%	0.003%
7	2.883	477	480	482	rBV	250	158	0.02%	0.002%
8	2.948	496	500	503	rBV2	245	211	0.02%	0.002%
9	2.967	504	506	509	rVV2	360	210	0.02%	0.002%
10	2.983	509	511	515	rVB2	304	196	0.02%	0.002%
11	3.012	515	520	526	rVB3	500	600	0.06%	0.007%
12	3.051	526	532	538	rBV4	890	1161	0.11%	0.014%
13	3.089	542	544	548	rVB	284	191	0.02%	0.002%
14	3.112	548	551	554	rBV2	201	155	0.02%	0.002%
15	3.186	563	574	590	rBV2	4353	9478	0.92%	0.112%
16	3.295	606	608	612	rVB2	325	184	0.02%	0.002%
17	3.317	612	615	618	rVB2	300	201	0.02%	0.002%
18	3.346	618	624	628	rBV3	404	395	0.04%	0.005%
19	3.369	628	631	635	rBV2	398	376	0.04%	0.004%
20	3.481	663	666	669	rBV	219	158	0.02%	0.002%
21	3.507	670	674	675	rVV	224	163	0.02%	0.002%
22	3.726	740	742	747	rVB2	282	173	0.02%	0.002%
23	3.780	755	759	762	rBV2	280	236	0.02%	0.003%
24	3.951	810	812	815	rVB3	321	210	0.02%	0.002%
25	3.999	822	827	828	rBV2	332	229	0.02%	0.003%
26	4.028	834	836	840	rVB	358	195	0.02%	0.002%
27	4.051	840	843	846	rBV	219	204	0.02%	0.002%
28	4.105	855	860	865	rBV2	409	557	0.05%	0.007%
29	4.350	935	936	940	rVB2	373	202	0.02%	0.002%
30	4.382	940	946	948	rBV	213	275	0.03%	0.003%
31	4.620	1007	1020	1066	rVV	124598	309991	30.24%	3.661%
32	4.970	1126	1129	1137	rBV3	337	389	0.04%	0.005%
33	5.067	1141	1159	1184	rBV	195020	428273	41.78%	5.058%
34	5.218	1201	1206	1208	rBV2	394	339	0.03%	0.004%
35	5.282	1223	1226	1230	rBV3	511	548	0.05%	0.006%
36	5.340	1241	1244	1248	rVB3	326	218	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048087.D
 Acq On : 15 Apr 2022 02:30
 Operator : SY/MD
 Sample : N2419-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.520	1296	1300	1304	rBV2	260	304	0.03%	0.004%
38	5.726	1343	1364	1389	rBV2	373811	1025116	100.00%	12.107%
39	6.060	1463	1468	1470	rBV3	403	281	0.03%	0.003%
40	6.250	1512	1527	1552	rBV	342345	654678	63.86%	7.732%
41	6.391	1567	1571	1574	rVB	460	290	0.03%	0.003%
42	6.423	1579	1581	1584	rBV2	258	168	0.02%	0.002%
43	6.526	1610	1613	1614	rBV	742	412	0.04%	0.005%
44	6.584	1628	1631	1636	rVB	289	259	0.03%	0.003%
45	6.693	1649	1665	1686	rBV	245599	483955	47.21%	5.716%
46	6.845	1708	1712	1715	rBV2	345	226	0.02%	0.003%
47	6.861	1715	1717	1720	rVB	347	163	0.02%	0.002%
48	6.931	1737	1739	1745	rVB2	299	307	0.03%	0.004%
49	6.973	1747	1752	1756	rVV2	244	301	0.03%	0.004%
50	7.002	1756	1761	1764	rVV2	170	176	0.02%	0.002%
51	7.044	1770	1774	1782	rBV3	430	545	0.05%	0.006%
52	7.131	1798	1801	1806	rBV2	272	254	0.02%	0.003%
53	7.185	1810	1818	1831	rVV5	2584	4874	0.48%	0.058%
54	7.427	1890	1893	1898	rVB2	198	192	0.02%	0.002%
55	7.568	1924	1937	1954	rBV	111531	198844	19.40%	2.348%
56	7.693	1969	1976	1984	rVB5	2052	2967	0.29%	0.035%
57	7.899	2026	2040	2056	rBV	431226	752969	73.45%	8.893%
58	8.111	2105	2106	2111	rVB2	344	242	0.02%	0.003%
59	8.179	2111	2127	2145	rBV	81268	139174	13.58%	1.644%
60	8.475	2209	2219	2227	rBV2	2881	4656	0.45%	0.055%
61	8.536	2234	2238	2240	rBV	382	304	0.03%	0.004%
62	8.632	2255	2268	2303	rBV	349108	676810	66.02%	7.994%
63	8.845	2332	2334	2337	rVB	649	366	0.04%	0.004%
64	8.877	2337	2344	2347	rBV2	593	806	0.08%	0.010%
65	9.214	2447	2449	2453	rVB	240	163	0.02%	0.002%
66	9.417	2498	2512	2550	rBV	526725	900220	87.82%	10.632%
67	9.562	2554	2557	2560	rVV2	444	344	0.03%	0.004%
68	9.578	2560	2562	2567	rVB3	566	409	0.04%	0.005%
69	9.645	2579	2583	2591	rBV4	569	537	0.05%	0.006%
70	9.690	2592	2597	2606	rVB2	998	1251	0.12%	0.015%
71	9.976	2684	2686	2693	rVB2	330	298	0.03%	0.004%
72	10.015	2693	2698	2700	rBV	191	169	0.02%	0.002%
73	10.070	2712	2715	2719	rVB	227	166	0.02%	0.002%
74	10.108	2721	2727	2731	rBV3	446	625	0.06%	0.007%
75	10.131	2731	2734	2739	rVV	253	254	0.02%	0.003%
76	10.250	2768	2771	2775	rBV2	325	237	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048087.D
 Acq On : 15 Apr 2022 02:30
 Operator : SY/MD
 Sample : N2419-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.311	2786	2790	2794	rBV2	319	293	0.03%	0.003%
78	10.343	2797	2800	2802	rBV	260	201	0.02%	0.002%
79	10.378	2808	2811	2816	rBV	222	275	0.03%	0.003%
80	10.491	2843	2846	2848	rVB3	354	223	0.02%	0.003%
81	10.529	2855	2858	2861	rBV2	179	159	0.02%	0.002%
82	10.616	2882	2885	2892	rBV2	253	205	0.02%	0.002%
83	10.758	2914	2929	2947	rBV	371886	606054	59.12%	7.158%
84	10.899	2964	2973	2983	rVB3	4512	7743	0.76%	0.091%
85	10.979	2996	2998	3004	rVB2	299	280	0.03%	0.003%
86	11.005	3004	3006	3011	rBV2	316	269	0.03%	0.003%
87	11.143	3045	3049	3050	rBV2	211	154	0.02%	0.002%
88	11.311	3097	3101	3103	rBV2	363	296	0.03%	0.003%
89	11.468	3142	3150	3153	rBV6	861	1285	0.13%	0.015%
90	11.719	3225	3228	3231	rVB	328	196	0.02%	0.002%
91	11.748	3234	3237	3242	rVB3	521	455	0.04%	0.005%
92	11.812	3244	3257	3275	rBV	549707	879867	85.83%	10.392%
93	12.069	3329	3337	3348	rVB7	2950	5294	0.52%	0.063%
94	12.195	3362	3376	3399	rBV	479131	791126	77.17%	9.344%
95	12.504	3466	3472	3476	rBV3	351	486	0.05%	0.006%
96	12.532	3476	3481	3483	rBV3	336	270	0.03%	0.003%
97	12.774	3550	3556	3564	rVB3	902	1606	0.16%	0.019%
98	13.224	3694	3696	3699	rVB	488	236	0.02%	0.003%
99	13.844	3886	3889	3890	rBV2	581	323	0.03%	0.004%
100	14.455	4076	4079	4084	rVB3	535	380	0.04%	0.004%



Sum of corrected areas: 8466888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048087.D
Acq On : 15 Apr 2022 02:30
Operator : SY/MD
Sample : N2419-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

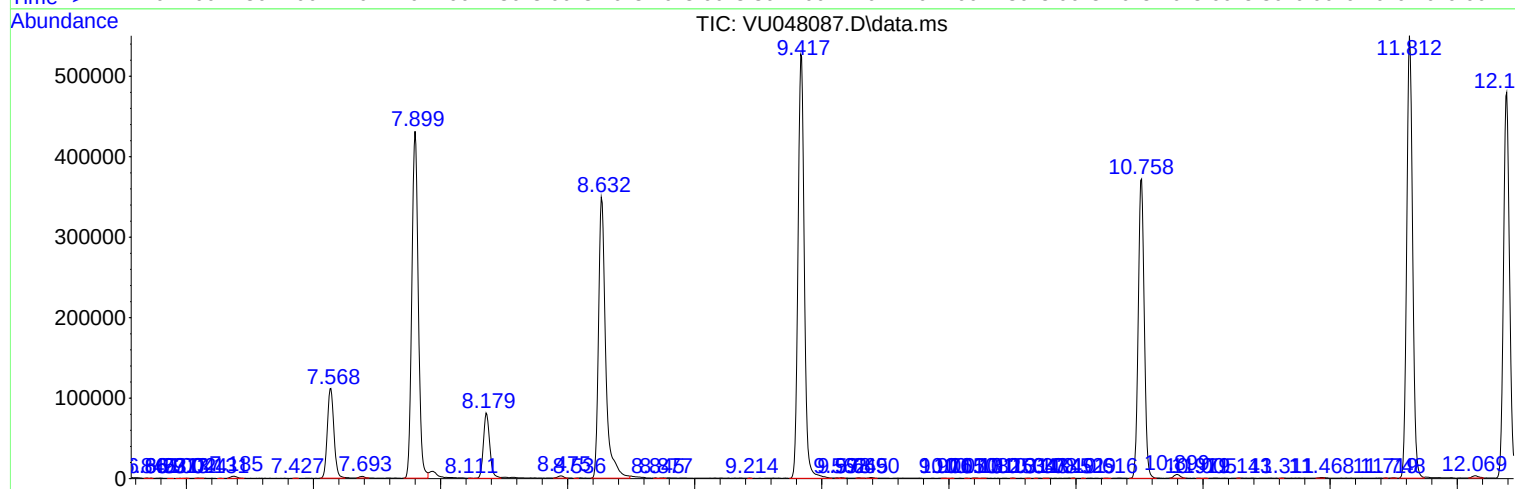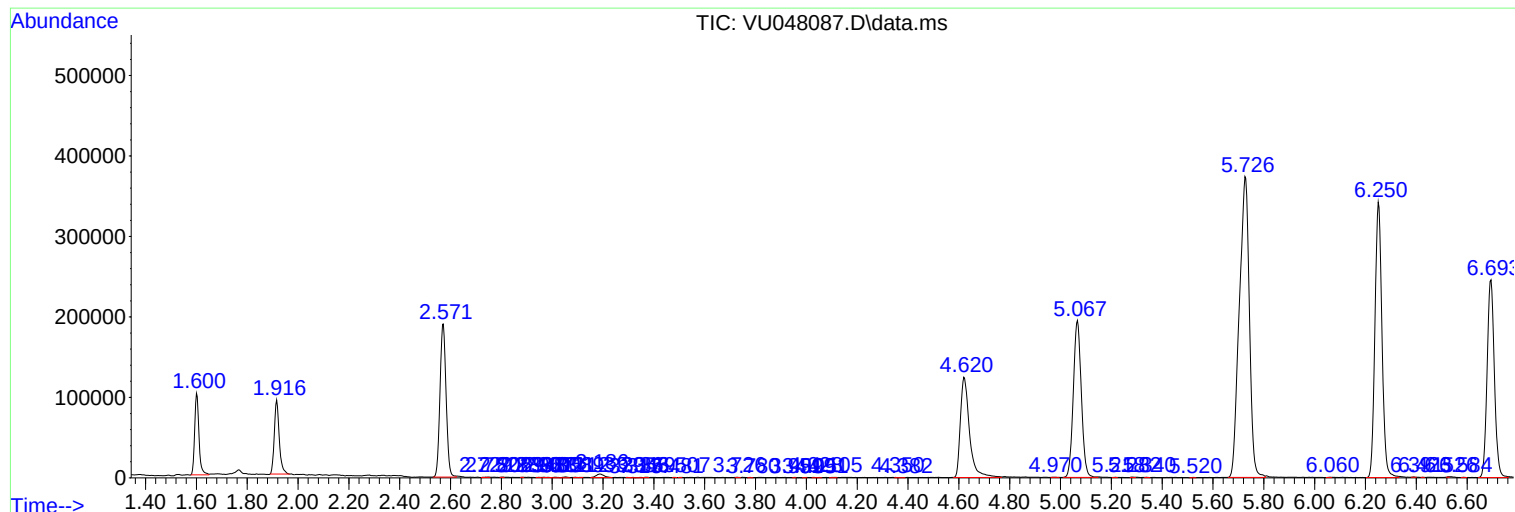

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048087.D
Acq On : 15 Apr 2022 02:30
Operator : SY/MD
Sample : N2419-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
Data File : VU048087.D
Acq On : 15 Apr 2022 02:30
Operator : SY/MD
Sample : N2419-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------