


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041422\
 Data File : VU048042.D
 Acq On : 14 Apr 2022 08:54
 Operator : SY/MD
 Sample : BFB064
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB064

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 19 03:36:43 2022

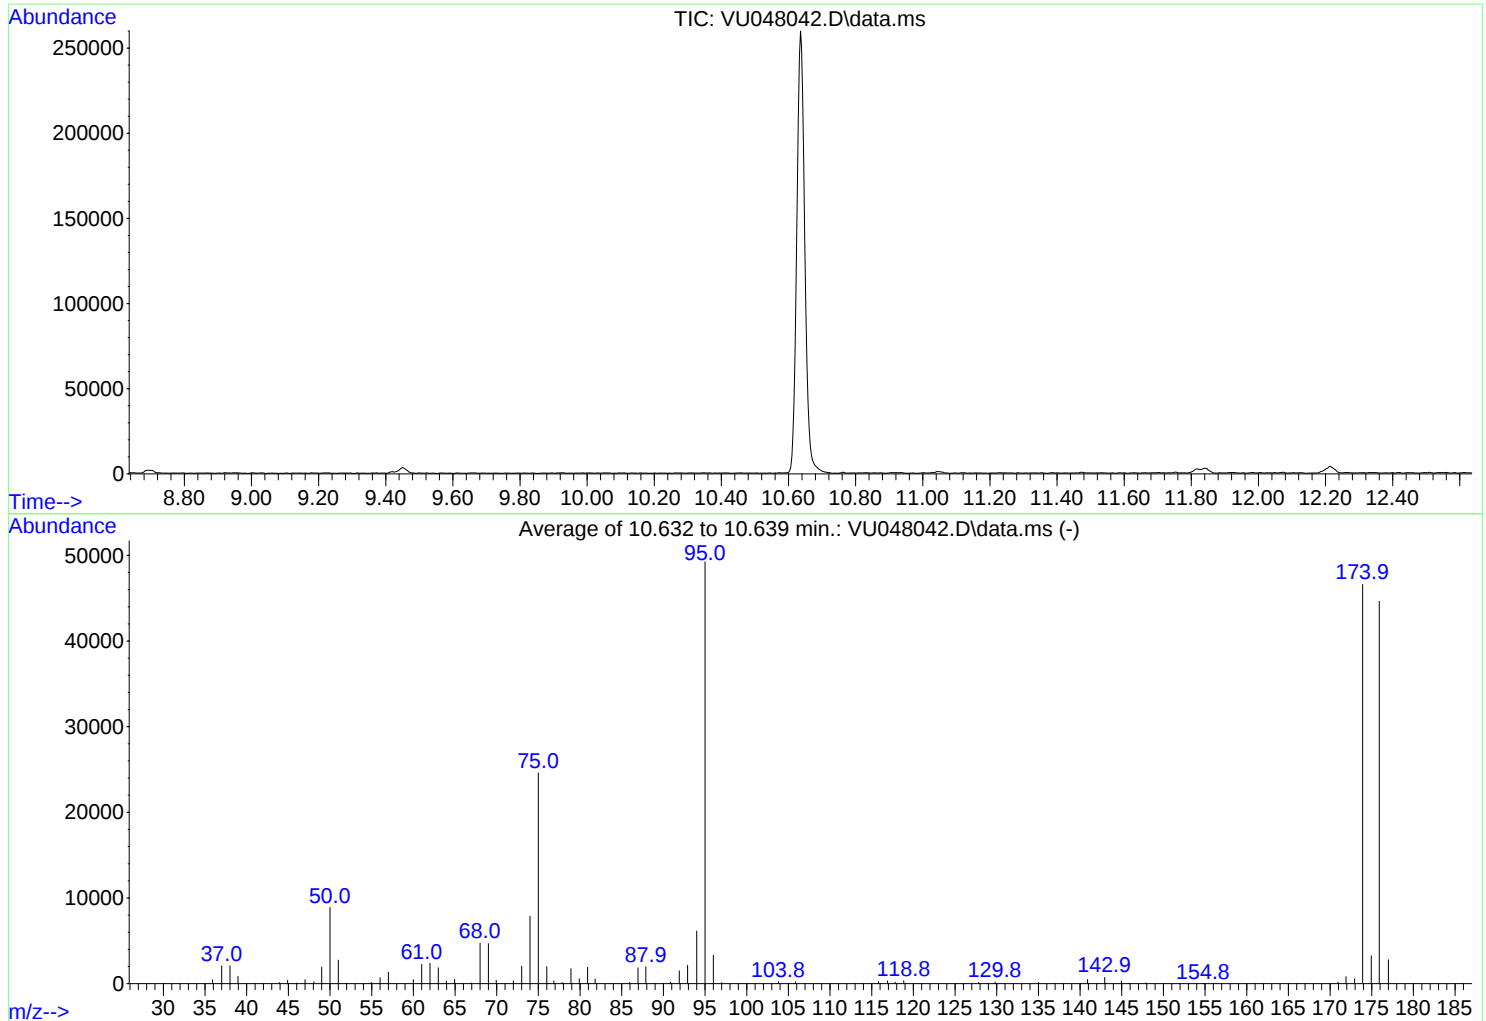

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	8901	PASS
75	95	30	80	49.9	24595	PASS
95	95	100	100	100.0	49245	PASS
96	95	5	9	6.7	3301	PASS
173	174	0.00	2	1.2	553	PASS
174	95	50	120	94.7	46611	PASS
175	174	5	9	7.0	3255	PASS
176	174	95	101	95.8	44645	PASS
177	176	5	9	6.2	2781	PASS

m/z	Abundance
39.90	157.0
43.90	492.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.90	503.0
37.00	2119.0
38.00	2047.0
39.00	883.0
39.80	154.0
43.90	681.0
44.90	411.0
47.00	486.0
48.10	229.0
49.00	1869.0
50.00	8743.0
51.00	2778.0
51.90	102.0
54.90	136.0
56.00	734.0
57.00	1364.0
60.00	421.0
61.00	2101.0
62.00	2326.0
63.00	1893.0
64.00	351.0
65.00	476.0
66.80	113.0
68.00	4773.0
69.00	4899.0
69.90	389.0
72.00	296.0
73.00	2034.0
74.00	7831.0
75.00	24136.0
76.00	2017.0
76.80	275.0
77.80	148.0
78.90	1737.0
79.90	579.0
80.90	1818.0
81.80	548.0
85.90	148.0
87.00	1899.0
87.90	1872.0
90.90	139.0
91.90	1461.0
92.90	2098.0
94.00	5799.0
95.00	48224.0
96.00	3458.0
97.00	107.0
103.80	230.0
105.90	232.0
115.80	215.0
116.90	335.0
117.80	195.0
118.90	304.0
127.70	115.0
129.80	192.0
135.00	116.0
140.90	490.0
142.90	724.0
144.90	298.0
145.90	101.0
147.90	152.0
154.80	112.0
170.90	181.0
171.90	805.0
172.90	511.0
173.90	44280.0
174.90	3058.0
175.90	42368.0
177.00	2707.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.90	475.0
37.00	2127.0
38.00	2160.0
39.00	868.0
39.90	143.0
43.90	617.0
44.90	408.0
46.00	115.0
47.00	494.0
48.00	231.0
49.00	2017.0
50.00	9195.0
51.00	2856.0
55.00	155.0
56.00	731.0
57.00	1363.0
60.00	474.0
61.00	2356.0
62.00	2440.0
63.00	1887.0
64.00	287.0
64.90	536.0
67.00	112.0
68.00	4914.0
69.00	4794.0
69.90	407.0
72.00	351.0
73.00	2085.0
74.00	8101.0
75.00	25368.0
76.00	2017.0
76.80	323.0
77.90	130.0
78.90	1799.0
79.90	583.0
80.90	1993.0
81.80	566.0
85.90	143.0
86.90	1822.0
87.90	2030.0
90.80	170.0
91.90	1573.0
92.90	2230.0
94.00	6366.0
95.00	50840.0
96.00	3417.0
97.00	113.0
103.80	234.0
105.80	238.0
115.80	235.0
116.90	338.0
117.80	204.0
118.80	344.0
127.80	133.0
128.70	102.0
129.80	194.0
135.00	144.0
140.90	483.0
143.00	742.0
144.90	322.0
147.90	143.0
170.90	184.0
171.90	844.0
173.00	588.0
173.90	48184.0
175.00	3338.0
175.90	45920.0
177.00	2875.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.90	397.0
37.00	1983.0
38.00	2004.0
38.90	773.0
40.00	157.0
43.90	571.0
44.90	370.0
46.00	101.0
47.00	426.0
48.00	213.0
49.00	1948.0
50.00	8766.0
51.00	2630.0
55.00	141.0
56.00	639.0
57.00	1278.0
60.00	487.0
61.00	2289.0
62.00	2373.0
63.00	1790.0
63.90	245.0
64.90	494.0
66.90	109.0
68.00	4507.0
69.00	4331.0
70.00	382.0
72.00	340.0
73.00	2007.0
74.00	7703.0
75.00	24280.0
76.00	1910.0
76.90	334.0
77.80	121.0
78.90	1706.0
79.90	527.0
80.90	1932.0
81.80	503.0
86.00	121.0
86.90	1806.0
87.90	1974.0
90.80	187.0
91.90	1464.0
92.90	2127.0
94.00	6230.0
95.00	48672.0
96.00	3029.0
97.00	118.0
103.80	222.0
105.80	215.0
115.80	235.0
116.90	286.0
117.80	170.0
118.80	385.0
127.90	167.0
129.80	170.0
135.00	121.0
140.90	487.0
143.00	725.0
145.00	288.0
171.00	144.0
171.90	831.0
173.00	560.0
173.90	47368.0
175.00	3369.0
175.90	45648.0
177.00	2762.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064