

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
 Data File : VU053690.D
 Acq On : 13 Apr 2023 18:31
 Operator : JC/MD
 Sample : 02299-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	68	79	95	rBV	87987	114042	2.41%	0.826%
2	1.909	169	177	199	rVB	59708	96217	2.03%	0.697%
3	2.572	367	383	407	rBV	2883033	4729902	100.00%	34.279%
4	3.861	765	784	814	rVB	1049345	2447664	51.75%	17.739%
5	4.620	1005	1020	1045	rBV	72414	180619	3.82%	1.309%
6	5.054	1141	1155	1178	rVB	95086	210908	4.46%	1.529%
7	5.311	1216	1235	1260	rBV	1034440	2328560	49.23%	16.876%
8	5.719	1340	1362	1380	rBV3	187794	483628	10.22%	3.505%
9	6.243	1511	1525	1556	rBV	188090	360445	7.62%	2.612%
10	6.536	1603	1616	1634	rBV2	48319	91200	1.93%	0.661%
11	6.687	1648	1663	1679	rBV2	113689	222607	4.71%	1.613%
12	7.562	1923	1935	1952	rBV	55932	97104	2.05%	0.704%
13	7.893	2026	2038	2055	rBV	235014	409235	8.65%	2.966%
14	8.176	2113	2126	2145	rBV	33633	59516	1.26%	0.431%
15	8.629	2255	2267	2295	rBV	257845	466241	9.86%	3.379%
16	9.414	2496	2511	2535	rBV	261317	439266	9.29%	3.183%
17	10.751	2916	2927	2942	rBV	93675	150562	3.18%	1.091%
18	11.809	3243	3256	3274	rBV	272549	440094	9.30%	3.189%
19	12.092	3332	3344	3361	rBV	61768	96858	2.05%	0.702%
20	12.189	3361	3374	3392	rBV2	225336	373567	7.90%	2.707%




Sum of corrected areas: 13798235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053690.D
Acq On : 13 Apr 2023 18:31
Operator : JC/MD
Sample : 02299-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

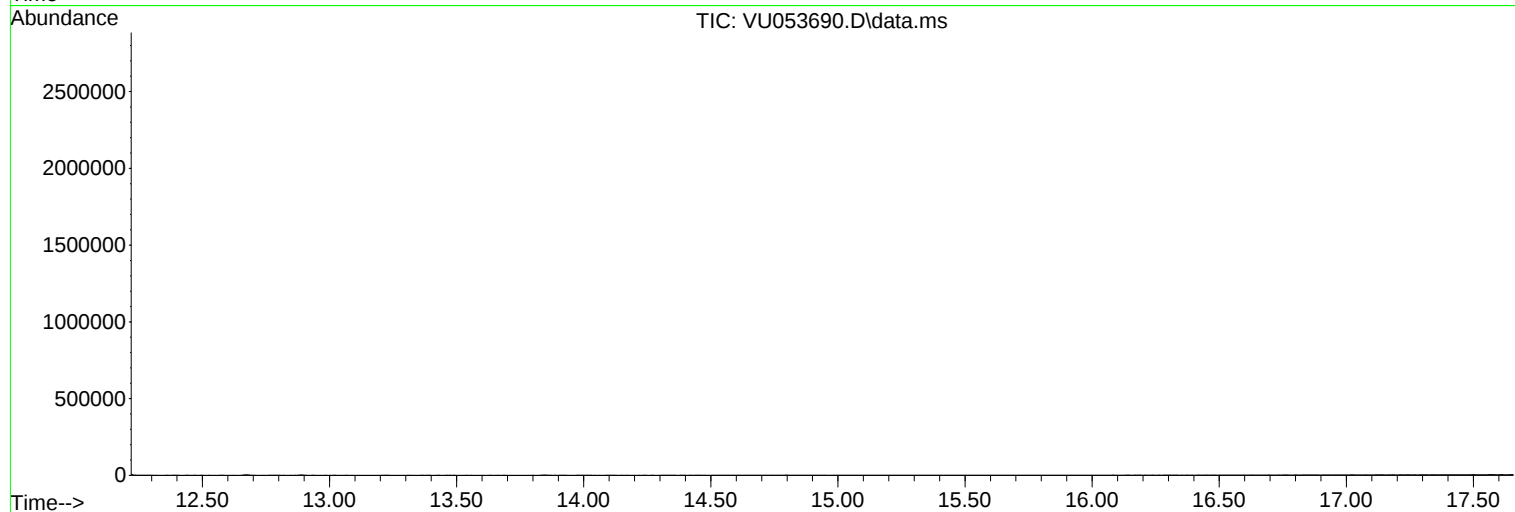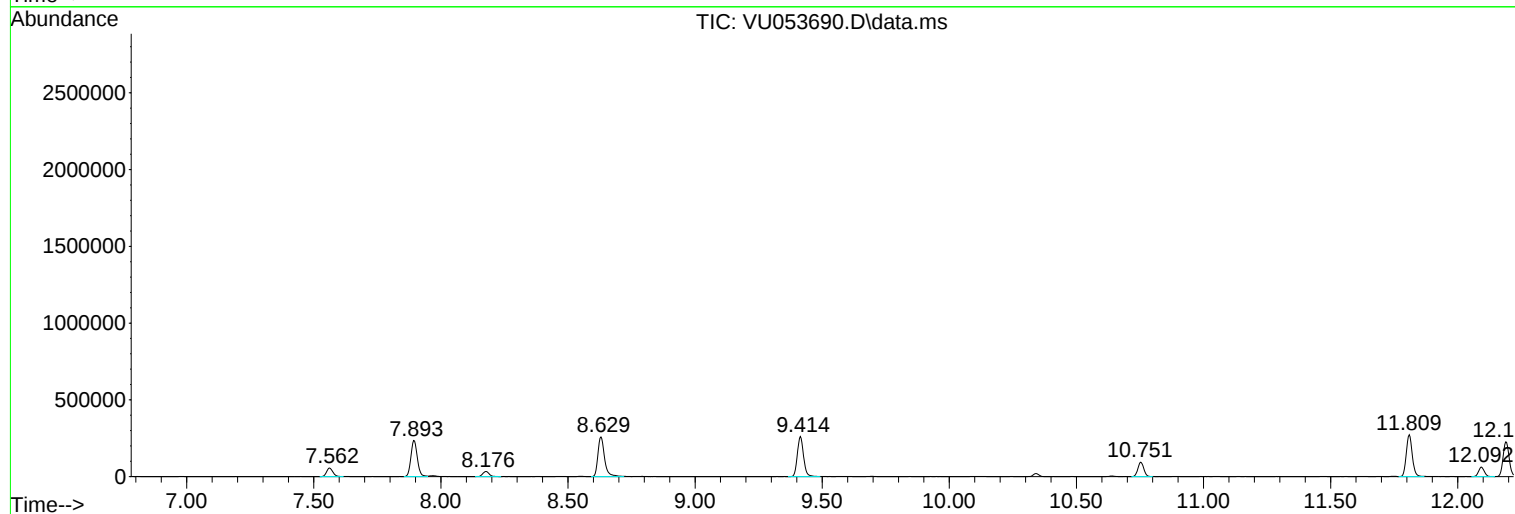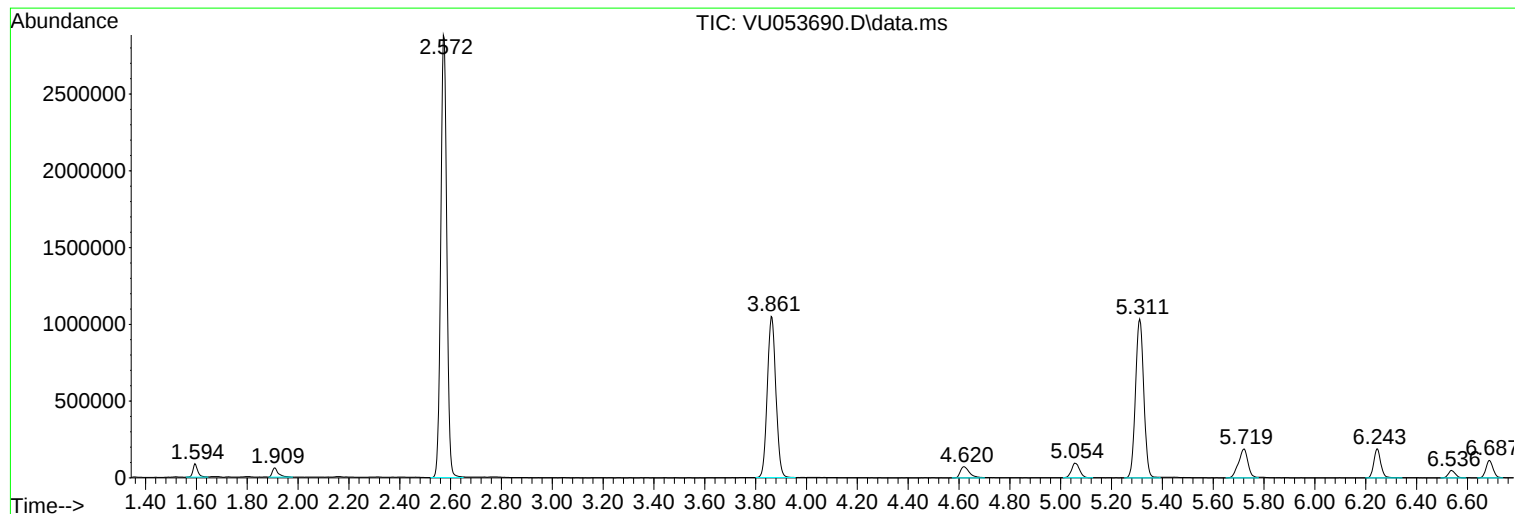

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053690.D
Acq On : 13 Apr 2023 18:31
Operator : JC/MD
Sample : 02299-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.092	1.10 ug/L	96858	1,4-Dichlorobenzene-d4	11.809

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 1,2,2,4-tetrachloro-	194	C4H6Cl4	042525-60-0	40
2			Methyl 3,3-dichloropropenoate	154	C4H4Cl2O2	002257-46-7	27
3			Cyclopropane, 1,1-dichloro-2-chl...	172	C5H7Cl3	015997-19-0	25
4			4-Pyridinecarboxaldehyde N-oxide	123	C6H5NO2	007216-42-4	12
5			Benzoyl chloride, 2-fluoro-	158	C7H4ClFO	000393-52-2	12

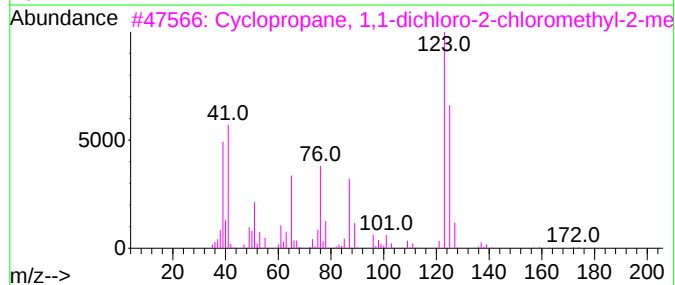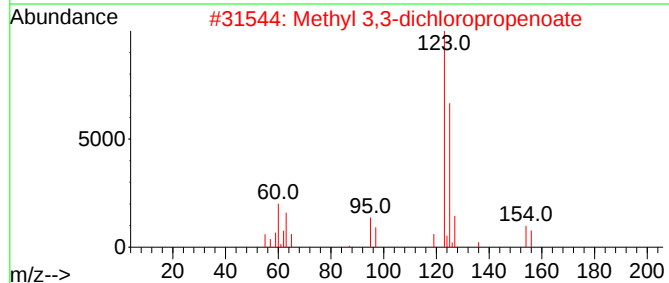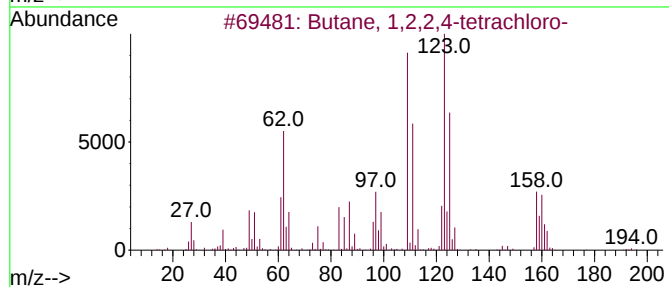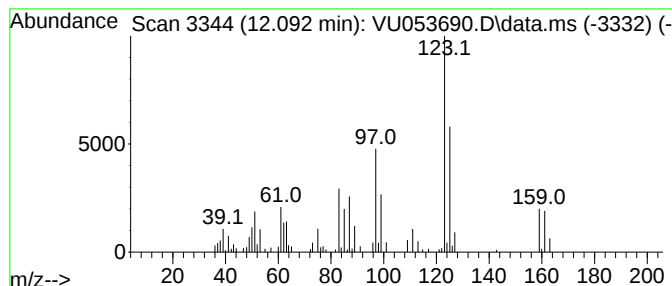

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053690.D
Acq On : 13 Apr 2023 18:31
Operator : JC/MD
Sample : 02299-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	12.092	1.1	ug/L	96858	3	11.809	440094	5.0