

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
 Data File : VU053694.D
 Acq On : 13 Apr 2023 20:10
 Operator : JC/MD
 Sample : 02340-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	96	rBV	66689	82117	20.39%	2.263%
2	1.909	168	177	189	rBV	50286	69960	17.37%	1.928%
3	2.562	368	380	393	rBV	102235	169730	42.15%	4.677%
4	2.626	393	400	412	rVB	2791	4566	1.13%	0.126%
5	4.623	1009	1021	1046	rBV	57650	139924	34.75%	3.856%
6	5.060	1138	1157	1179	rVB2	83261	183088	45.47%	5.045%
7	5.314	1223	1236	1252	rVB2	14288	30577	7.59%	0.843%
8	5.719	1343	1362	1384	rBV3	156259	402670	100.00%	11.097%
9	6.246	1514	1526	1543	rBV	157905	298869	74.22%	8.236%
10	6.687	1650	1663	1681	rBV	95733	188182	46.73%	5.186%
11	7.562	1923	1935	1950	rBV3	49199	85596	21.26%	2.359%
12	7.893	2025	2038	2055	rBV	203440	356131	88.44%	9.814%
13	7.967	2055	2061	2076	rVB3	5270	9408	2.34%	0.259%
14	8.176	2115	2126	2144	rBV2	29551	50831	12.62%	1.401%
15	8.629	2256	2267	2299	rBV	201819	364314	90.47%	10.040%
16	9.414	2496	2511	2532	rBV	220268	374962	93.12%	10.333%
17	10.751	2915	2927	2941	rBV	71901	117018	29.06%	3.225%
18	10.893	2960	2971	2985	rVB3	3364	4961	1.23%	0.137%
19	11.809	3244	3256	3274	rBV	242996	389315	96.68%	10.729%
20	12.192	3360	3375	3389	rBV	188256	306533	76.13%	8.447%




Sum of corrected areas: 3628752

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053694.D
Acq On : 13 Apr 2023 20:10
Operator : JC/MD
Sample : 02340-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

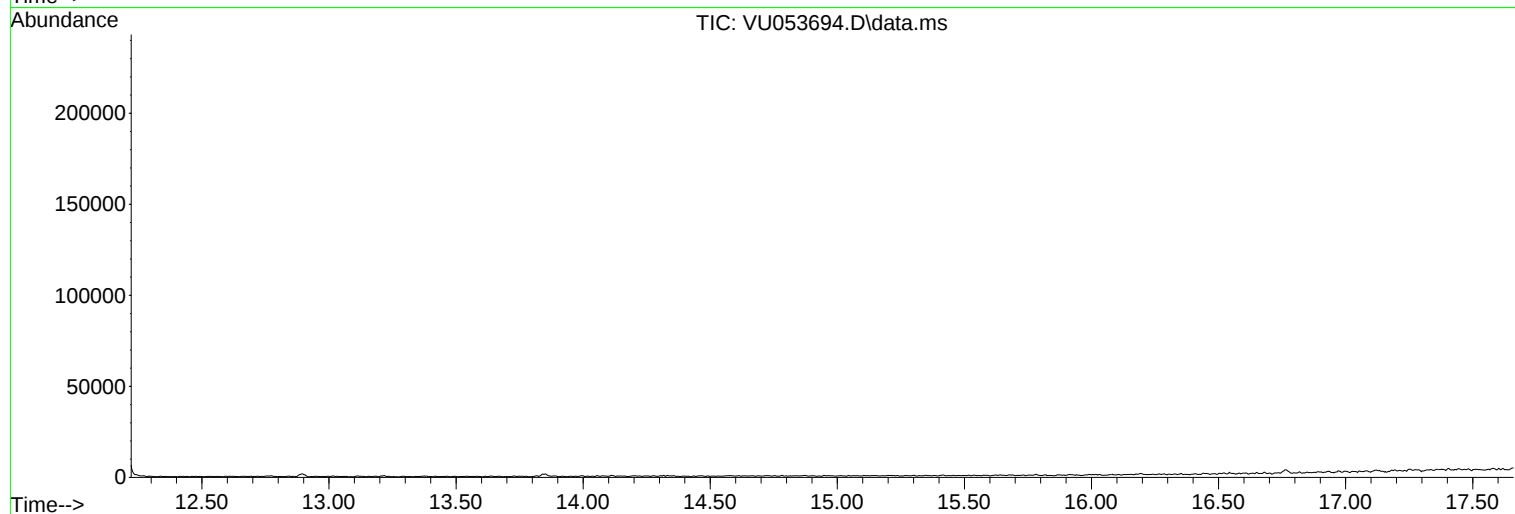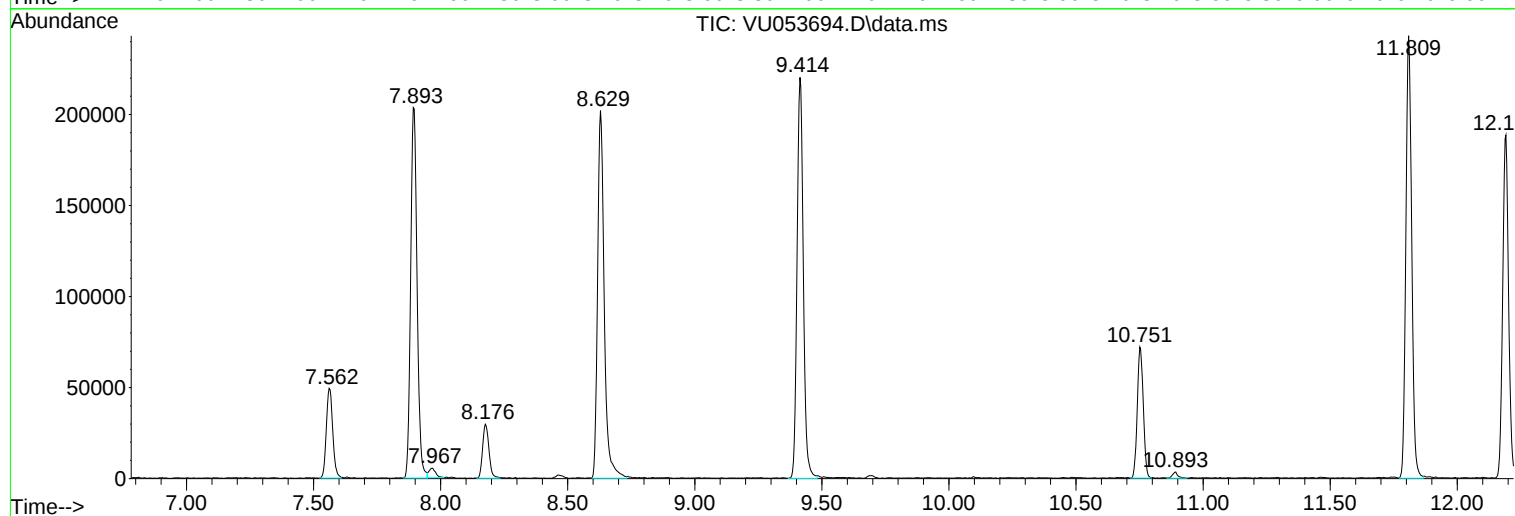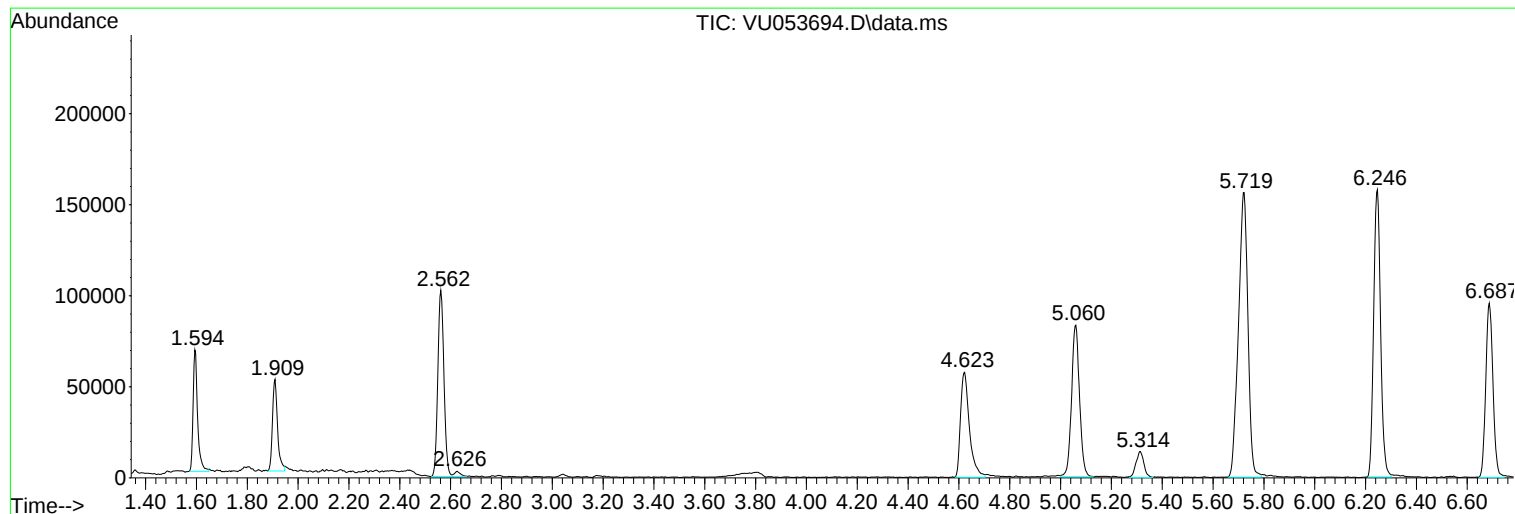

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053694.D
Acq On : 13 Apr 2023 20:10
Operator : JC/MD
Sample : 02340-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053694.D
Acq On : 13 Apr 2023 20:10
Operator : JC/MD
Sample : 02340-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc