

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
 Data File : VU053706.D
 Acq On : 14 Apr 2023 11:17
 Operator : JC/MD
 Sample : 02254-20DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	69160	83910	6.86%	1.600%
2	1.913	170	178	189	rBV	55778	72046	5.89%	1.374%
3	2.575	368	384	401	rBV4	276409	517643	42.32%	9.873%
4	3.179	560	572	588	rBV2	6238	13451	1.10%	0.257%
5	3.861	772	784	798	rVB3	9939	25962	2.12%	0.495%
6	4.633	1010	1024	1057	rBV2	45461	137993	11.28%	2.632%
7	5.060	1142	1157	1181	rVB	86229	190154	15.55%	3.627%
8	5.311	1215	1235	1256	rBV	543544	1223040	100.00%	23.326%
9	5.723	1342	1363	1386	rBV3	163338	426035	34.83%	8.126%
10	6.247	1512	1526	1542	rBV	168089	321377	26.28%	6.129%
11	6.687	1648	1663	1678	rBV2	98529	193840	15.85%	3.697%
12	7.562	1922	1935	1953	rBV2	50628	87979	7.19%	1.678%
13	7.893	2026	2038	2057	rBV	209511	370627	30.30%	7.069%
14	8.176	2116	2126	2140	rBV2	30221	51739	4.23%	0.987%
15	8.629	2253	2267	2298	rBV	179194	332203	27.16%	6.336%
16	9.414	2499	2511	2530	rBV	230170	389702	31.86%	7.433%
17	10.751	2916	2927	2943	rVB	71761	113624	9.29%	2.167%
18	11.809	3243	3256	3275	rBV	235730	387191	31.66%	7.385%
19	12.189	3359	3374	3395	rBV	185162	304641	24.91%	5.810%




Sum of corrected areas: 5243157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053706.D
Acq On : 14 Apr 2023 11:17
Operator : JC/MD
Sample : 02254-20DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

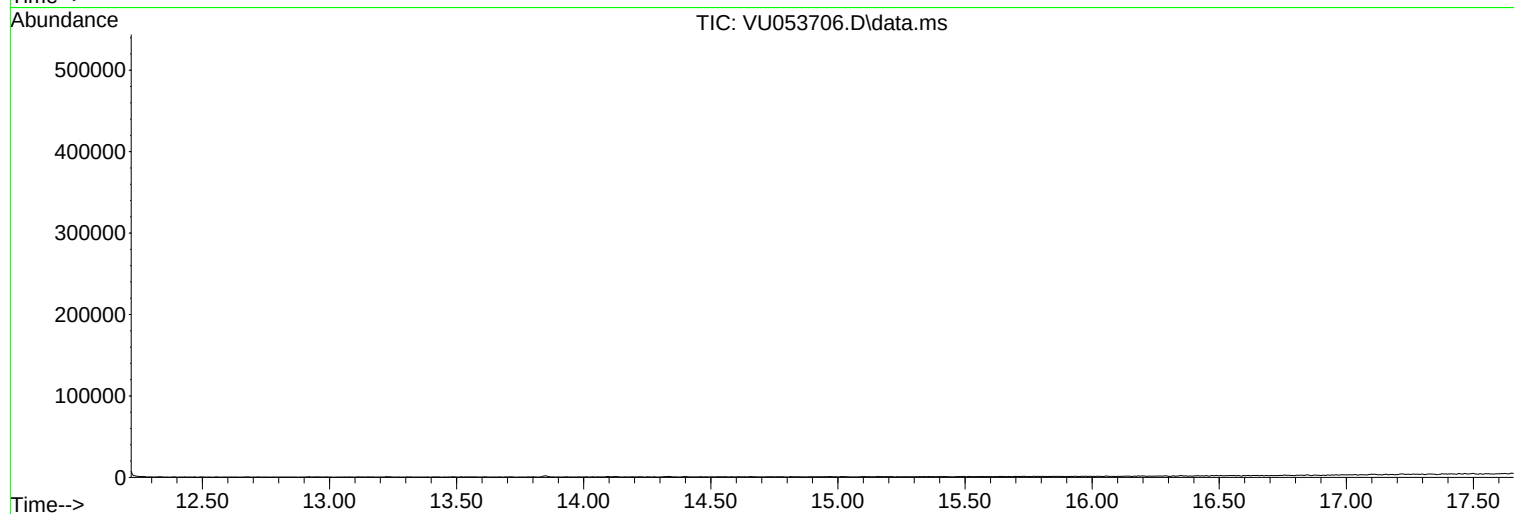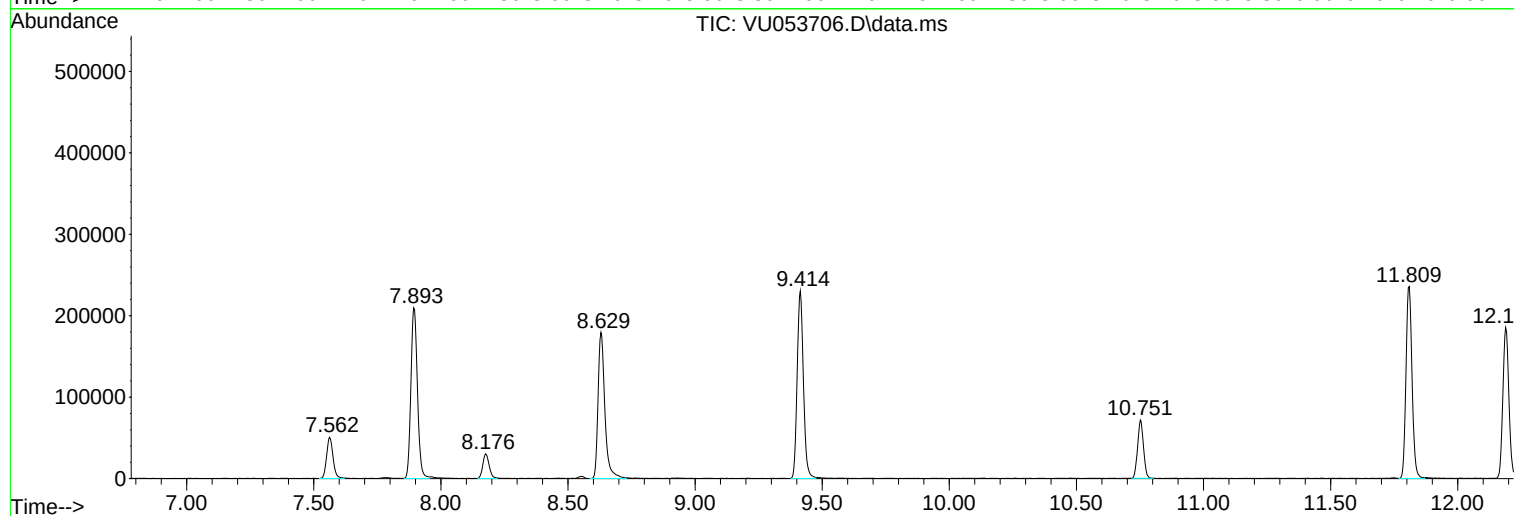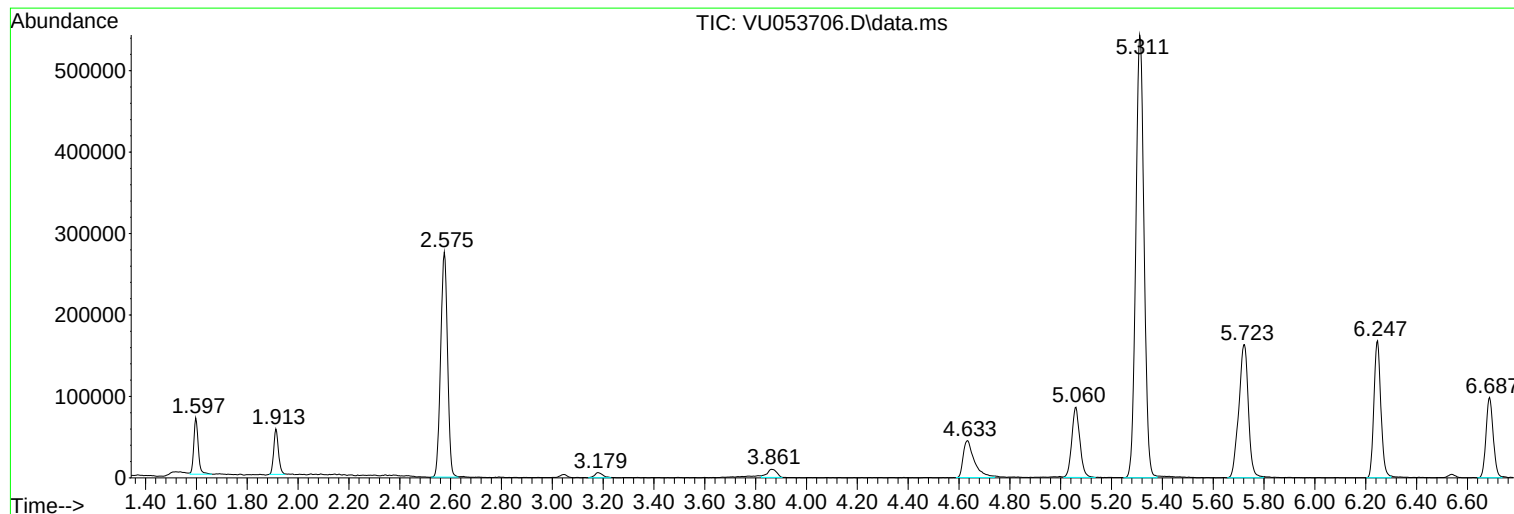

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053706.D
Acq On : 14 Apr 2023 11:17
Operator : JC/MD
Sample : 02254-20DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053706.D
Acq On : 14 Apr 2023 11:17
Operator : JC/MD
Sample : 02254-20DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc