

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
 Data File : VU053717.D
 Acq On : 14 Apr 2023 16:38
 Operator : JC/MD
 Sample : 02254-14DL 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AC5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rBV	68112	82071	9.98%	1.676%
2	1.912	169	178	192	rBV	56764	78171	9.50%	1.596%
3	2.572	369	383	402	rBV4	233024	448419	54.52%	9.156%
4	3.864	772	785	804	rVB2	38430	91618	11.14%	1.871%
5	4.629	1009	1023	1056	rBV	52261	150094	18.25%	3.065%
6	5.057	1141	1156	1179	rVB2	86586	194806	23.68%	3.978%
7	5.311	1217	1235	1255	rBV	362828	822516	100.00%	16.795%
8	5.723	1342	1363	1379	rBV2	170111	435677	52.97%	8.896%
9	6.243	1512	1525	1544	rBV	157749	297997	36.23%	6.085%
10	6.539	1606	1617	1630	rVB7	7835	14827	1.80%	0.303%
11	6.687	1649	1663	1681	rBV	102618	202649	24.64%	4.138%
12	7.562	1922	1935	1949	rBV2	52238	91961	11.18%	1.878%
13	7.893	2026	2038	2066	rBV	213153	376074	45.72%	7.679%
14	8.176	2114	2126	2149	rBV	33072	55647	6.77%	1.136%
15	8.629	2253	2267	2302	rBV	216401	390592	47.49%	7.976%
16	9.414	2498	2511	2538	rBV	213458	360421	43.82%	7.359%
17	10.751	2912	2927	2945	rBV	76874	125358	15.24%	2.560%
18	11.809	3244	3256	3277	rBV	229442	365020	44.38%	7.453%
19	12.189	3362	3374	3396	rBV	189921	313474	38.11%	6.401%




Sum of corrected areas: 4897392

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053717.D
Acq On : 14 Apr 2023 16:38
Operator : JC/MD
Sample : 02254-14DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

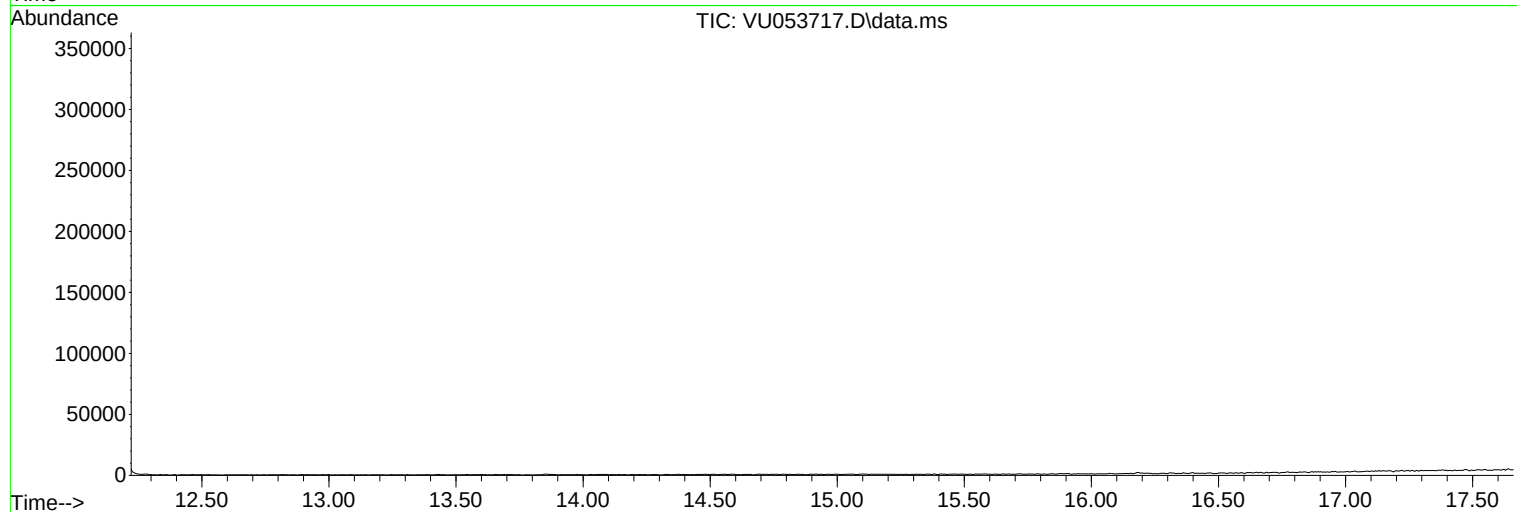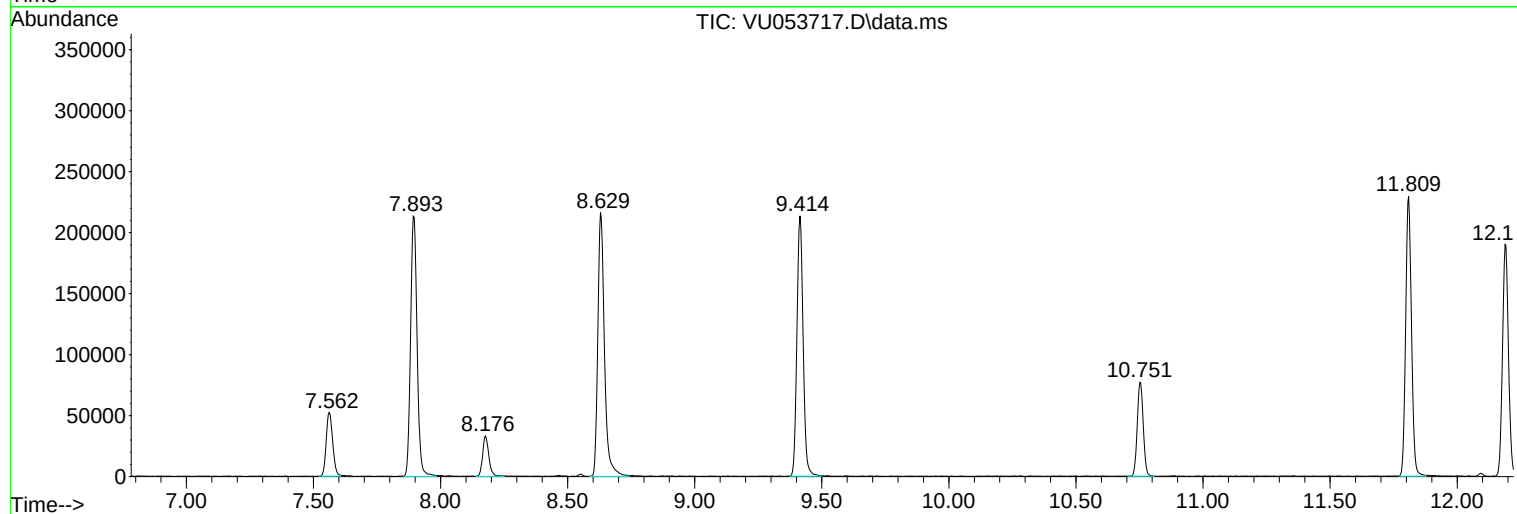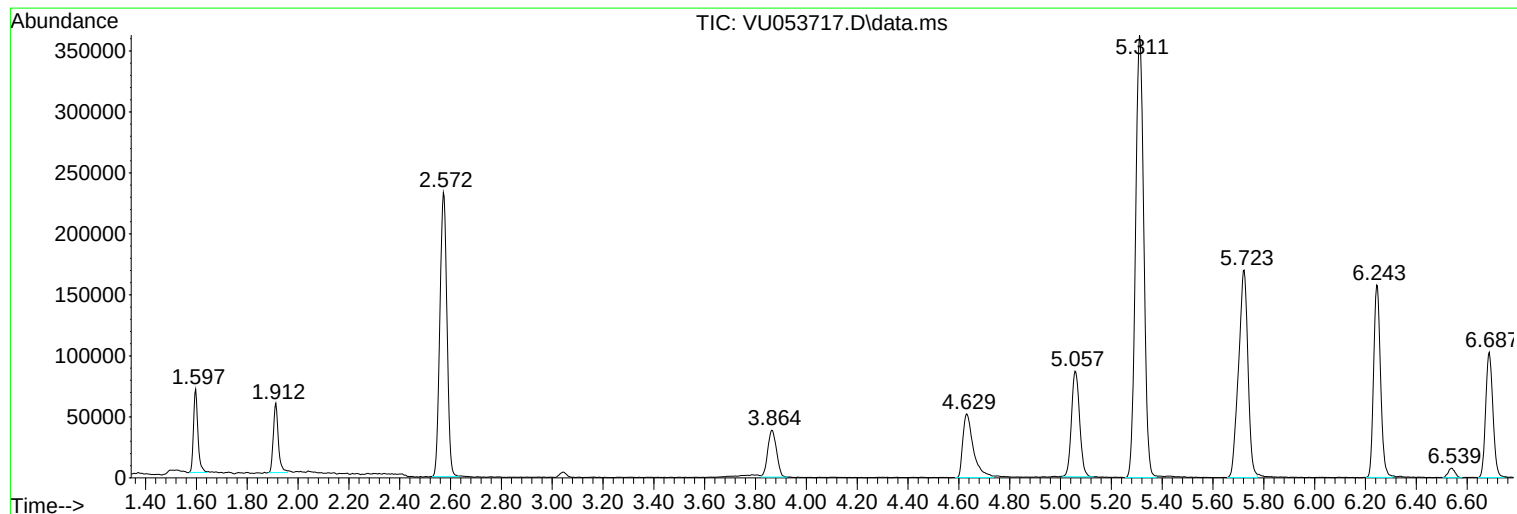

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053717.D
Acq On : 14 Apr 2023 16:38
Operator : JC/MD
Sample : 02254-14DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053717.D
Acq On : 14 Apr 2023 16:38
Operator : JC/MD
Sample : 02254-14DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------