

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
 Data File : VU053722.D
 Acq On : 14 Apr 2023 18:41
 Operator : JC/MD
 Sample : 02340-06DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE08DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rBV	63187	75727	19.07%	1.882%
2	1.912	169	178	195	rBV	51627	73828	18.59%	1.835%
3	2.568	367	382	400	rVB3	111754	204882	51.59%	5.092%
4	3.044	520	530	541	rBV3	4538	8127	2.05%	0.202%
5	3.864	776	785	806	rVB2	7038	16113	4.06%	0.400%
6	4.633	1011	1024	1055	rBV	50663	163829	41.25%	4.072%
7	5.060	1141	1157	1175	rVB	81948	180270	45.39%	4.480%
8	5.317	1227	1237	1247	rVB6	3008	5984	1.51%	0.149%
9	5.723	1343	1363	1382	rBV2	154233	397155	100.00%	9.871%
10	6.247	1512	1526	1546	rBV	157122	302877	76.26%	7.528%
11	6.539	1602	1617	1635	rBV2	146457	278730	70.18%	6.928%
12	6.687	1651	1663	1687	rVB	93151	184060	46.34%	4.575%
13	7.565	1924	1936	1948	rBV2	48009	83078	20.92%	2.065%
14	7.896	2023	2039	2063	rBV	198965	347189	87.42%	8.629%
15	8.179	2116	2127	2141	rBV	28566	47823	12.04%	1.189%
16	8.552	2231	2243	2256	rBV2	91339	154293	38.85%	3.835%
17	8.629	2256	2267	2294	rVV	197881	354671	89.30%	8.815%
18	9.414	2499	2511	2534	rBV	223820	367124	92.44%	9.124%
19	10.751	2916	2927	2944	rBV	72086	117826	29.67%	2.928%
20	11.809	3244	3256	3273	rBV	230939	368417	92.76%	9.157%
21	12.189	3362	3374	3394	rBV	180886	291495	73.40%	7.245%




Sum of corrected areas: 4023498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053722.D
Acq On : 14 Apr 2023 18:41
Operator : JC/MD
Sample : 02340-06DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

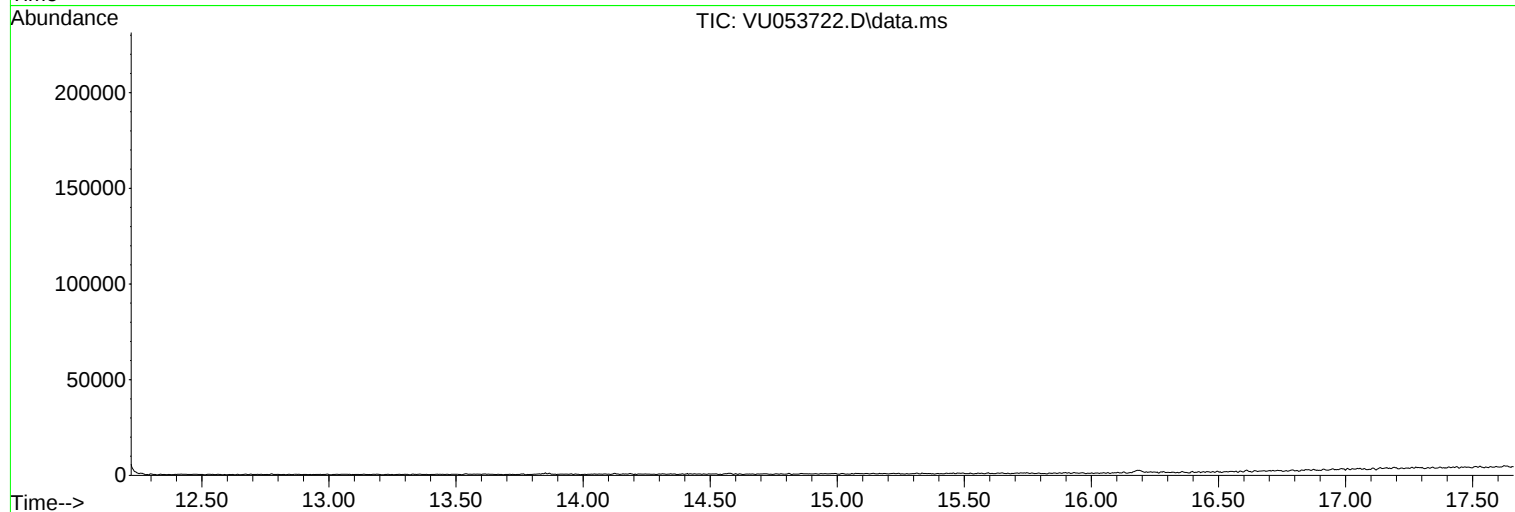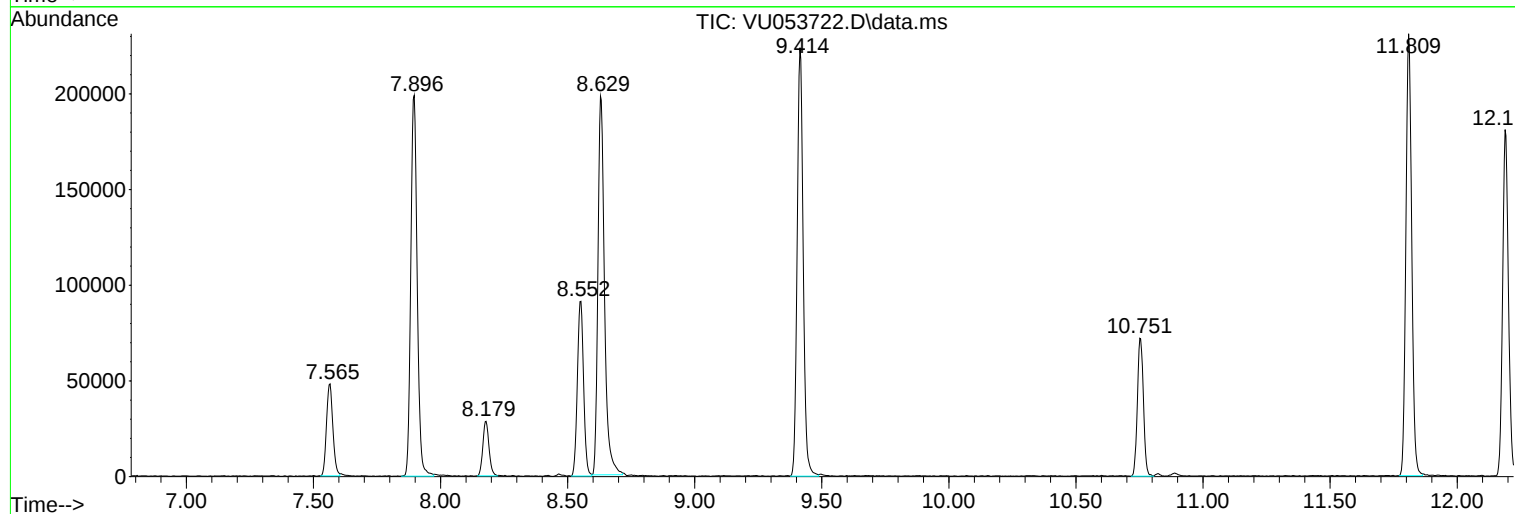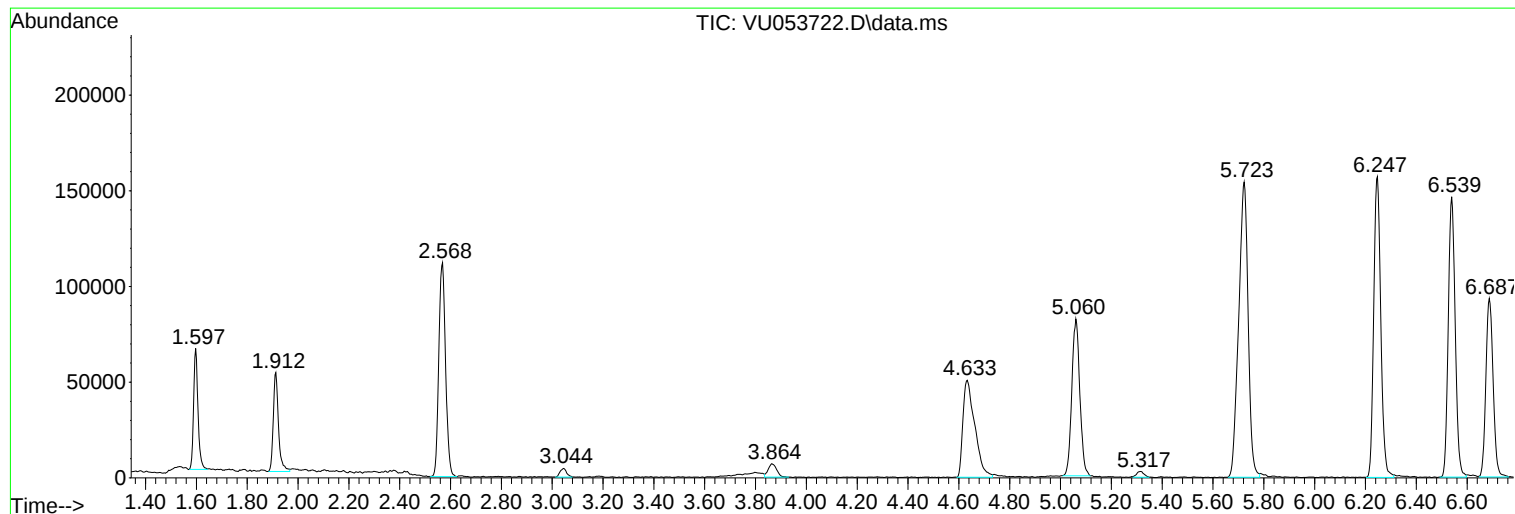

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053722.D
Acq On : 14 Apr 2023 18:41
Operator : JC/MD
Sample : 02340-06DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053722.D
Acq On : 14 Apr 2023 18:41
Operator : JC/MD
Sample : 02340-06DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc