


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053683.D
Acq On : 13 Apr 2023 13:56
Operator : JC/MD
Sample : BFB002
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB002

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 18 00:19:36 2023

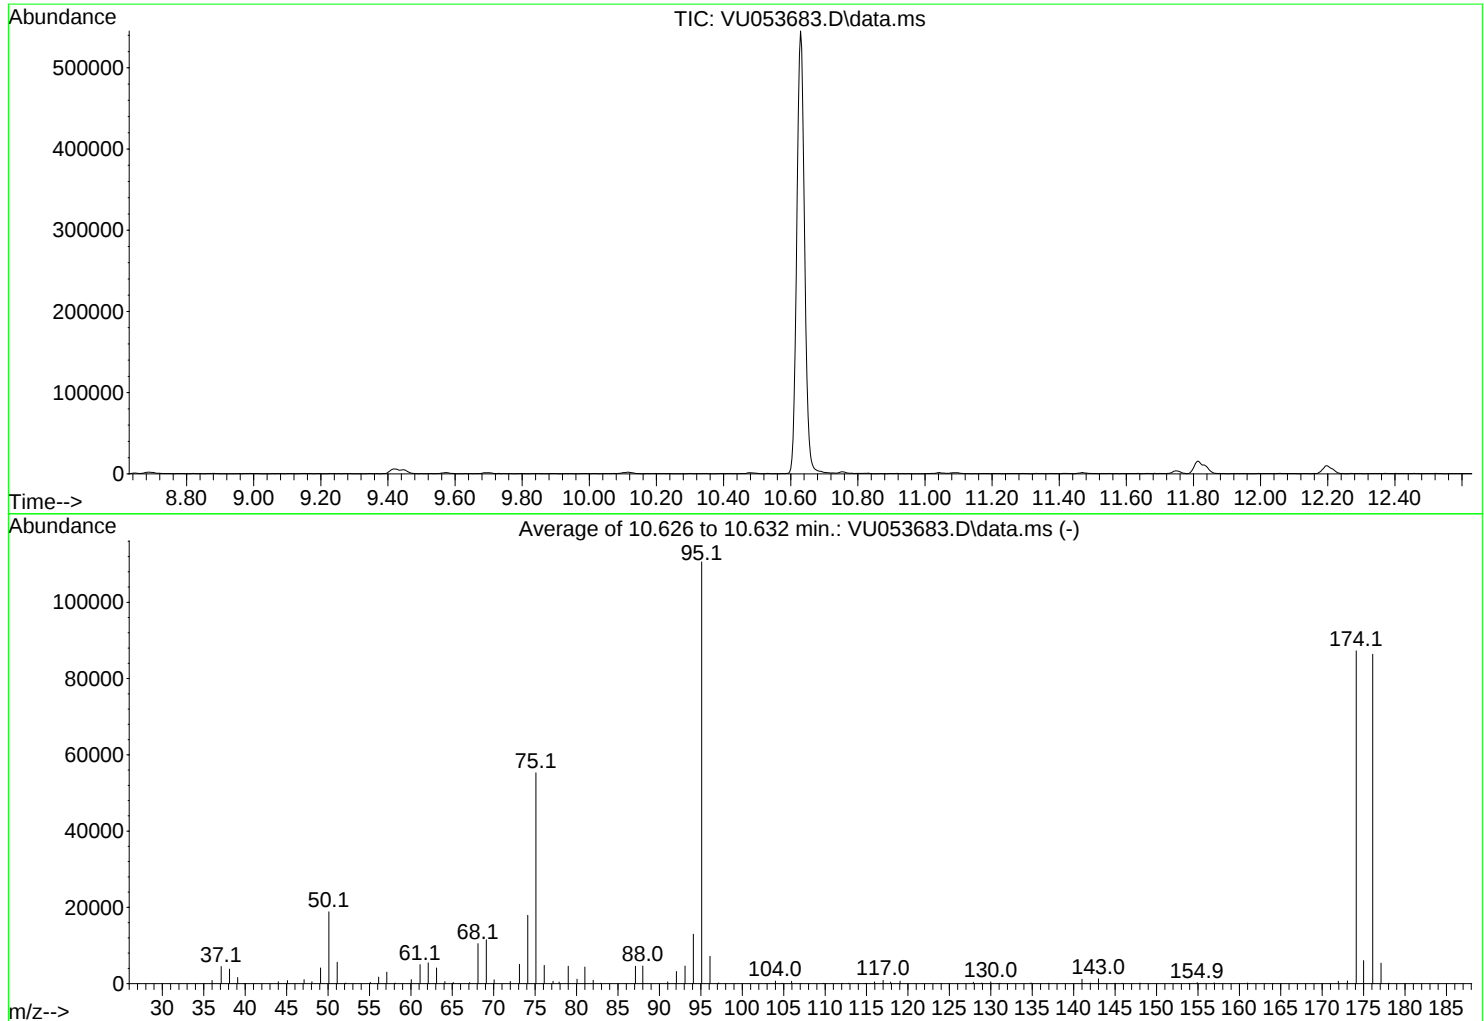

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	18851	PASS
75	95	30	80	50.0	55307	PASS
95	95	100	100	100.0	110616	PASS
96	95	5	9	6.5	7199	PASS
173	174	0.00	2	0.8	700	PASS
174	95	50	120	78.9	87291	PASS
175	174	5	9	6.9	6037	PASS
176	174	95	101	99.0	86384	PASS
177	176	5	9	6.2	5367	PASS

m/z	Abundance
39.90	109.0
44.00	273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
36.00	831.0
37.10	4407.0
38.10	3986.0
39.10	1513.0
39.90	131.0
44.10	905.0
45.10	834.0
47.10	1015.0
48.10	442.0
49.10	4063.0
50.10	18424.0
51.10	5469.0
52.10	191.0
55.10	356.0
56.10	1619.0
57.10	3127.0
58.10	171.0
60.10	1073.0
61.10	5105.0
62.10	5522.0
63.10	4214.0
64.10	536.0
65.10	273.0
67.10	310.0
68.10	10579.0
69.10	11671.0
70.10	890.0
72.00	606.0
73.10	5147.0
74.10	17512.0
75.10	54456.0
76.10	5130.0
77.20	527.0
77.90	365.0
79.00	4643.0
80.10	1086.0
81.00	4226.0
82.00	916.0
82.90	144.0
87.10	4208.0
88.00	4582.0
91.10	411.0
92.10	2931.0
93.10	4520.0
94.10	12692.0
95.10	108104.0
96.10	7080.0
97.20	228.0
102.90	102.0
104.00	771.0
104.80	158.0
106.00	566.0
112.10	155.0
112.80	120.0
116.00	385.0
117.00	815.0
117.90	392.0
119.00	673.0
127.90	348.0
128.90	148.0
130.00	452.0
130.80	147.0
131.10	157.0
134.80	258.0
137.00	108.0
141.00	1087.0
142.00	192.0
143.00	1218.0
144.90	164.0
145.90	117.0
148.10	190.0
153.90	103.0
154.90	308.0
157.00	198.0
161.00	127.0
171.90	526.0
173.00	611.0
174.10	83528.0
175.00	6114.0
176.10	82504.0
177.10	5333.0
178.10	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
36.00	895.0
37.10	4636.0
38.10	4000.0
39.10	1618.0
39.90	139.0
44.10	775.0
45.10	831.0
47.10	1099.0
48.00	476.0
49.10	4262.0
50.10	19616.0
51.10	5767.0
52.20	173.0
55.10	330.0
56.10	1786.0
57.10	3108.0
58.10	194.0
60.10	1102.0
61.10	5163.0
62.10	5626.0
63.10	4293.0
64.10	559.0
65.10	335.0
67.10	290.0
68.10	10742.0
69.10	11802.0
70.00	1059.0
72.00	624.0
73.10	5172.0
74.10	18384.0
75.10	57008.0
76.10	4882.0
77.10	668.0
77.90	421.0
79.00	4696.0
80.10	1191.0
81.00	4469.0
82.00	894.0
82.90	117.0
87.10	4711.0
88.00	4790.0
91.00	431.0
92.00	3290.0
93.10	4776.0
94.10	13275.0
95.10	114304.0
96.10	7366.0
97.20	217.0
104.00	711.0
104.80	153.0
105.90	651.0
107.10	128.0
109.80	123.0
112.10	130.0
112.80	142.0
114.90	135.0
115.90	463.0
117.00	911.0
117.90	403.0
119.10	701.0
124.00	113.0
127.90	387.0
128.90	169.0
130.00	515.0
131.10	159.0
134.80	247.0
137.00	123.0
141.00	1218.0
142.00	200.0
143.00	1309.0
145.00	139.0
145.90	111.0
148.00	181.0
153.90	108.0
154.90	295.0
156.90	202.0
161.00	175.0
171.90	638.0
173.00	741.0
174.10	90440.0
175.00	6192.0
176.10	89080.0
177.10	5427.0
178.00	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
36.00	812.0
37.10	4449.0
38.10	3476.0
39.10	1609.0
39.90	126.0
44.00	711.0
45.10	766.0
47.10	1071.0
48.00	546.0
49.10	3971.0
50.10	18512.0
51.10	5575.0
52.20	146.0
55.10	284.0
56.10	1753.0
57.10	2789.0
58.10	163.0
60.00	999.0
61.10	4756.0
62.10	5249.0
63.10	3853.0
64.10	490.0
65.10	395.0
67.10	273.0
68.10	10178.0
69.10	11044.0
70.10	1055.0
72.00	555.0
73.10	4913.0
74.10	17880.0
75.10	54456.0
76.10	4384.0
77.10	673.0
77.90	465.0
79.00	4383.0
80.00	1239.0
81.00	4351.0
82.00	789.0
82.90	100.0
87.10	4838.0
88.00	4545.0
90.90	493.0
92.10	3303.0
93.10	4536.0
94.10	12992.0
95.10	109440.0
96.10	7150.0
97.00	187.0
104.00	574.0
104.80	132.0
105.90	691.0
107.10	112.0
109.80	109.0
111.00	128.0
112.80	143.0
114.90	141.0
115.90	528.0
117.00	901.0
117.90	429.0
119.10	673.0
124.00	136.0
127.90	362.0
128.90	177.0
130.00	469.0
131.10	119.0
134.90	198.0
136.90	165.0
141.00	1200.0
142.10	151.0
143.00	1300.0
145.10	102.0
145.80	112.0
147.90	187.0
154.90	264.0
157.00	185.0
161.00	160.0
172.00	699.0
173.10	749.0
174.10	87904.0
175.00	5804.0
176.10	87568.0
177.10	5342.0
178.00	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002