


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041423\
Data File : VU053702.D
Acq On : 14 Apr 2023 09:02
Operator : JC/MD
Sample : BFB003
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB003

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 18 00:19:36 2023

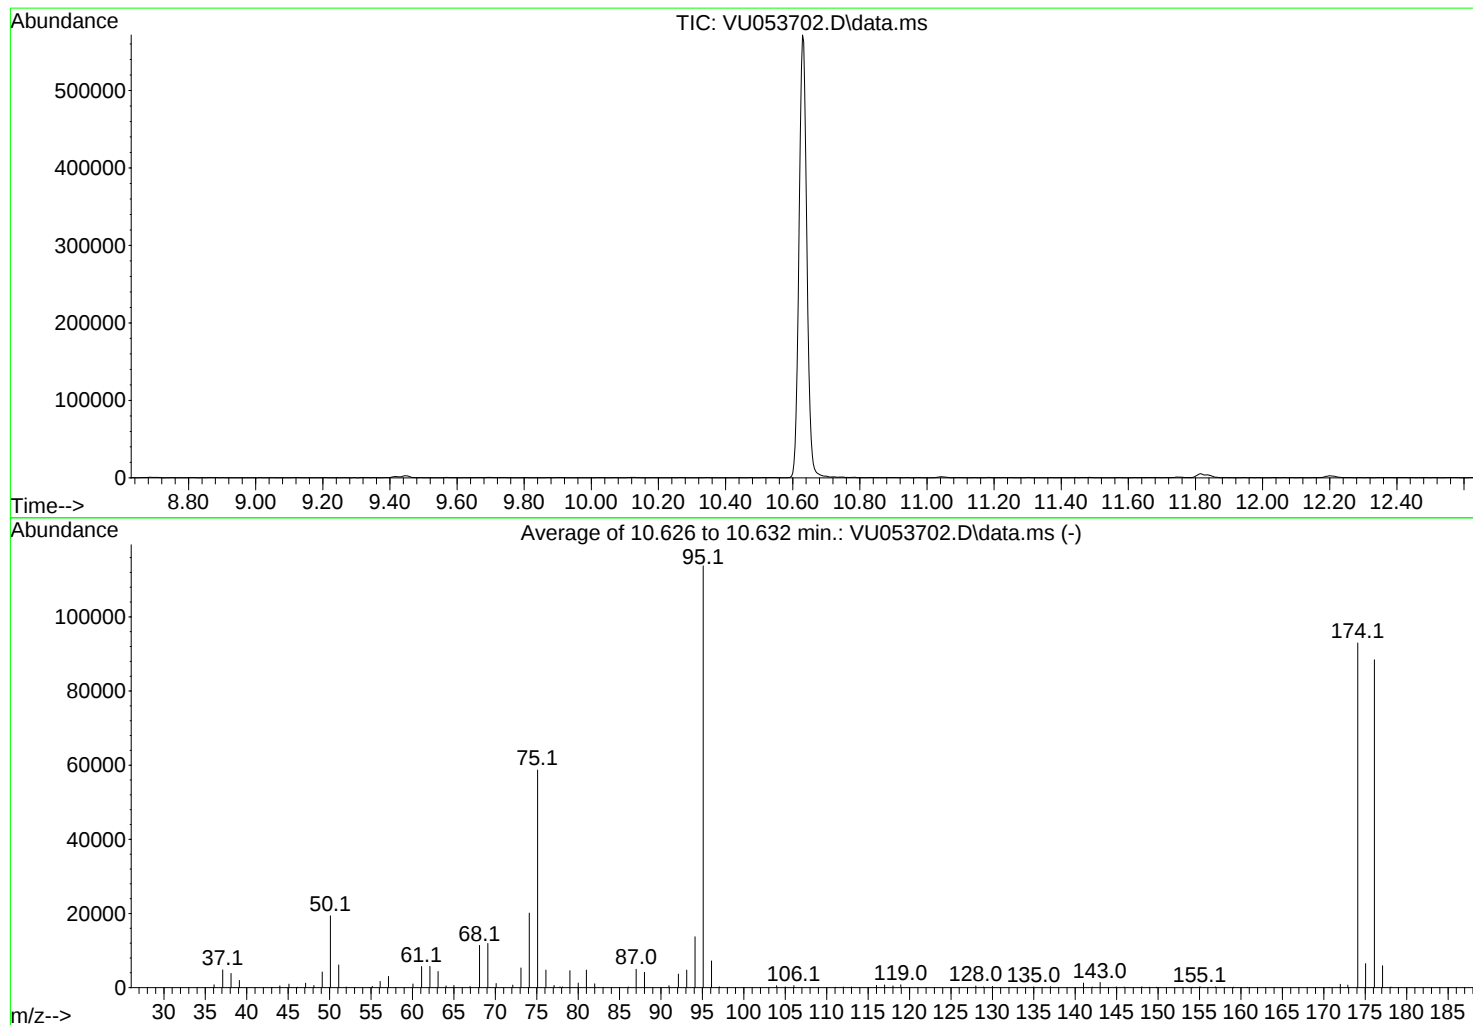

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	19392	PASS
75	95	30	80	51.6	58677	PASS
95	95	100	100	100.0	113765	PASS
96	95	5	9	6.3	7223	PASS
173	174	0.00	2	0.8	704	PASS
174	95	50	120	81.7	92965	PASS
175	174	5	9	7.0	6475	PASS
176	174	95	101	95.1	88445	PASS
177	176	5	9	6.7	5930	PASS

m/z	Abundance
44.00	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
36.10	783.0
37.10	4659.0
38.10	3961.0
39.10	1977.0
43.10	118.0
44.10	745.0
45.10	1000.0
46.10	149.0
47.10	1178.0
48.10	612.0
49.10	3969.0
50.10	18976.0
51.10	6172.0
52.00	200.0
55.10	374.0
56.10	1576.0
57.10	2993.0
60.10	934.0
61.10	5508.0
62.10	5678.0
63.10	4158.0
64.00	509.0
65.00	544.0
66.90	268.0
68.10	11035.0
69.10	11200.0
70.10	1154.0
72.10	619.0
73.10	5185.0
74.10	19392.0
75.10	56304.0
76.10	4765.0
77.10	651.0
77.80	369.0
79.00	4245.0
80.00	1200.0
81.00	4666.0
82.00	944.0
83.10	117.0
86.10	175.0
87.00	4789.0
88.00	4188.0
91.00	530.0
92.10	3493.0
93.10	4548.0
94.10	12860.0
95.10	107928.0
96.10	7253.0
97.10	179.0
104.00	534.0
105.00	148.0
106.10	516.0
111.10	123.0
112.00	167.0
113.00	109.0
116.00	573.0
117.00	717.0
118.00	469.0
118.90	788.0
128.00	511.0
128.90	218.0
130.00	311.0
135.00	146.0
137.00	270.0
141.00	1143.0
142.10	126.0
143.00	1366.0
145.00	205.0
145.90	202.0
148.10	207.0
148.90	120.0
149.80	127.0
154.10	116.0
155.00	257.0
157.00	208.0
170.60	126.0
172.00	839.0
172.90	745.0
174.10	86688.0
175.00	6234.0
176.10	82768.0
177.10	5803.0
178.10	206.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
36.10	828.0
37.10	4959.0
38.10	3805.0
39.10	1990.0
44.00	694.0
45.10	999.0
46.10	162.0
47.10	1216.0
48.10	570.0
49.10	4384.0
50.10	19856.0
51.10	6291.0
52.00	134.0
55.10	375.0
56.10	1788.0
57.10	3123.0
60.00	1045.0
61.10	5996.0
62.10	5918.0
63.10	4494.0
64.10	494.0
65.00	617.0
66.90	307.0
68.10	11806.0
69.10	12282.0
70.10	1171.0
72.10	716.0
73.10	5485.0
74.10	20808.0
75.10	60312.0
76.10	4851.0
77.10	607.0
77.80	319.0
78.10	350.0
79.00	4683.0
80.00	1323.0
81.00	4901.0
82.00	1105.0
83.00	129.0
86.10	213.0
87.00	5058.0
88.00	4255.0
91.00	525.0
92.10	3856.0
93.10	4865.0
94.10	14167.0
95.10	117392.0
96.10	7475.0
97.10	243.0
103.90	528.0
105.00	234.0
106.10	596.0
111.10	168.0
112.00	193.0
113.00	171.0
116.00	673.0
117.00	717.0
118.00	502.0
119.00	821.0
128.00	471.0
128.90	244.0
130.00	345.0
135.00	209.0
137.00	247.0
141.00	1331.0
142.00	165.0
143.00	1480.0
145.00	233.0
145.90	190.0
148.10	240.0
149.00	138.0
149.80	142.0
154.20	117.0
155.00	270.0
156.90	240.0
159.20	147.0
160.80	134.0
170.70	122.0
172.00	975.0
172.90	725.0
174.10	95840.0
175.10	6604.0
176.10	91160.0
177.10	6106.0
178.10	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
36.00	737.0
37.10	4720.0
38.10	3811.0
39.10	1861.0
44.00	689.0
45.10	919.0
46.10	103.0
47.10	1192.0
48.10	552.0
49.10	4386.0
50.10	19344.0
51.10	5958.0
52.00	137.0
55.20	334.0
56.10	1719.0
57.10	2998.0
58.00	130.0
60.00	1062.0
61.10	5653.0
62.10	5599.0
63.10	4429.0
64.10	476.0
65.00	627.0
67.00	282.0
68.10	11329.0
69.10	12299.0
70.10	998.0
72.10	687.0
73.10	5265.0
74.10	20104.0
75.10	59416.0
76.10	4611.0
77.10	559.0
78.10	324.0
79.00	4778.0
80.00	1250.0
81.00	4668.0
82.00	1104.0
86.10	176.0
87.00	5042.0
88.00	3938.0
90.90	502.0
92.10	3695.0
93.10	4785.0
94.10	14093.0
95.10	115976.0
96.10	6942.0
97.00	288.0
104.00	500.0
105.00	281.0
106.00	548.0
111.10	145.0
112.00	145.0
113.00	190.0
116.00	593.0
117.00	733.0
118.00	435.0
119.00	727.0
128.00	441.0
129.00	219.0
130.00	366.0
130.90	116.0
135.00	254.0
137.00	227.0
141.00	1292.0
142.00	187.0
143.00	1432.0
144.90	255.0
145.90	170.0
147.90	212.0
149.00	122.0
149.80	133.0
152.90	120.0
155.10	241.0
156.90	210.0
159.00	194.0
160.80	139.0
172.00	955.0
172.90	643.0
174.10	96368.0
175.10	6587.0
176.10	91408.0
177.10	5881.0
178.10	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003