



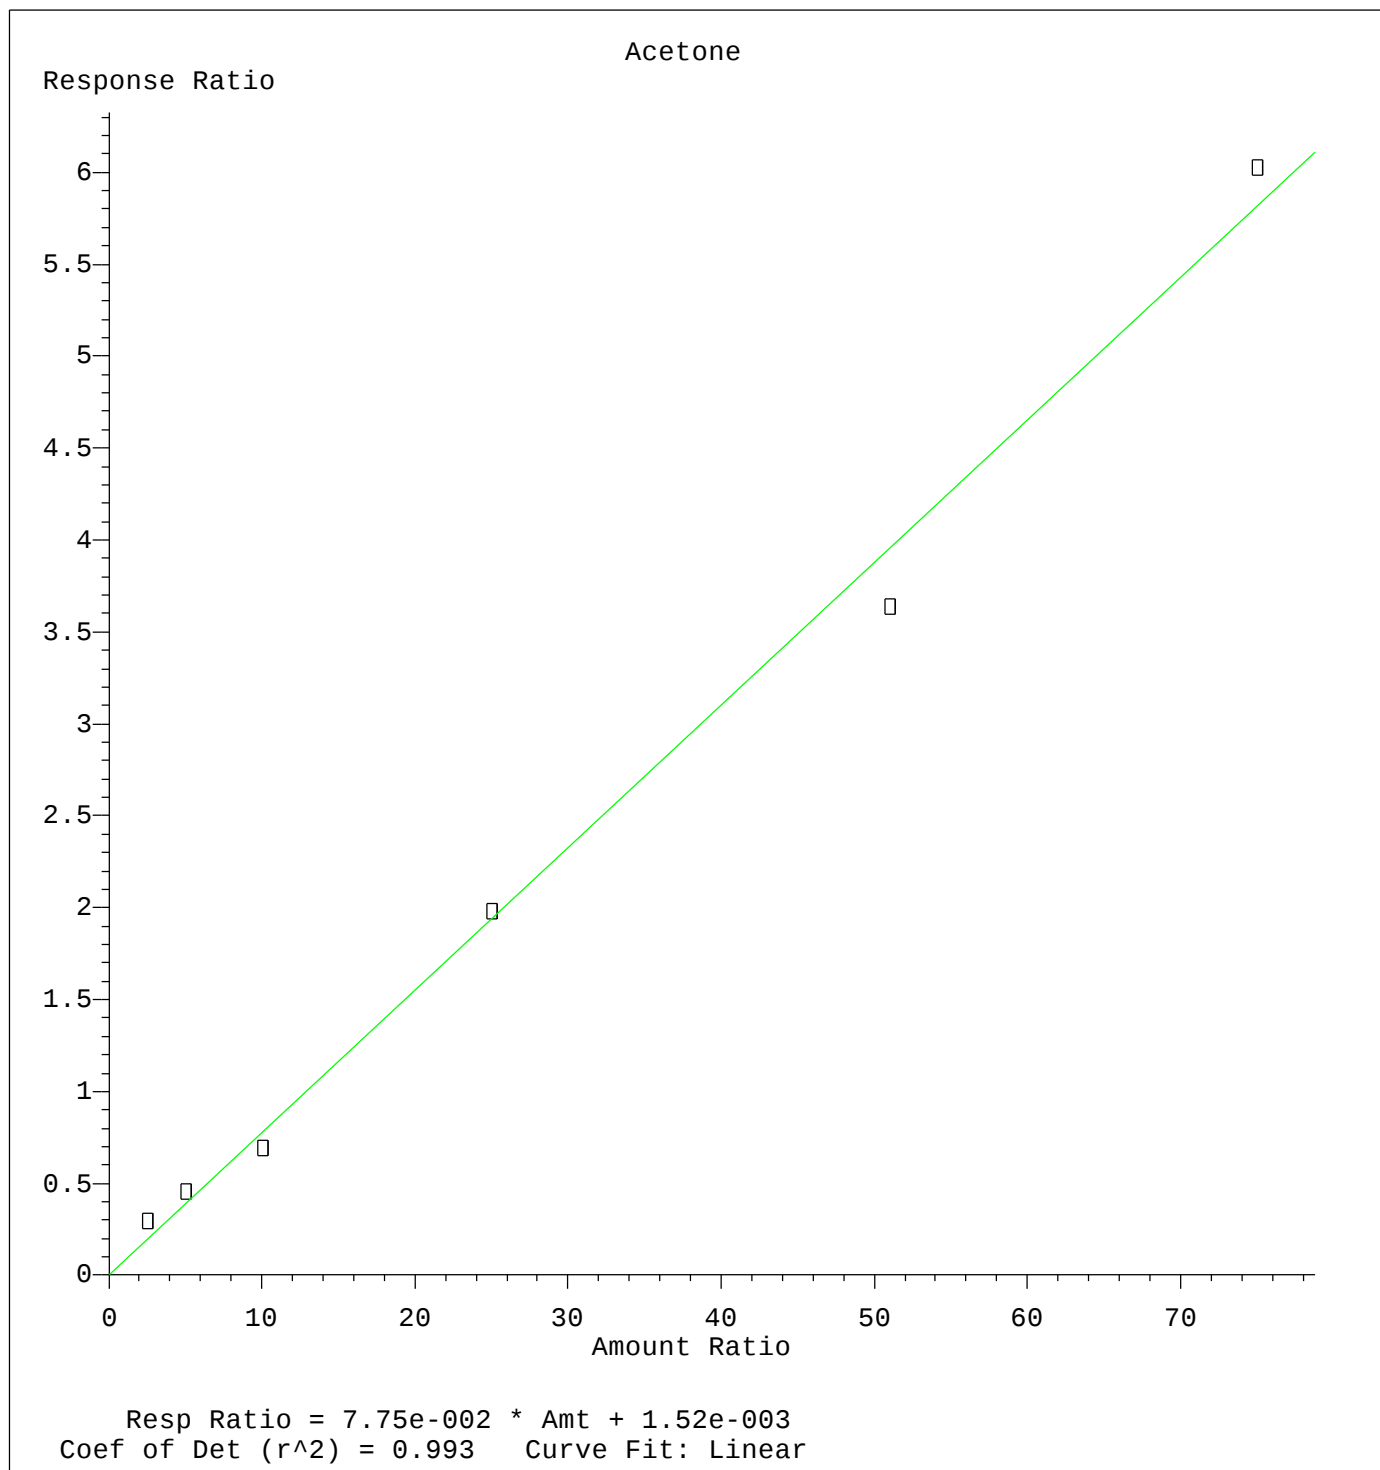


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Calibration Table Last Updated: Tue Apr 16 04:55:56 2019

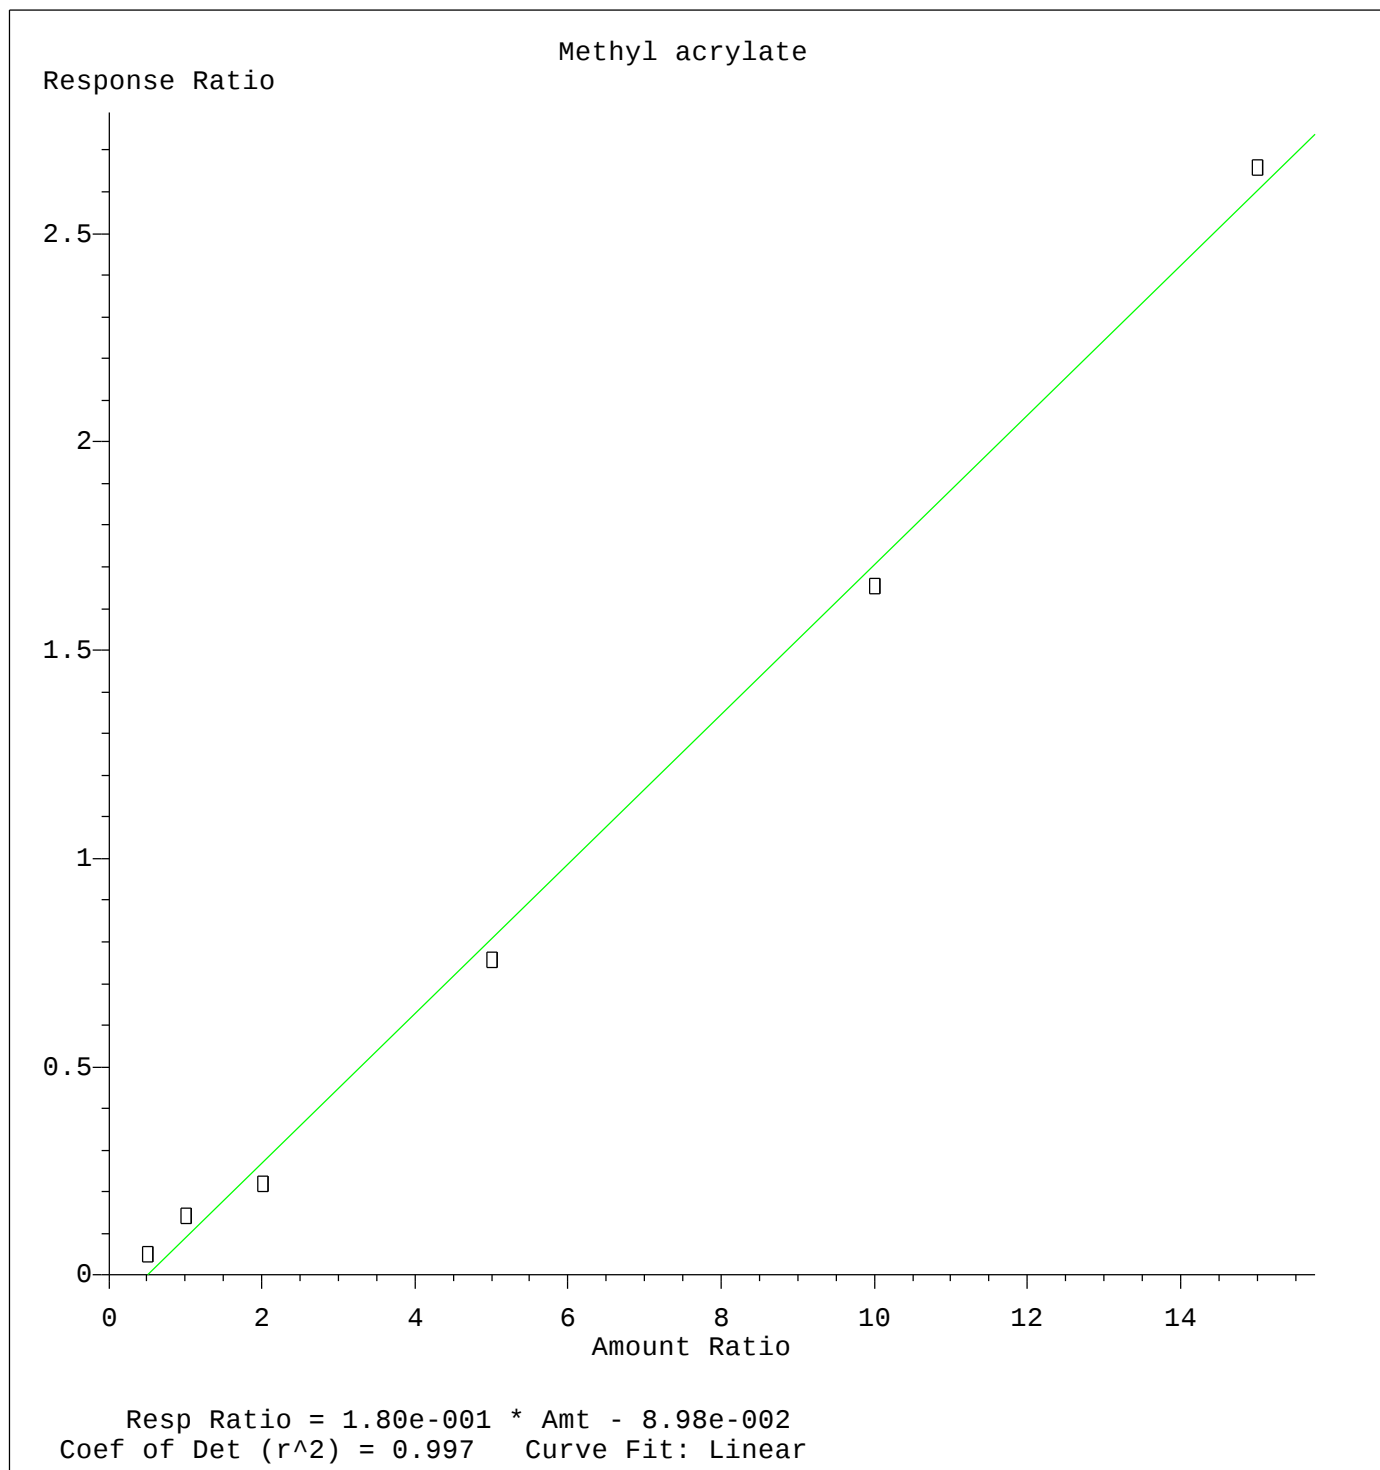

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Calibration Table Last Updated: Tue Apr 16 04:55:56 2019

Ethyl methacrylate

Response Ratio

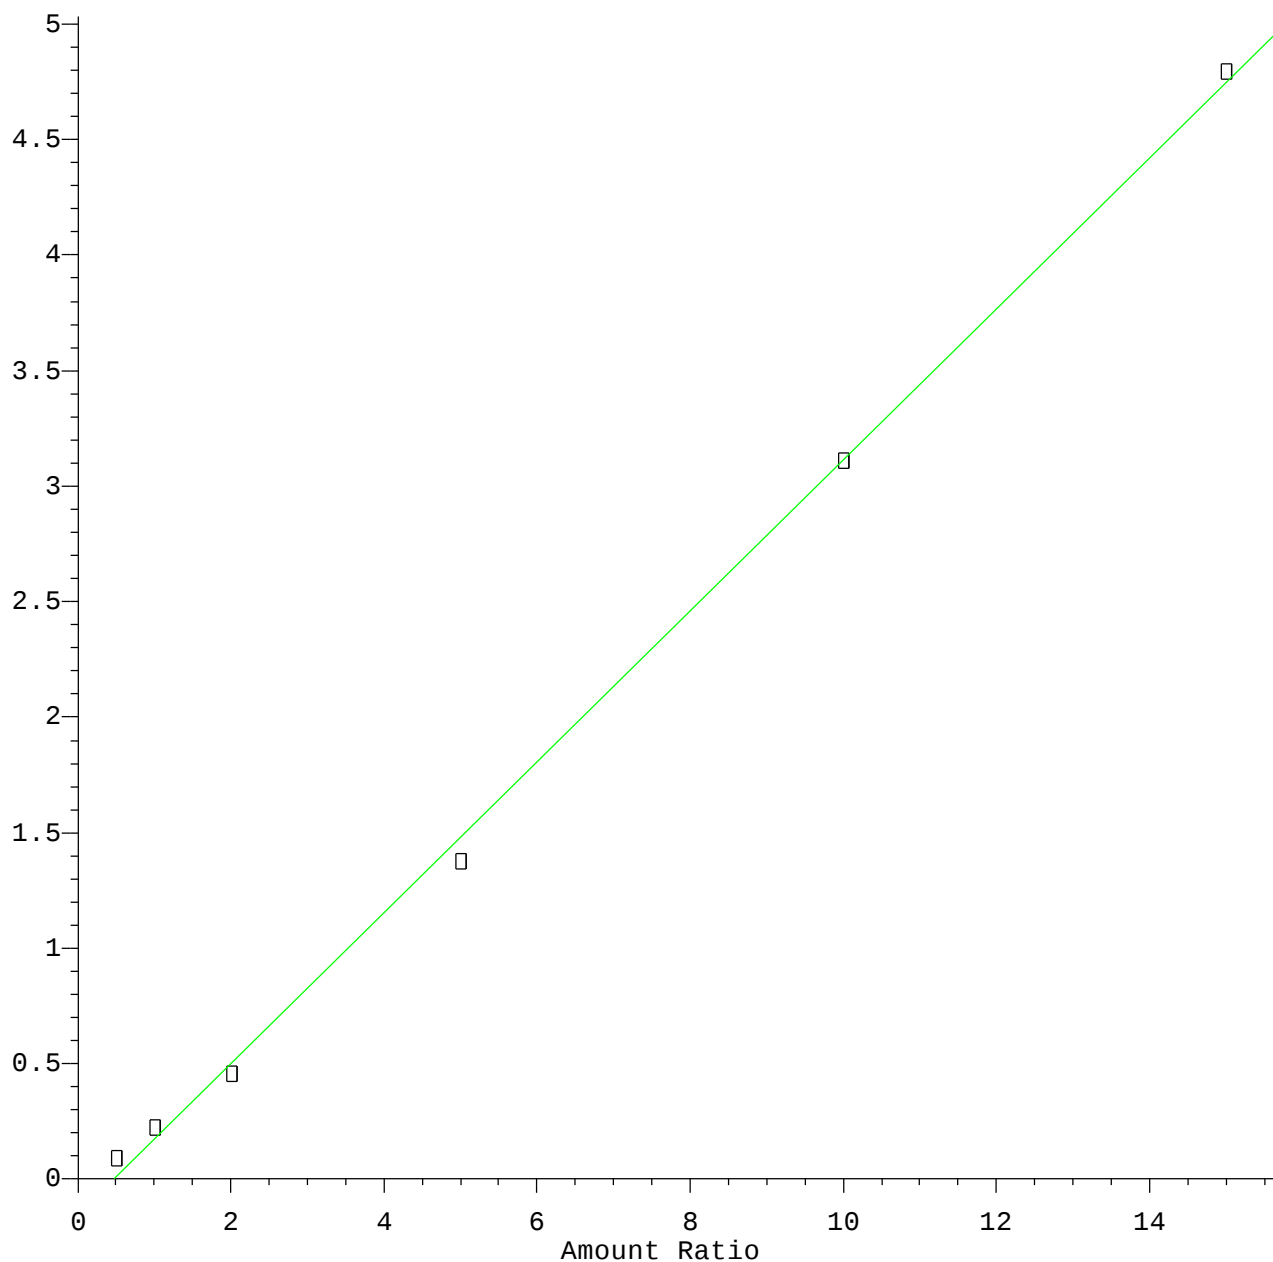


Resp Ratio = $3.27 \times 10^{-1} \times \text{Amt} - 1.51 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Calibration Table Last Updated: Tue Apr 16 04:55:56 2019


Styrene

Response Ratio

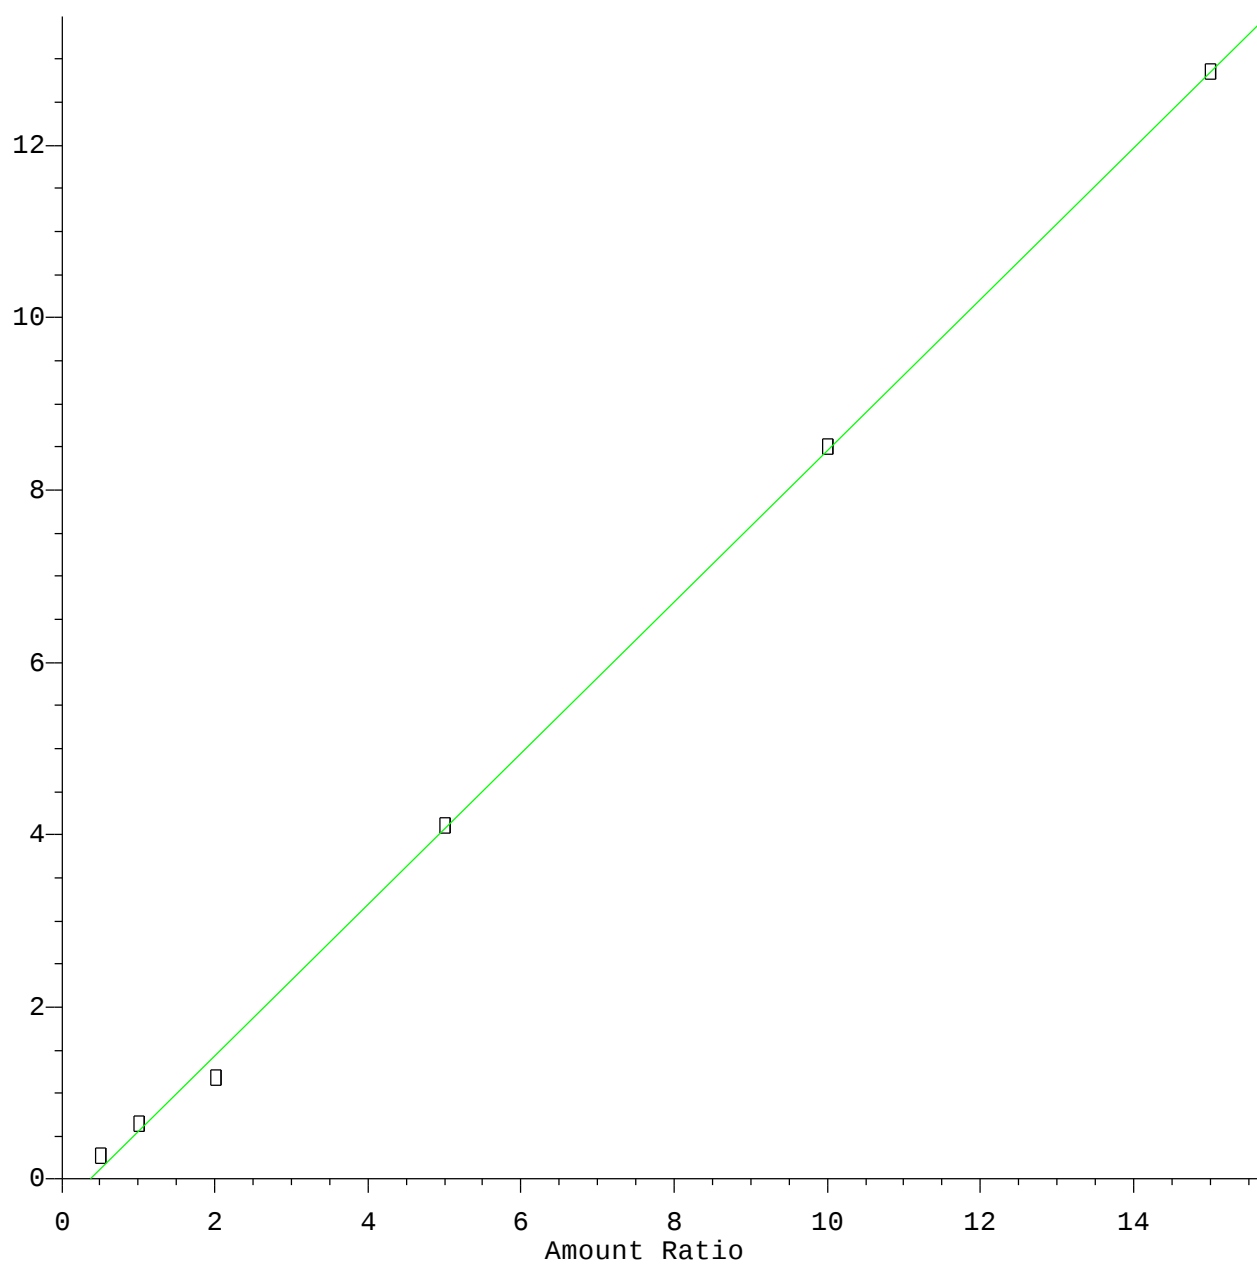

Resp Ratio = $8.78 \times 10^{-1} \times \text{Amt} - 3.17 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Calibration Table Last Updated: Tue Apr 16 04:55:56 2019

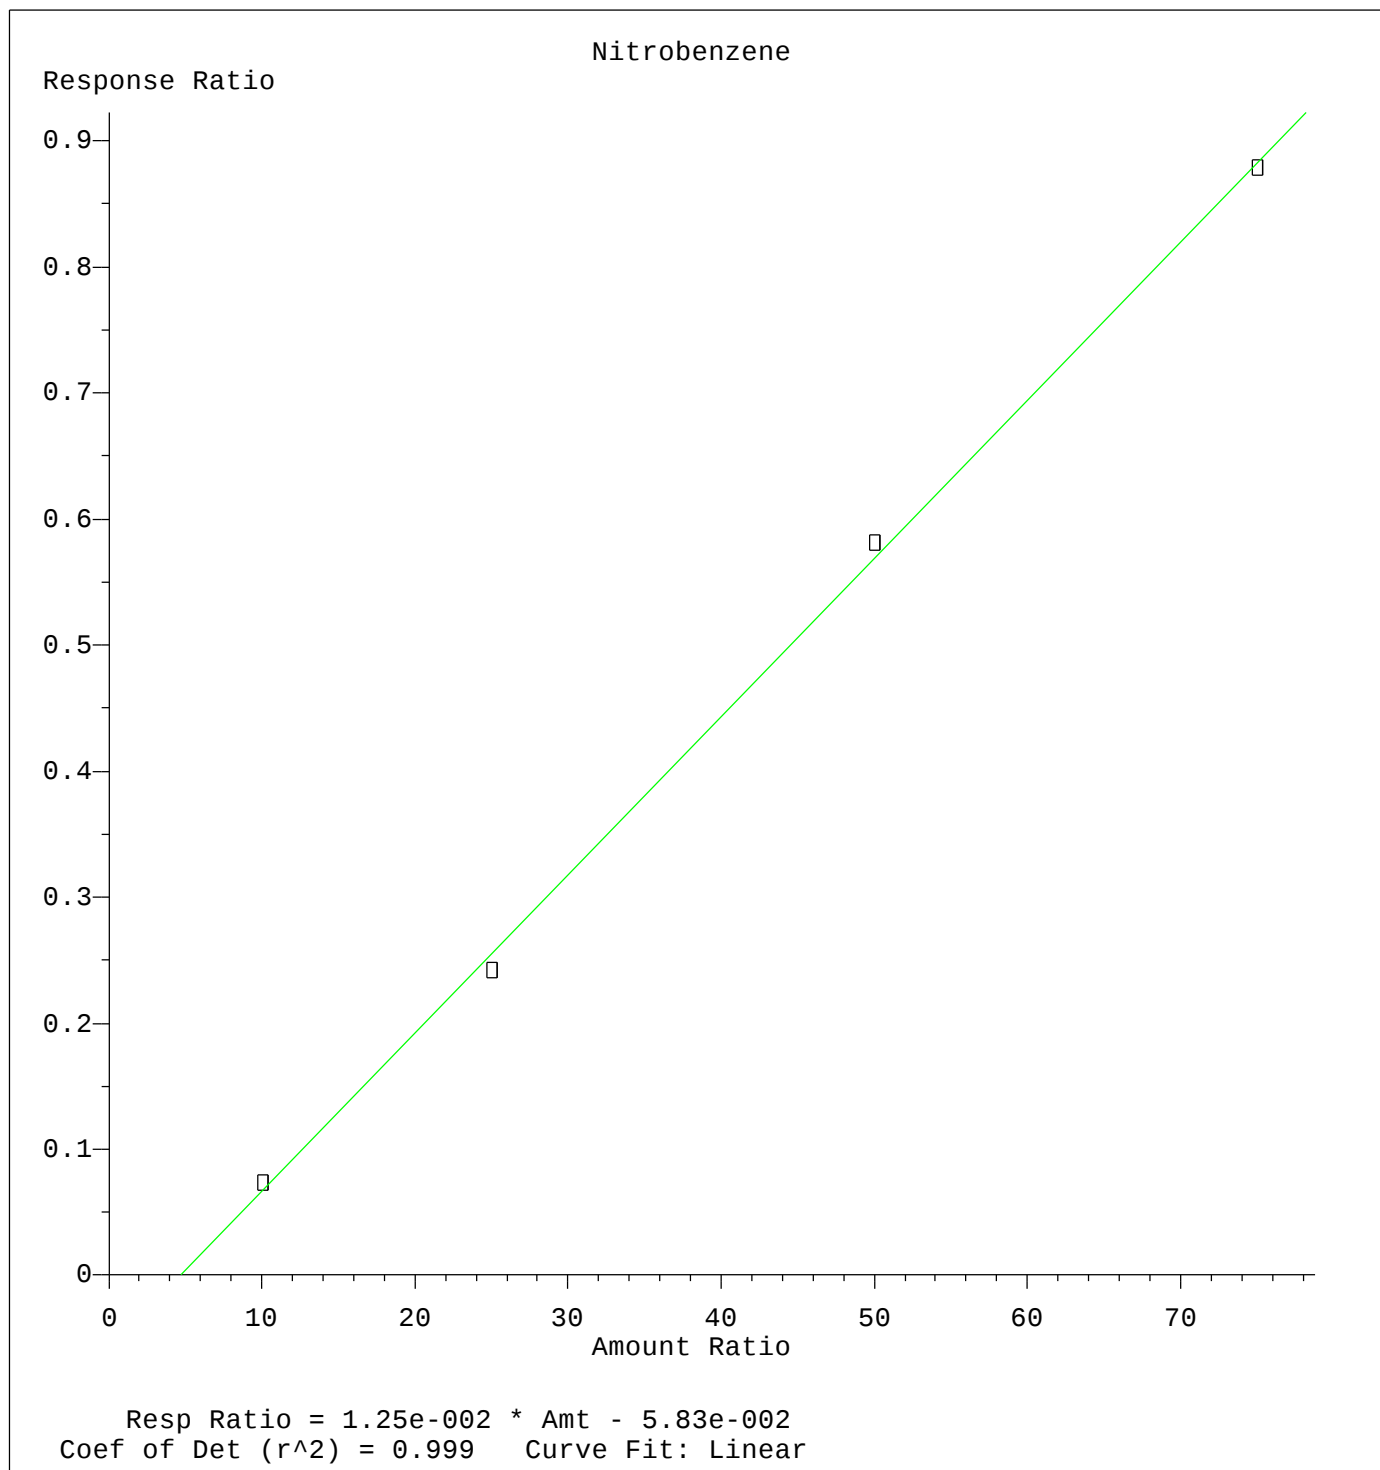

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Calibration Table Last Updated: Tue Apr 16 04:55:56 2019

Naphthalene

Response Ratio

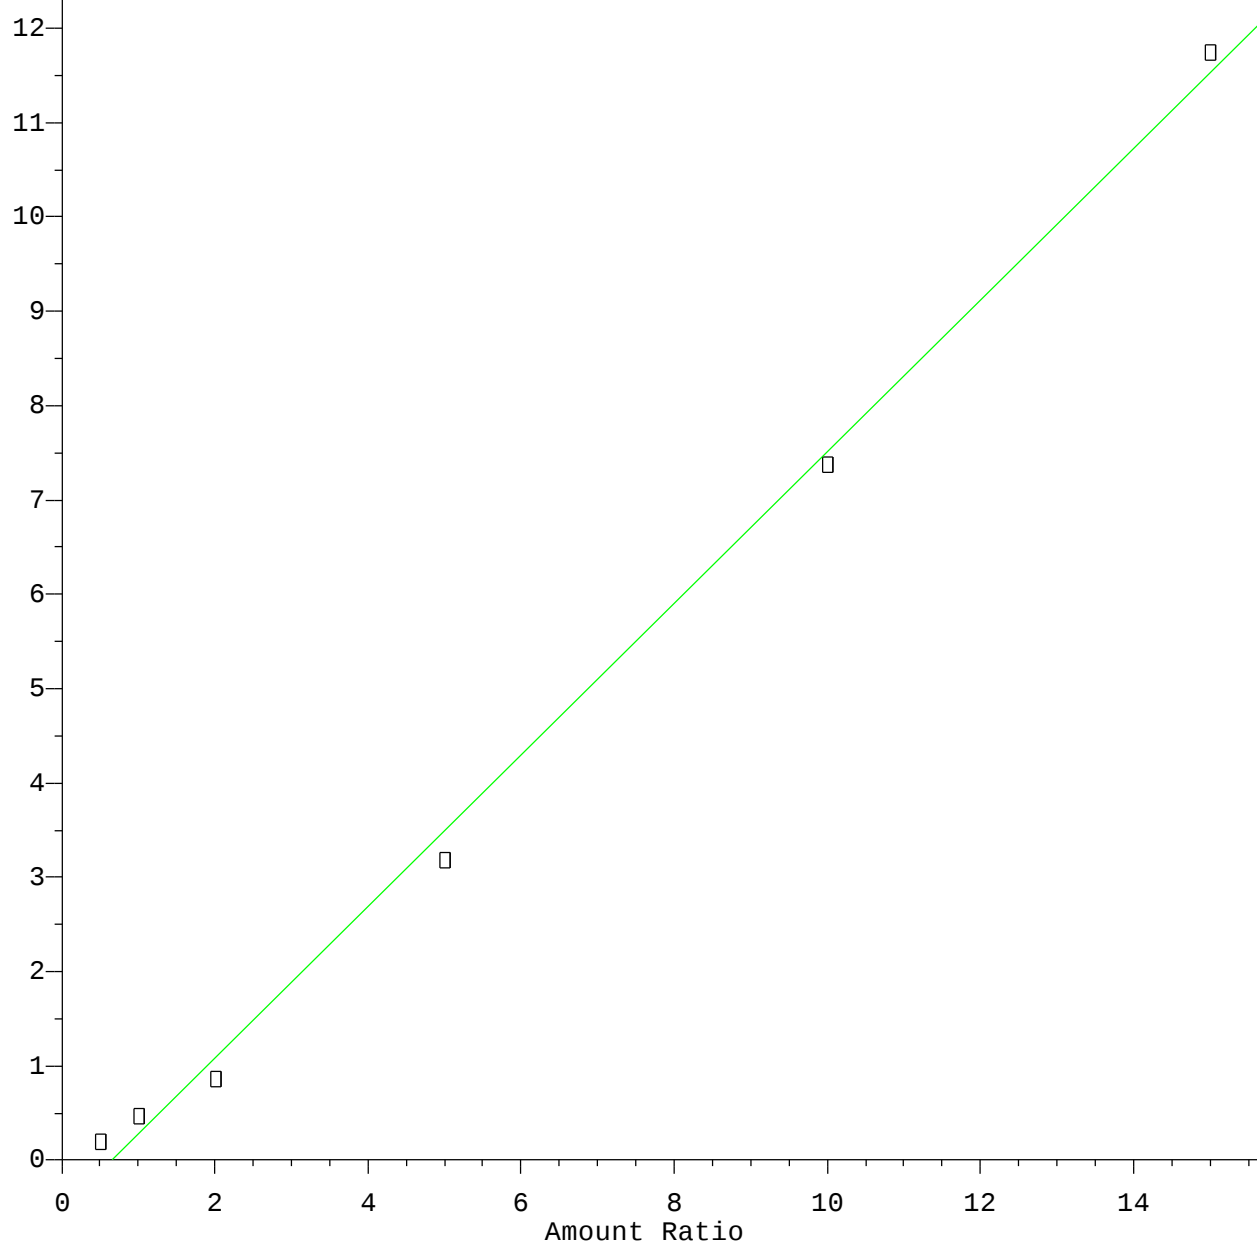

Resp Ratio = $8.03 \times 10^{-1} \times \text{Amt} - 5.20 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Calibration Table Last Updated: Tue Apr 16 04:55:56 2019