

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
 Data File : VU043122.D
 Acq On : 15 Apr 2021 15:43
 Operator : SY/MD
 Sample : M1986-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AT6

Manual Integrations
 APPROVED

MMDadoda
 4/19/2021 10:19:28 AM

Quant Time: Apr 16 05:36:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 16 05:01:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	89477	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	85915	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	42336	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	23358	5.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.60%
7) Chloroethane-d5	1.919	69	23276	5.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.60%
11) 1,1-Dichloroethene-d2	2.572	65	13180	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.20%
20) 2-Butanone-d5	4.642	46	111603	55.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.84%
24) Chloroform-d	5.073	84	58864	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
26) 1,2-Dichloroethane-d4	5.713	65	38436	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	5.739	84	110179	5.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.20%
36) 1,2-Dichloropropane-d6	6.700	67	35601	5.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.40%
41) Toluene-d8	7.906	98	104130	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
43) trans-1,3-Dichloroprop...	8.189	79	14894	5.08	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.60%
46) 2-Hexanone-d5	8.645	63	81820	56.00	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.00%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	30392	5.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.20%
66) 1,2-Dichlorobenzene-d4	12.201	152	39875	5.49	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.80%
Target Compounds						Qvalue
13) Acetone	2.645	43	2399m	1.64	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043122.D
Acq On : 15 Apr 2021 15:43
Operator : SY/MD
Sample : M1986-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0AT6

Manual Integrations
APPROVED

MMDadoda
4/19/2021 10:19:28 AM


Quant Time: Apr 16 05:36:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 16 05:01:39 2021
Response via : Initial Calibration

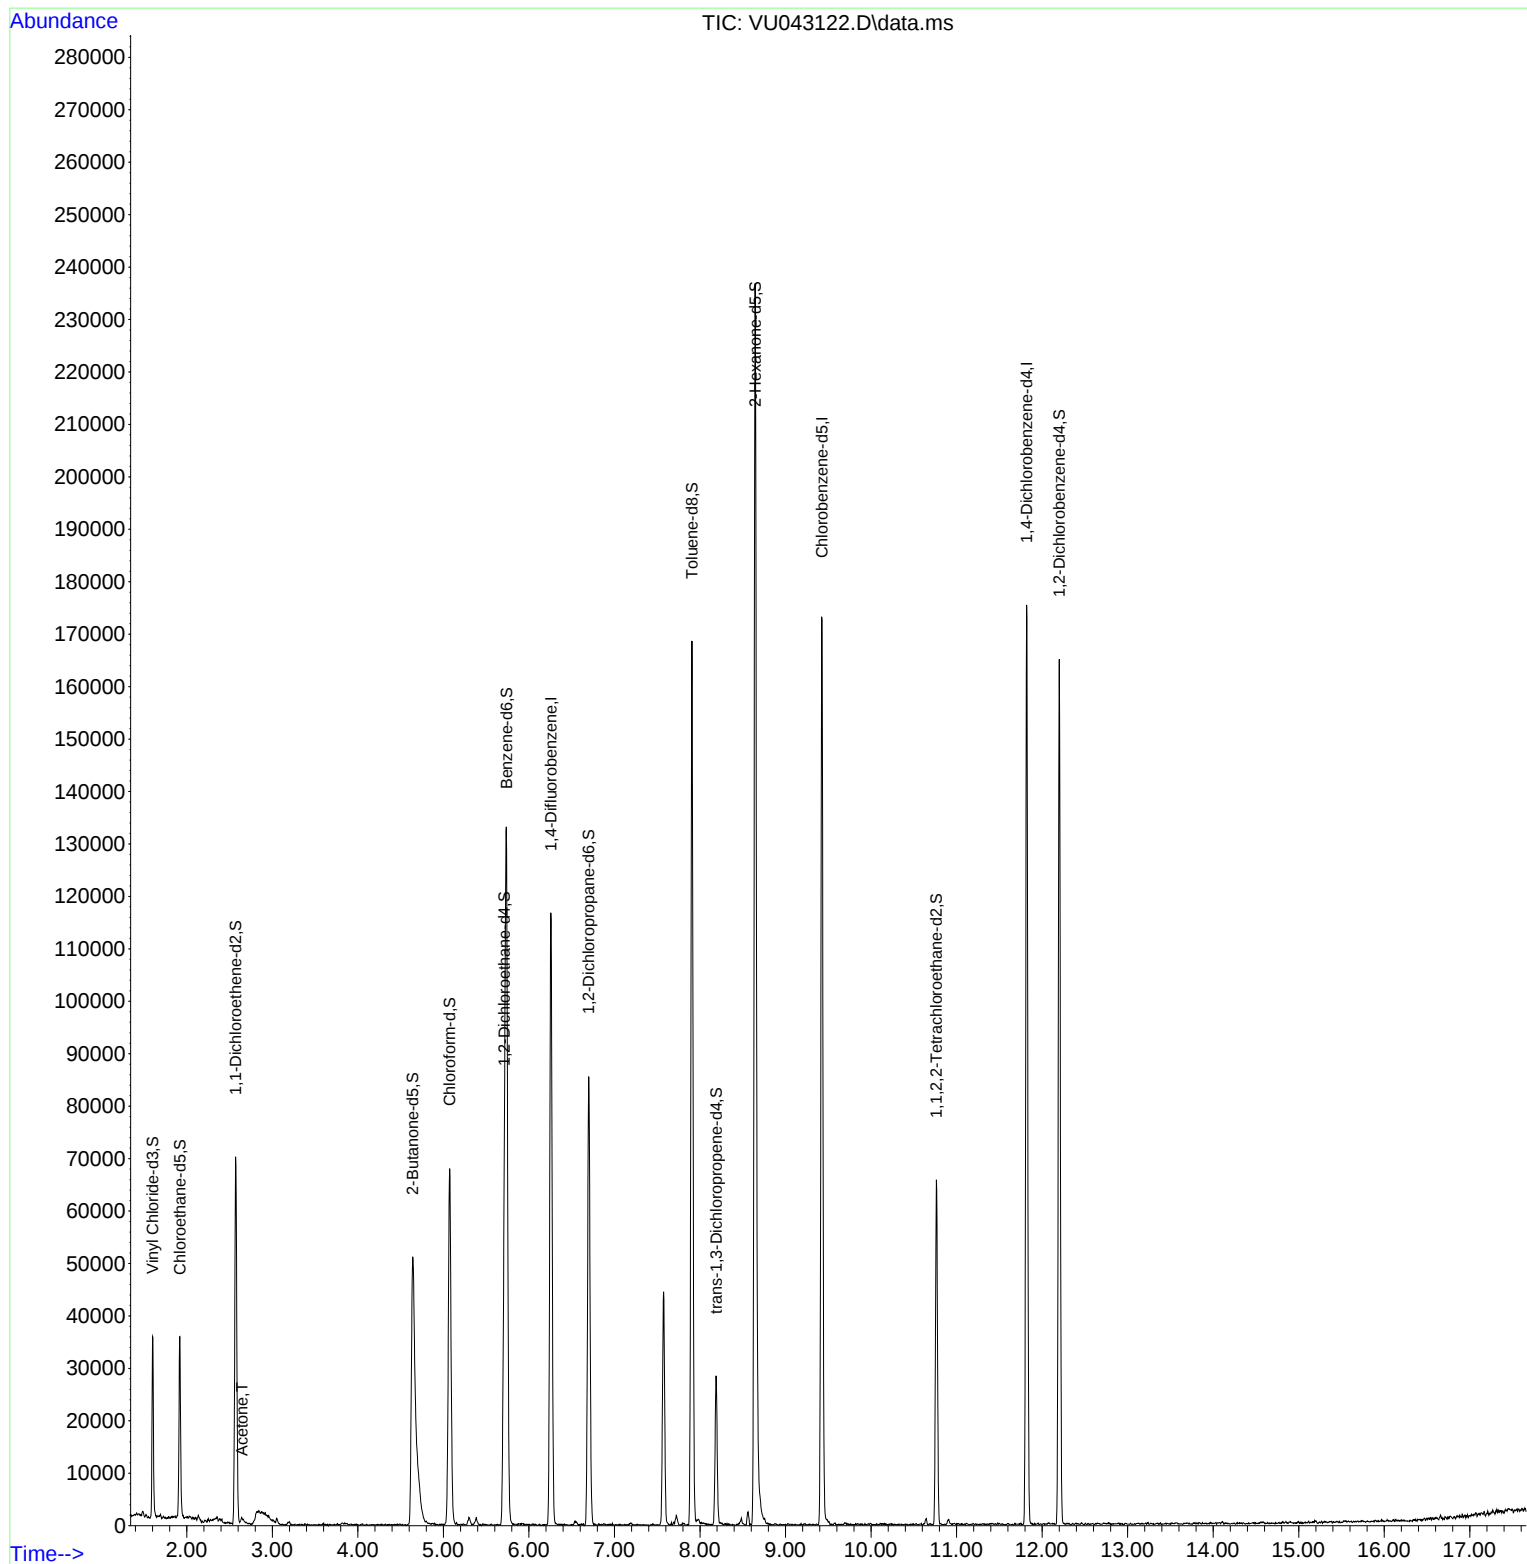

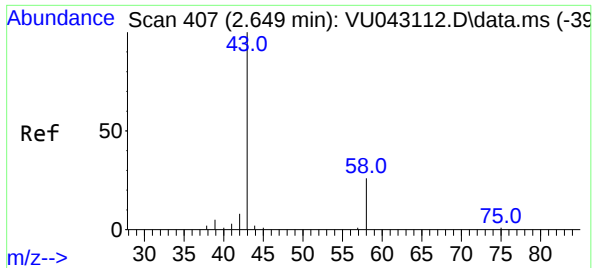

#13
 Acetone
 Concen: 1.64 ug/L m
 RT: 2.645 min Scan# 406
 Delta R.T. -0.003 min
 Lab File: VU043122.D
 Acq: 15 Apr 2021 15:43

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AT6

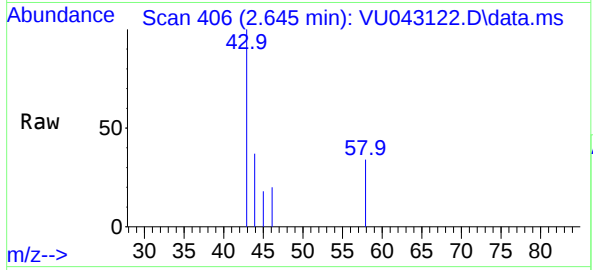

Tgt Ion: 43 Resp: 2399

Ion	Ratio	Lower	Upper
43	100		
58	14.8	0.0	25.0

Manual Integrations
 APPROVED
 MMDadoda
 4/19/2021 10:19:28 AM

