

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
 Data File : VU043148.D
 Acq On : 16 Apr 2021 02:34
 Operator : SY/MD
 Sample : M2055-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4522

Quant Time: Apr 16 07:18:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 16 07:14:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	66320	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	66949	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.822	152	31274	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	16891	5.01	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.20%
7) Chloroethane-d5	1.919	69	17112	5.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.80%
11) 1,1-Dichloroethene-d2	2.575	65	10279	5.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	105.40%
20) 2-Butanone-d5	4.642	46	94860	64.13	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.26%
24) Chloroform-d	5.073	84	47312	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.40%
26) 1,2-Dichloroethane-d4	5.713	65	32212	5.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.00%
32) Benzene-d6	5.735	84	87225	5.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.00%
36) 1,2-Dichloropropane-d6	6.700	67	28527	5.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.40%
41) Toluene-d8	7.906	98	76803	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
43) trans-1,3-Dichloroprop...	8.185	79	11244	4.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.60%
46) 2-Hexanone-d5	8.645	63	64875	56.98	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.96%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	25810	5.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.60%
66) 1,2-Dichlorobenzene-d4	12.201	152	31133	5.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.20%
Target Compounds						
12) 1,1-Dichloroethene	2.588	96	5592	1.52	ug/L	# 3
29) 1,1,1-Trichloroethane	5.321	97	3130	0.38	ug/L	# 83
47) Tetrachloroethene	8.562	164	2002	0.51	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043148.D
Acq On : 16 Apr 2021 02:34
Operator : SY/MD
Sample : M2055-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4522

Quant Time: Apr 16 07:18:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 16 07:14:05 2021
Response via : Initial Calibration

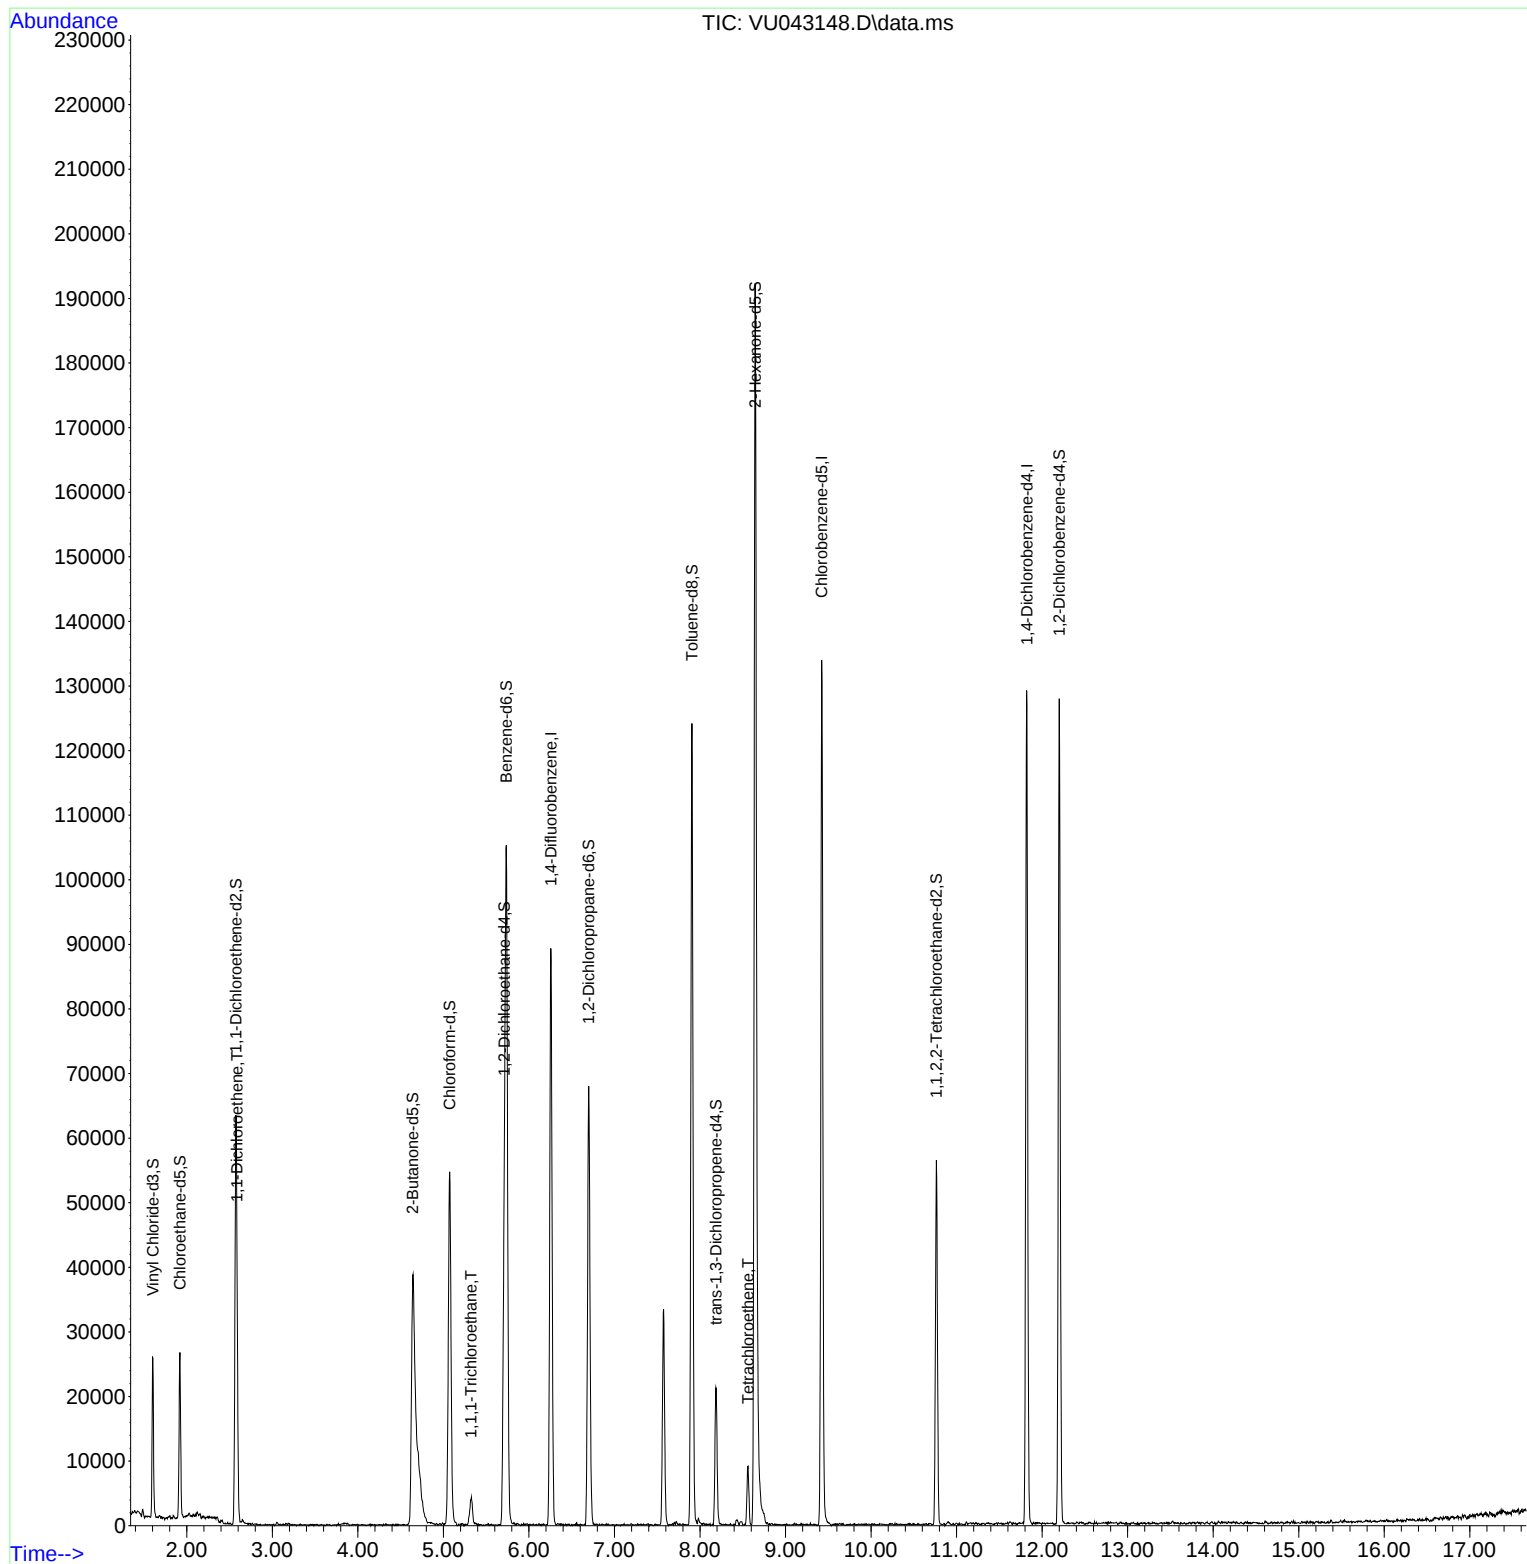

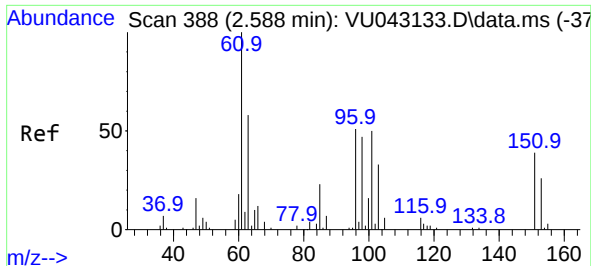

#12

1,1-Dichloroethene

Concen: 1.52 ug/L

RT: 2.588 min Scan# 388

Delta R.T. 0.000 min

Lab File: VU043148.D

Acq: 16 Apr 2021 02:34

Tgt Ion: 96 Resp: 5592

Ion Ratio Lower Upper

96 100

61 218.1 115.1 213.7#





63 315.9 84.1 156.1#

Instrument :

MSVOA_U

ClientSampled :

H4522

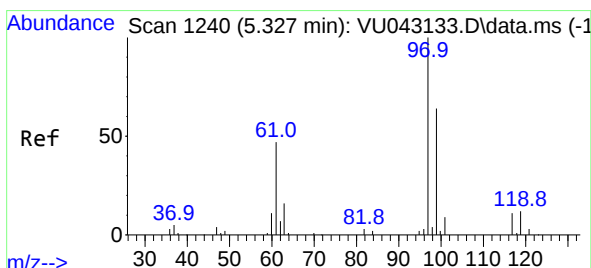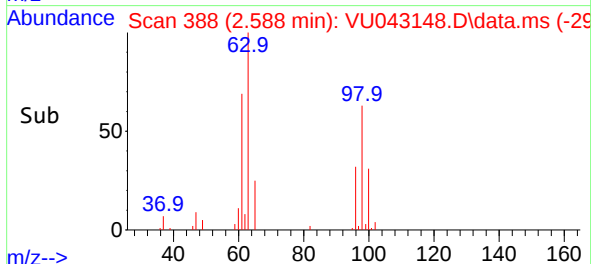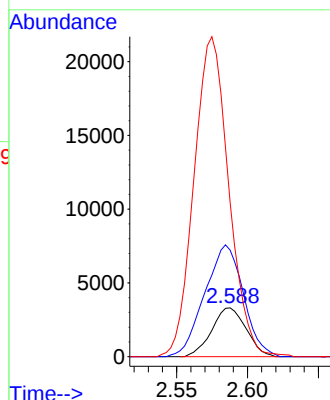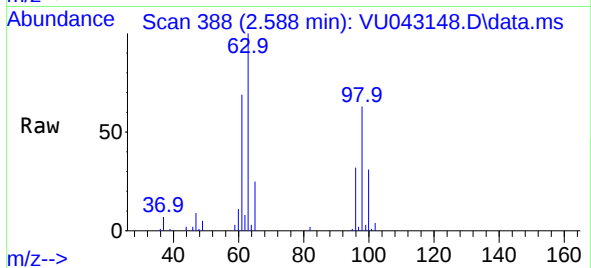

#29

1,1,1-Trichloroethane

Concen: 0.38 ug/L

RT: 5.321 min Scan# 1238

Delta R.T. -0.006 min

Lab File: VU043148.D

Acq: 16 Apr 2021 02:34




Tgt Ion: 97 Resp: 3130


Ion Ratio Lower Upper

97 100

99 71.4 50.3 75.5

61 56.9 32.7 49.1#

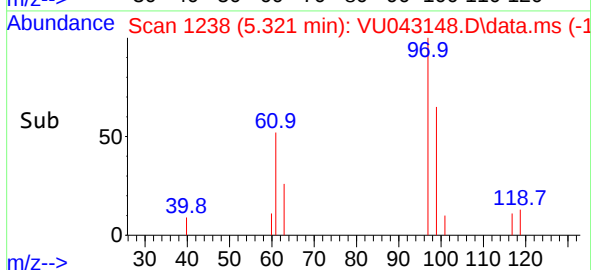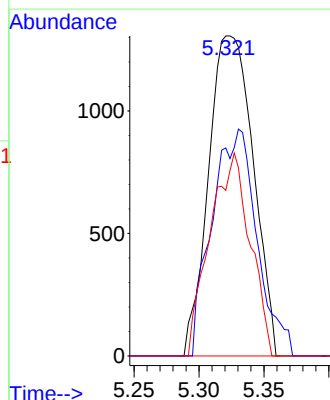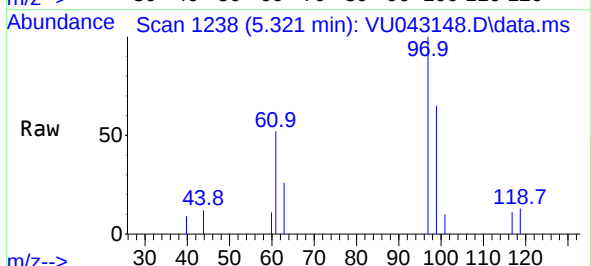

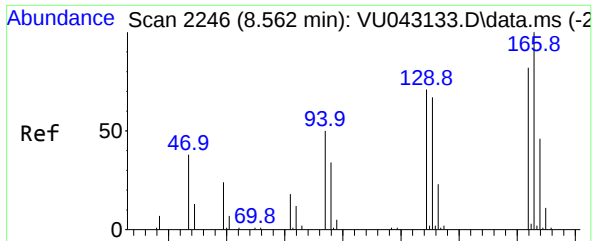

#47
Tetrachloroethene
Concen: 0.51 ug/L
RT: 8.562 min Scan# 2246
Delta R.T. 0.000 min
Lab File: VU043148.D
Acq: 16 Apr 2021 02:34

Instrument :
MSVOA_U
ClientSampleId :
H4522

Tgt Ion:164 Resp: 2002

Ion	Ratio	Lower	Upper
164	100		
129	75.1	66.6	123.8
131	82.5	65.9	122.3
166	114.7	93.7	173.9

