

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
 Data File : VU043119.D
 Acq On : 15 Apr 2021 14:32
 Operator : SY/MD
 Sample : M1986-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AT3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	72	81	91	rBV	35879	41009	3.63%	0.868%
2	1.919	171	180	193	rBV	31716	41139	3.64%	0.871%
3	2.086	224	232	240	rBV	21934	30236	2.68%	0.640%
4	2.144	240	250	267	rVB	174851	259438	22.96%	5.494%
5	2.571	371	383	404	rVB2	72891	120181	10.64%	2.545%
6	4.661	1013	1033	1057	rBV3	41136	172875	15.30%	3.661%
7	5.073	1145	1161	1188	rVB2	68063	154545	13.68%	3.273%
8	5.735	1346	1367	1384	rBV2	131348	347635	30.76%	7.361%
9	6.256	1516	1529	1549	rBV	115269	216623	19.17%	4.587%
10	6.552	1606	1621	1636	rBV	135677	255383	22.60%	5.408%
11	6.700	1651	1667	1686	rBV2	85477	164514	14.56%	3.484%
12	7.574	1927	1939	1953	rBV	43339	77862	6.89%	1.649%
13	7.906	2029	2042	2058	rBV	169351	287669	25.46%	6.091%
14	8.189	2117	2130	2152	rBV	29584	52311	4.63%	1.108%
15	8.562	2231	2246	2260	rBV	667066	1129974	100.00%	23.927%
16	8.645	2260	2272	2302	rVB	193529	439208	38.87%	9.300%
17	9.423	2502	2514	2536	rBV	167676	283435	25.08%	6.002%
18	10.764	2921	2931	2946	rVB	64937	107559	9.52%	2.278%
19	11.819	3247	3259	3277	rBV	169784	274084	24.26%	5.804%
20	12.201	3364	3378	3393	rBV	166185	266818	23.61%	5.650%




Sum of corrected areas: 4722498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043119.D
Acq On : 15 Apr 2021 14:32
Operator : SY/MD
Sample : M1986-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

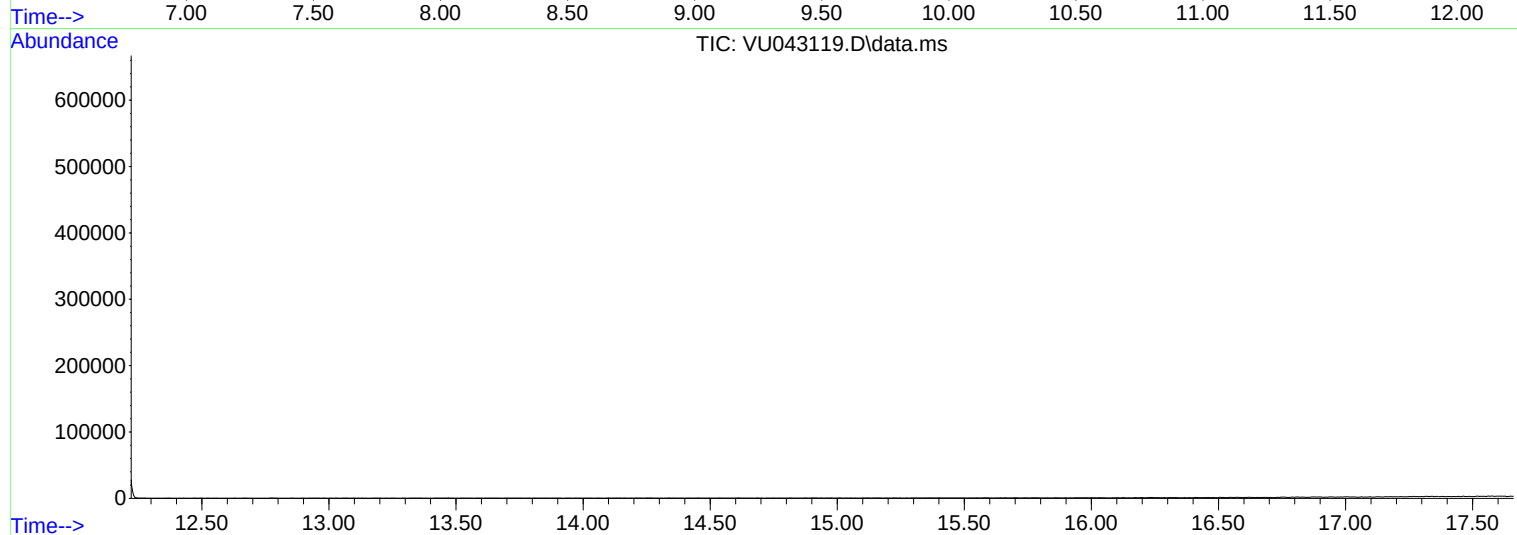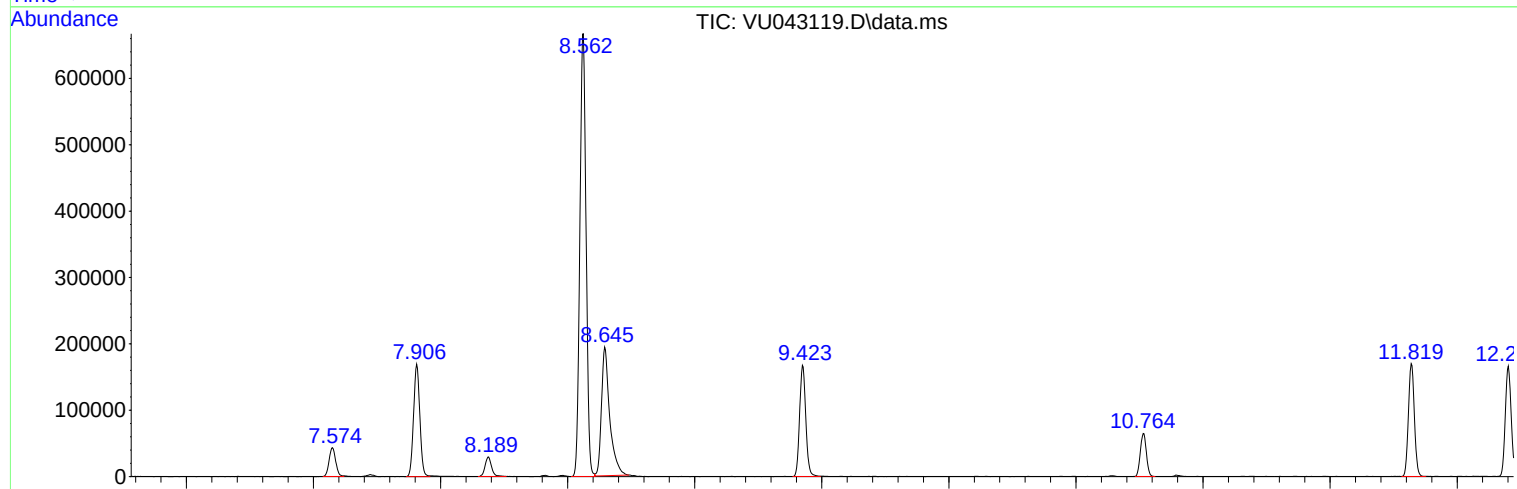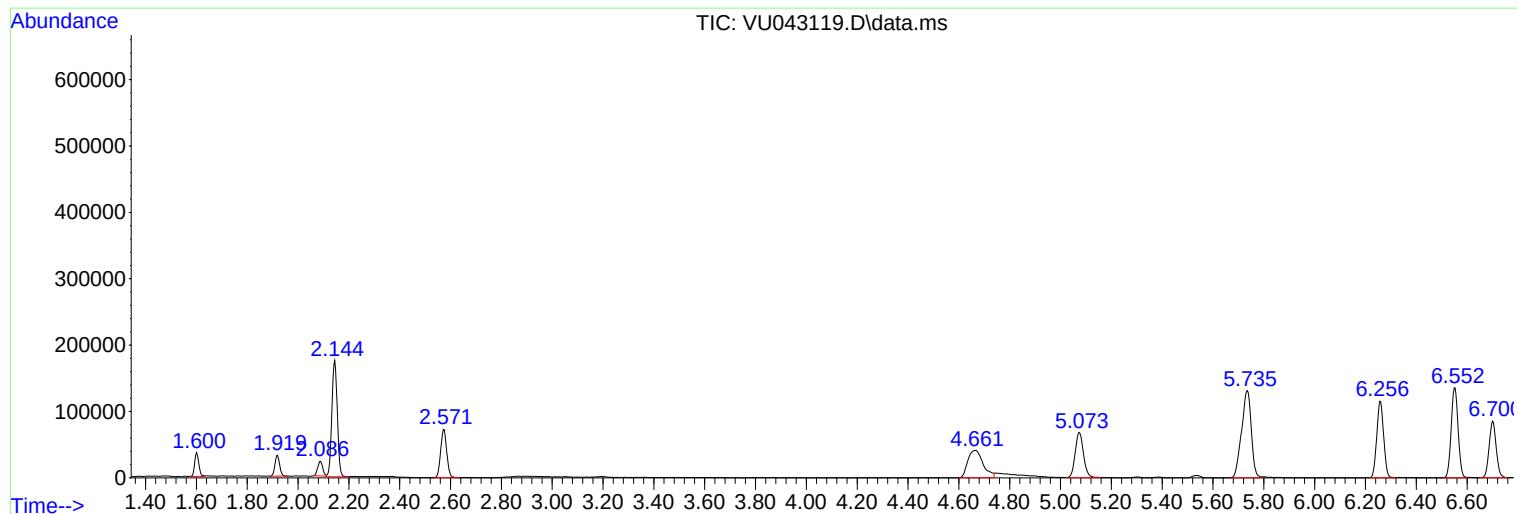

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043119.D
Acq On : 15 Apr 2021 14:32
Operator : SY/MD
Sample : M1986-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AT3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.086	0.70 ug/L	30236	1,4-Difluorobenzene	6.259

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	94
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	90
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	90
4			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7
5			Cyclopentene, 1-chloro-	102	C5H7Cl	000930-29-0	7

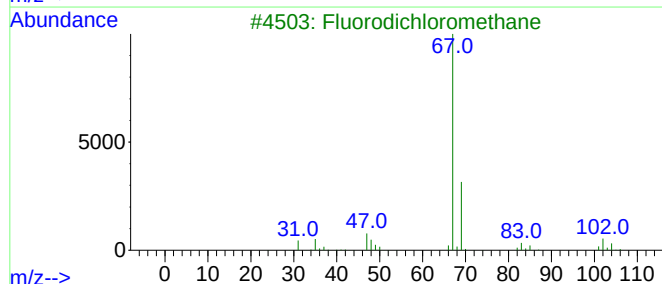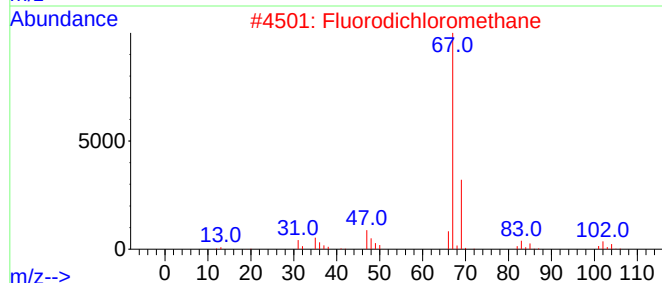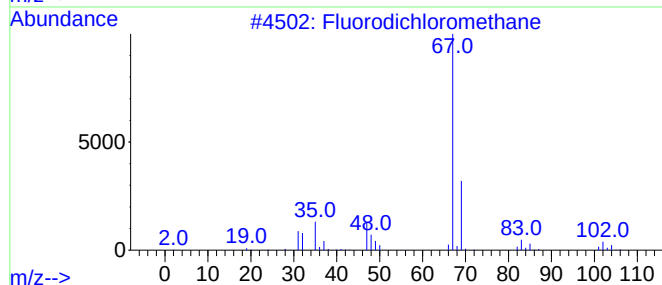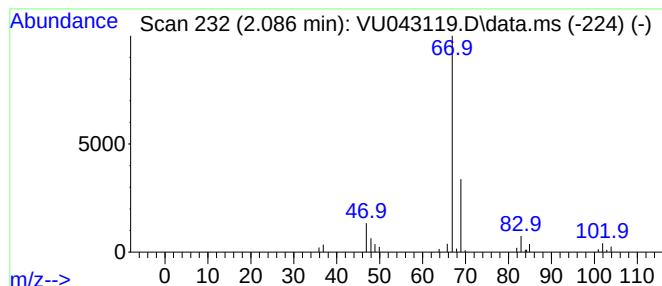

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043119.D
Acq On : 15 Apr 2021 14:32
Operator : SY/MD
Sample : M1986-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.086	0.7	ug/L	30236	1	6.259	216623	5.0