

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
 Data File : VU043142.D
 Acq On : 16 Apr 2021 00:10
 Operator : SY/MD
 Sample : M2055-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4481

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	10	17	23	rBV	11163	11047	2.09%	0.375%
2	1.600	74	81	91	rBV	25216	28575	5.40%	0.970%
3	1.919	172	180	194	rVB	25391	33169	6.27%	1.126%
4	2.575	371	384	397	rBV	57921	96761	18.30%	3.286%
5	3.369	620	631	645	rBV2	2932	6809	1.29%	0.231%
6	4.645	1011	1028	1050	rBV	30139	103432	19.56%	3.513%
7	5.073	1145	1161	1182	rBV	54819	125046	23.65%	4.247%
8	5.735	1345	1367	1384	rBV2	105398	278529	52.68%	9.459%
9	6.259	1516	1530	1544	rBV	84502	158016	29.88%	5.366%
10	6.549	1608	1620	1634	rBV2	22781	41362	7.82%	1.405%
11	6.700	1653	1667	1685	rBV2	69719	133943	25.33%	4.549%
12	7.575	1927	1939	1957	rBV2	32890	59152	11.19%	2.009%
13	7.906	2029	2042	2058	rBV	127416	216686	40.98%	7.359%
14	8.185	2118	2129	2145	rBV2	21563	36468	6.90%	1.239%
15	8.562	2232	2246	2260	rBV	311519	528753	100.00%	17.957%
16	8.645	2260	2272	2315	rVB	166313	390962	73.94%	13.278%
17	9.423	2501	2514	2529	rBV	123863	205602	38.88%	6.983%
18	10.764	2918	2931	2945	rBV	56602	93037	17.60%	3.160%
19	11.819	3247	3259	3274	rBV	121730	192256	36.36%	6.529%
20	12.201	3366	3378	3396	rVB	129815	204907	38.75%	6.959%




Sum of corrected areas: 2944512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043142.D
Acq On : 16 Apr 2021 00:10
Operator : SY/MD
Sample : M2055-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4481

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

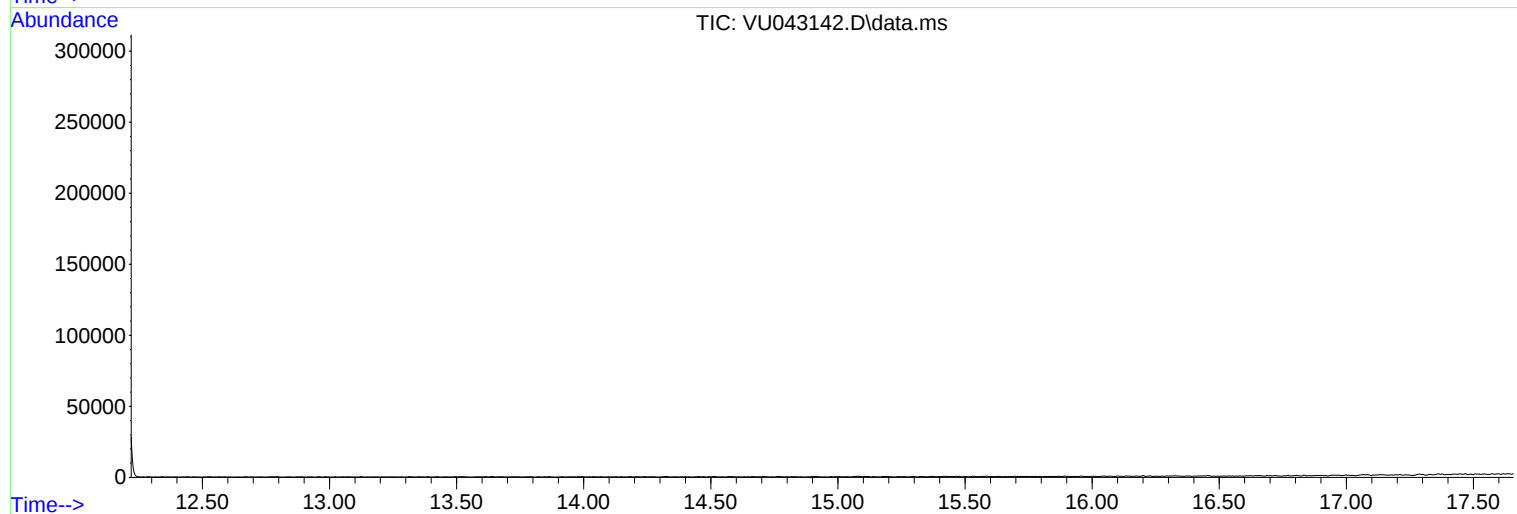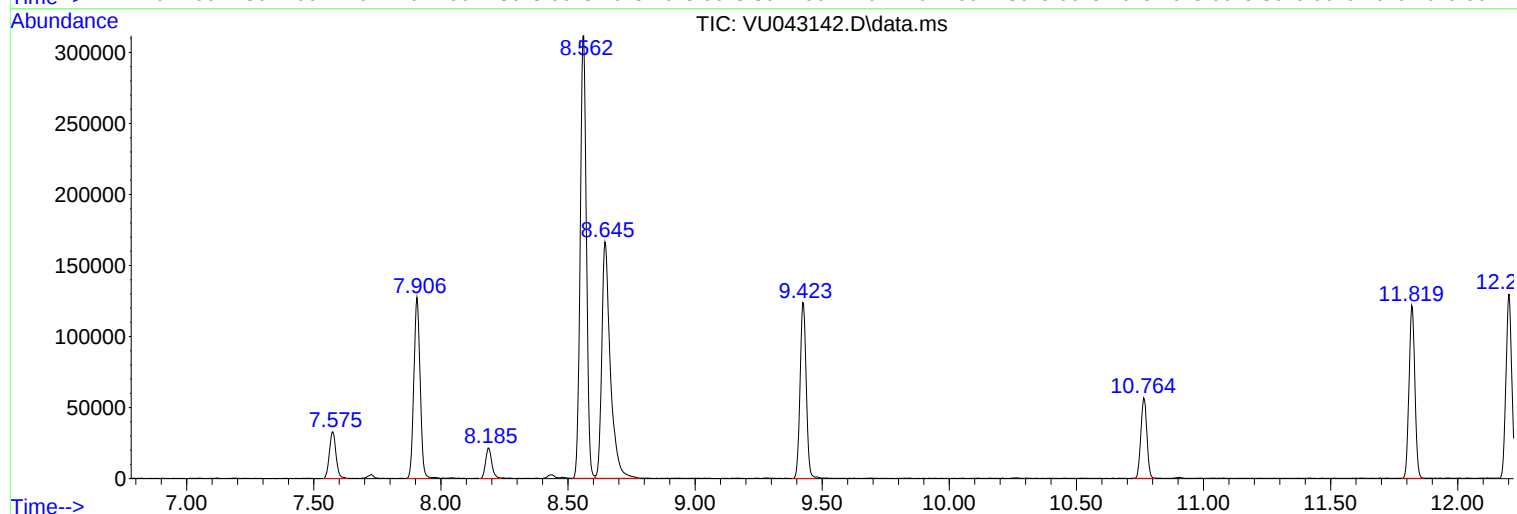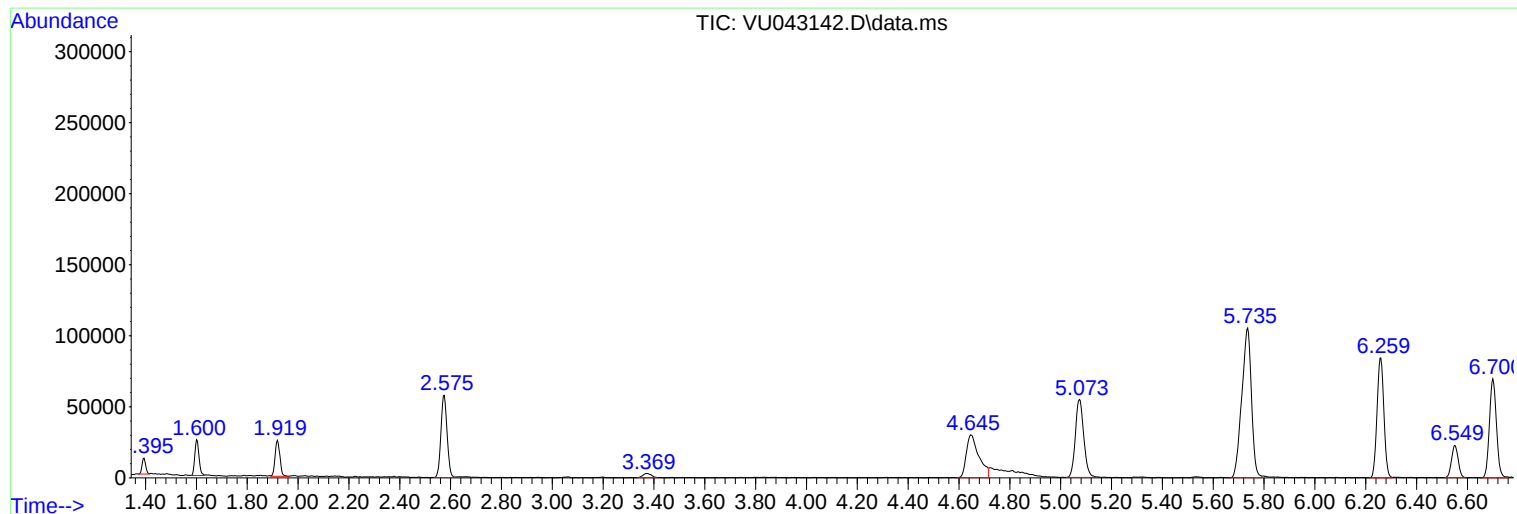

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043142.D
Acq On : 16 Apr 2021 00:10
Operator : SY/MD
Sample : M2055-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4481

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043142.D
Acq On : 16 Apr 2021 00:10
Operator : SY/MD
Sample : M2055-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4481

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
