

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
 Data File : VU043148.D
 Acq On : 16 Apr 2021 02:34
 Operator : SY/MD
 Sample : M2055-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rVB	24896	28804	7.59%	1.172%
2	1.919	171	180	194	rBV	25639	32871	8.67%	1.337%
3	2.575	372	384	399	rBV3	63346	116568	30.73%	4.743%
4	4.645	1008	1028	1081	rBV	38777	151794	40.02%	6.176%
5	5.073	1143	1161	1181	rBV	54596	119299	31.45%	4.854%
6	5.327	1226	1240	1253	rBV6	4269	9403	2.48%	0.383%
7	5.735	1347	1367	1391	rBV3	105209	278061	73.31%	11.314%
8	6.256	1516	1529	1550	rVB2	89253	166587	43.92%	6.778%
9	6.700	1654	1667	1684	rBV	67926	131286	34.61%	5.342%
10	7.575	1924	1939	1956	rVB2	33510	58683	15.47%	2.388%
11	7.906	2028	2042	2058	rBV	124098	214478	56.54%	8.727%
12	8.186	2119	2129	2144	rBV2	21266	36840	9.71%	1.499%
13	8.562	2237	2246	2257	rVB4	9107	14415	3.80%	0.587%
14	8.645	2257	2272	2303	rBV	192194	379308	100.00%	15.434%
15	9.423	2501	2514	2534	rBV	133915	219234	57.80%	8.920%
16	10.764	2920	2931	2946	rBV	56381	90012	23.73%	3.662%
17	11.819	3248	3259	3280	rVB	129124	206695	54.49%	8.410%
18	12.201	3365	3378	3393	rBV	127821	203346	53.61%	8.274%




Sum of corrected areas: 2457684

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043148.D
Acq On : 16 Apr 2021 02:34
Operator : SY/MD
Sample : M2055-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4522

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

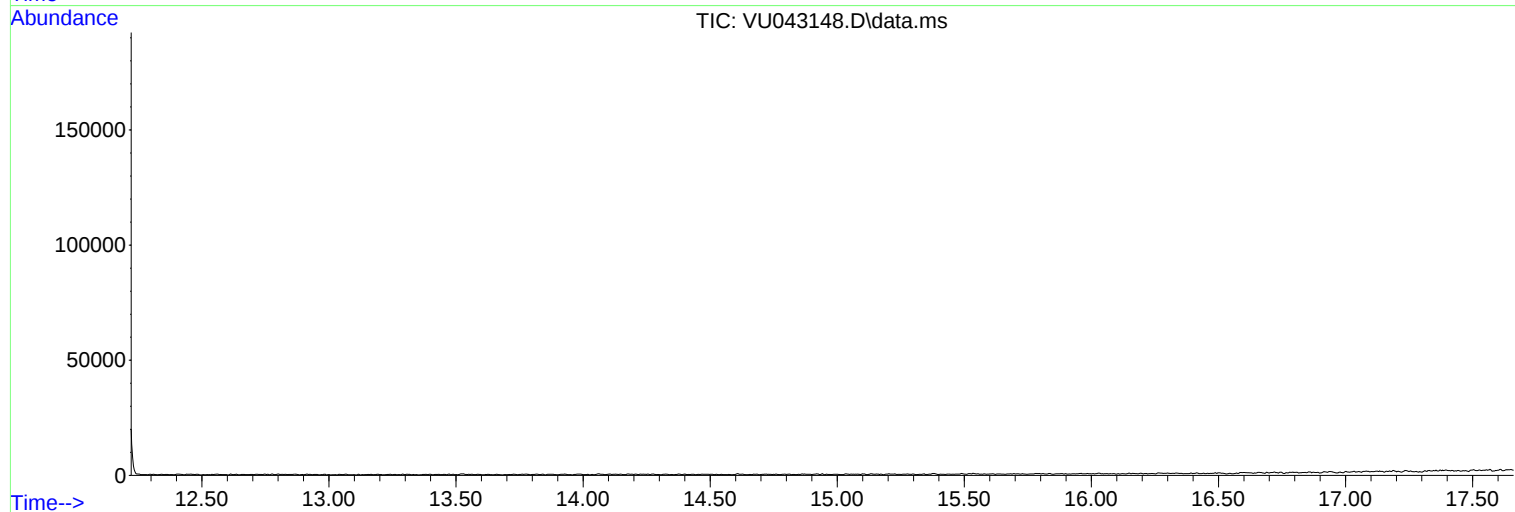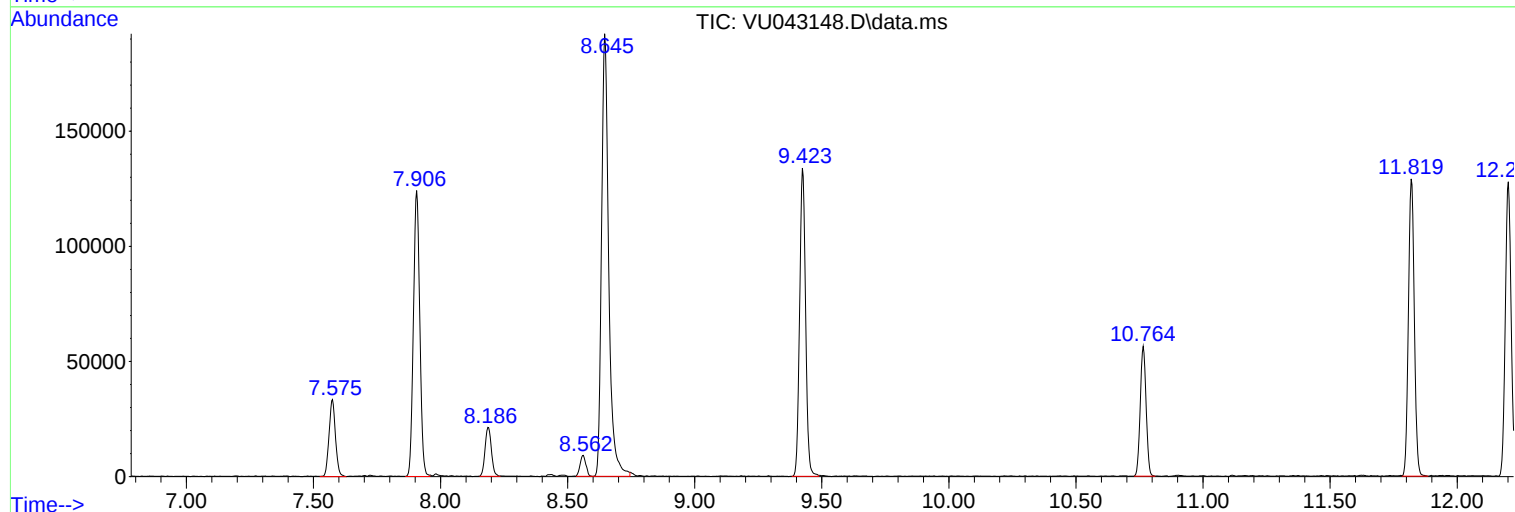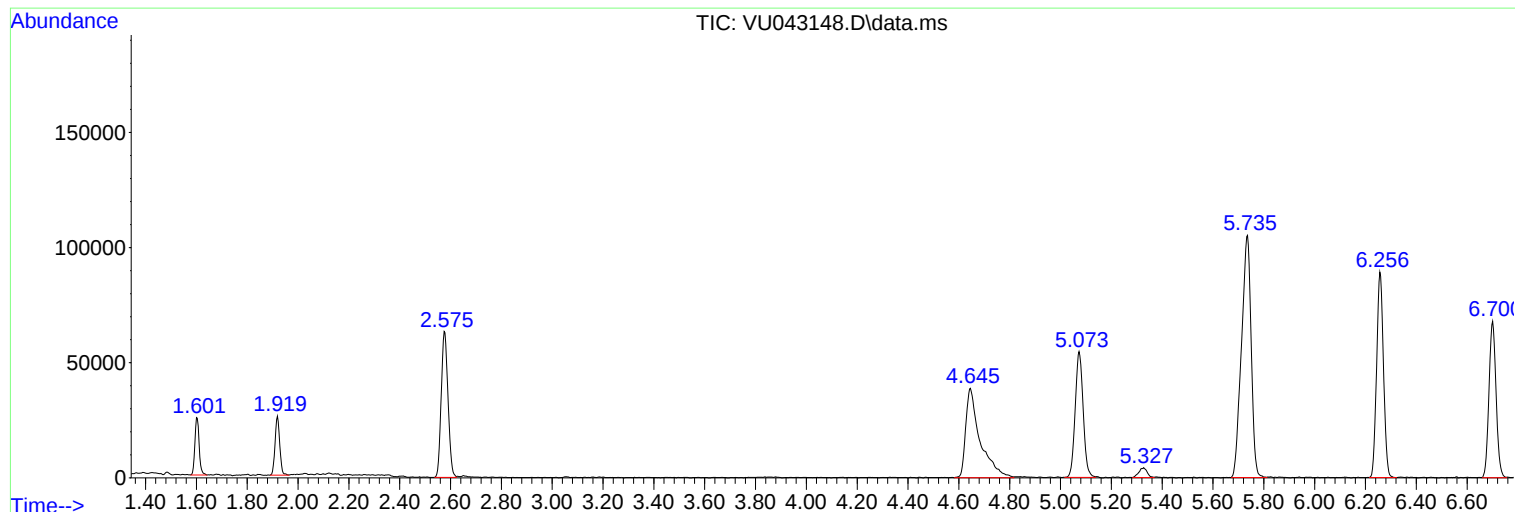

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043148.D
Acq On : 16 Apr 2021 02:34
Operator : SY/MD
Sample : M2055-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4522










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.575	1.76 ug/L	58683	1,4-Difluorobenzene	6.256

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
2			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	17
3			Cyclopropane	42	C3H6	000075-19-4	9
4			1,3-Cyclohexadiene	80	C6H8	000592-57-4	9
5			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	9

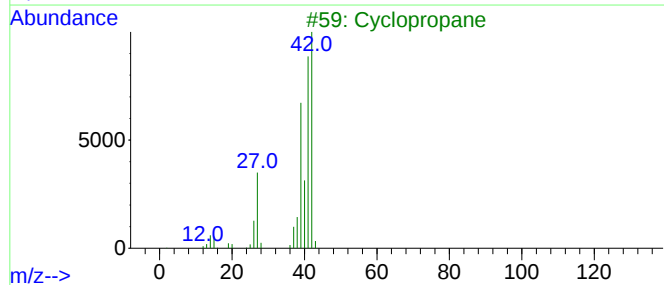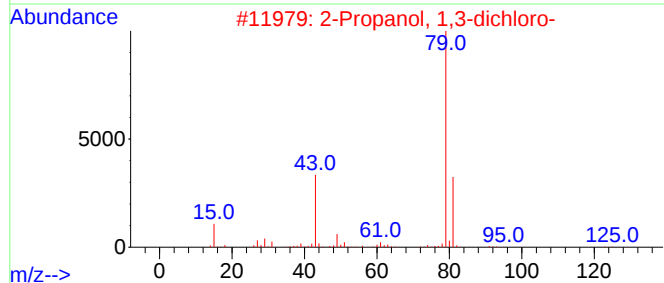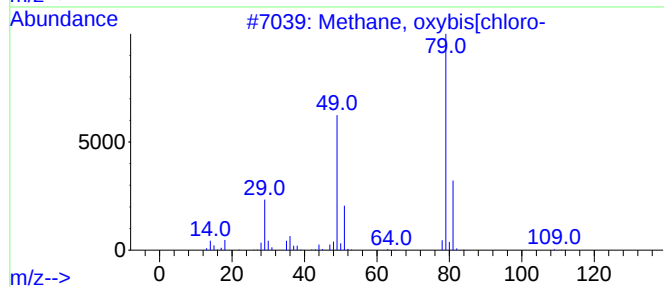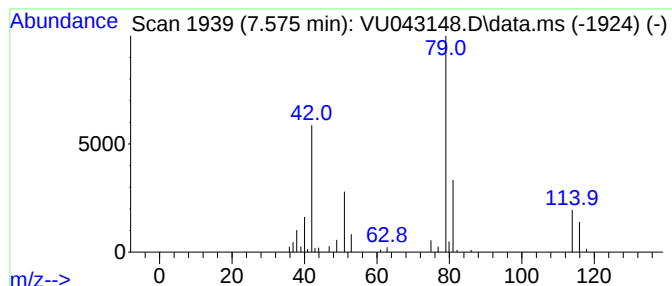

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043148.D
Acq On : 16 Apr 2021 02:34
Operator : SY/MD
Sample : M2055-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4522

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.575	1.8	ug/L	58683	1	6.256	166587	5.0