

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
 Data File : VU043151.D
 Acq On : 16 Apr 2021 03:46
 Operator : SY/MD
 Sample : M2055-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4495

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	11	17	26	rVB	13522	14029	3.66%	0.581%
2	1.604	73	82	95	rVB	26669	28987	7.56%	1.200%
3	1.919	172	180	191	rVB	25023	32201	8.40%	1.334%
4	2.572	371	383	398	rBV2	53525	88754	23.14%	3.675%
5	4.645	1009	1028	1050	rBV2	37342	130241	33.96%	5.394%
6	5.073	1145	1161	1183	rBV2	52752	118496	30.90%	4.907%
7	5.735	1341	1367	1385	rBV2	104639	277485	72.35%	11.491%
8	6.256	1516	1529	1548	rBV	89572	166663	43.46%	6.902%
9	6.700	1654	1667	1683	rBV2	67164	131308	34.24%	5.438%
10	7.575	1927	1939	1956	rBB2	33419	56435	14.71%	2.337%
11	7.726	1974	1986	1998	rVB6	3609	7030	1.83%	0.291%
12	7.906	2024	2042	2058	rBV	124384	213855	55.76%	8.856%
13	8.189	2119	2130	2142	rBV2	21381	35699	9.31%	1.478%
14	8.433	2196	2206	2216	rBV3	2808	4677	1.22%	0.194%
15	8.562	2237	2246	2258	rBV3	5177	7753	2.02%	0.321%
16	8.645	2258	2272	2304	rBV	185240	383523	100.00%	15.882%
17	9.427	2502	2515	2534	rBV	133311	219669	57.28%	9.097%
18	10.764	2920	2931	2944	rVB	56684	90999	23.73%	3.768%
19	11.819	3248	3259	3278	rBV	128669	205373	53.55%	8.505%
20	12.201	3364	3378	3392	rBV	125996	201587	52.56%	8.348%




Sum of corrected areas: 2414764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043151.D
Acq On : 16 Apr 2021 03:46
Operator : SY/MD
Sample : M2055-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4495

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

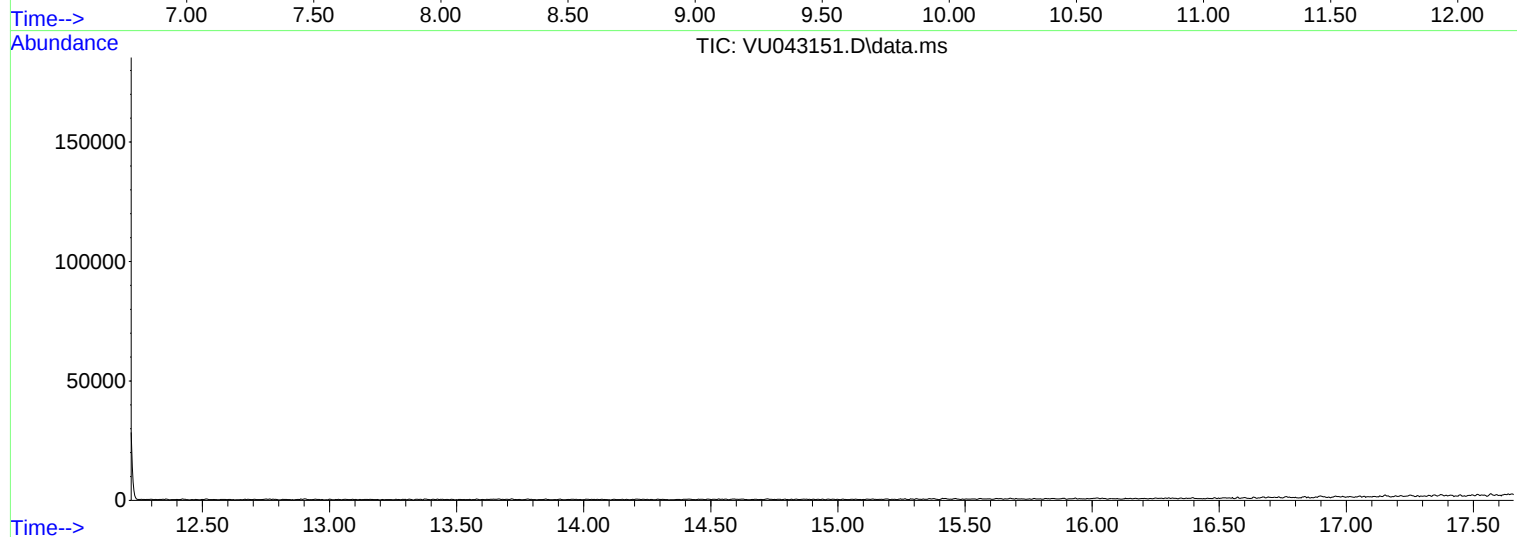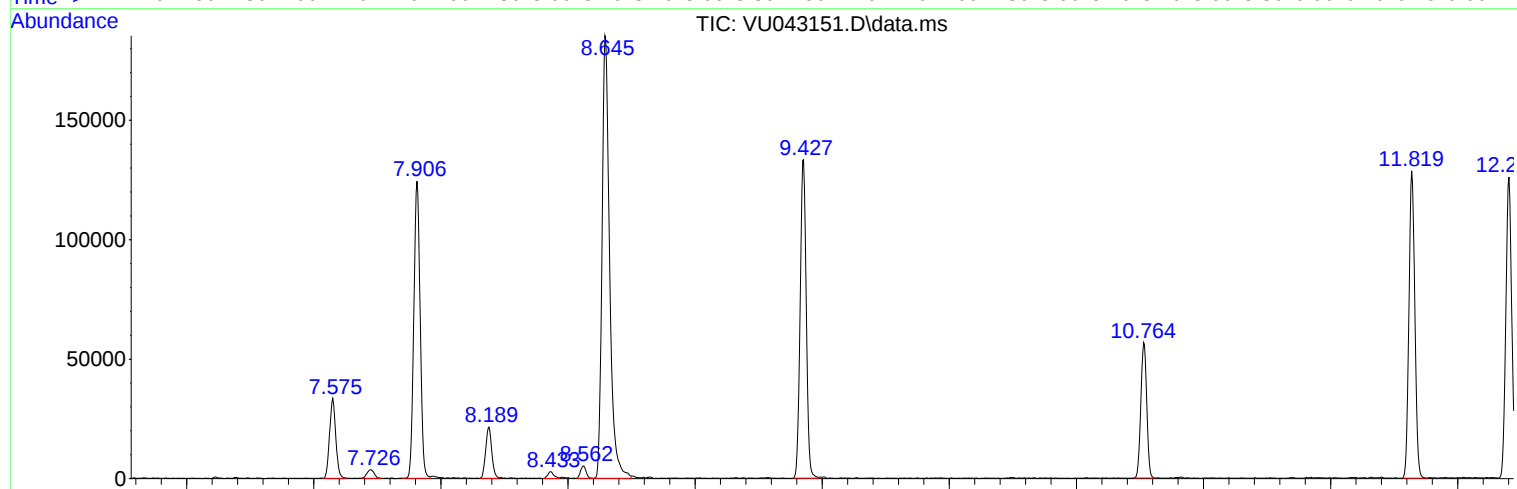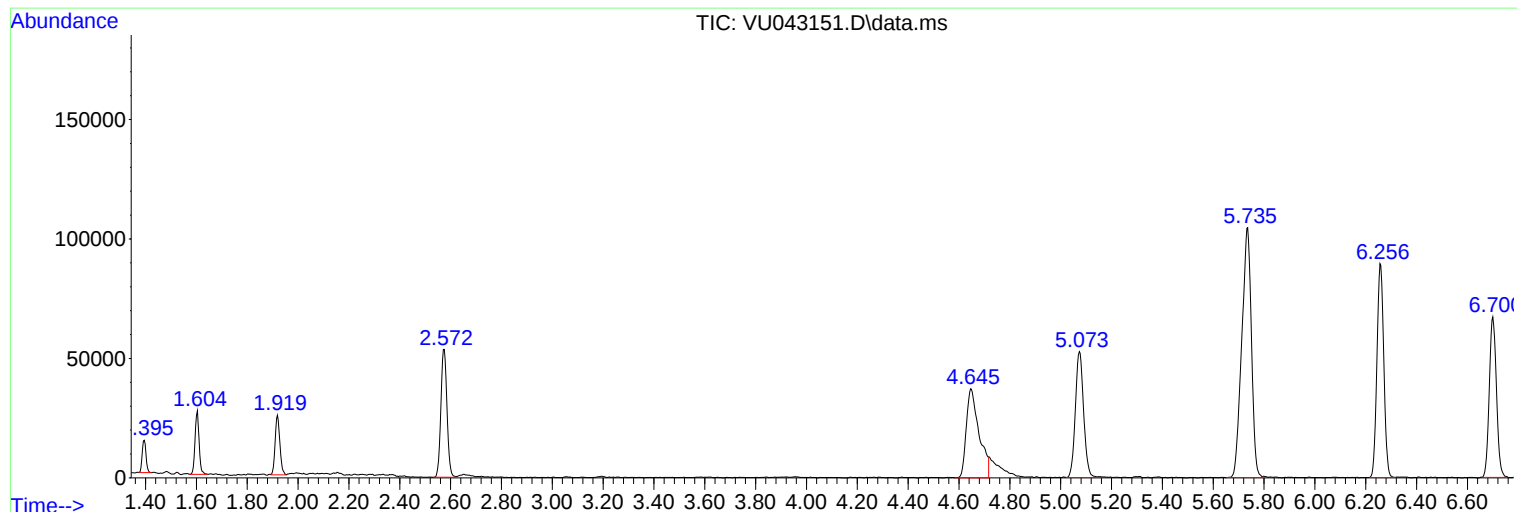

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043151.D
Acq On : 16 Apr 2021 03:46
Operator : SY/MD
Sample : M2055-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4495










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.575	1.69 ug/L	56435	1,4-Difluorobenzene	6.260

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclohexadiene	80	C6H8	000592-57-4	28
2			1,3-Cyclohexadiene	80	C6H8	000592-57-4	28
3			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
4			Cyclopropane	42	C3H6	000075-19-4	9
5			Thiophosgene	114	CCl2S	000463-71-8	9

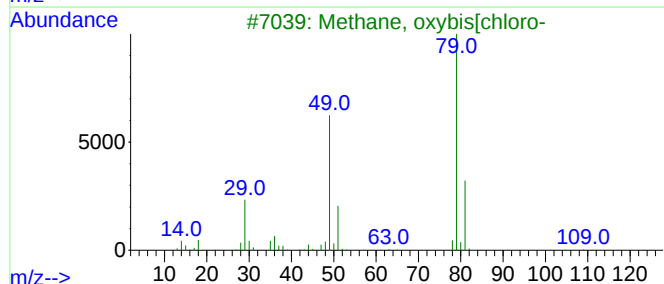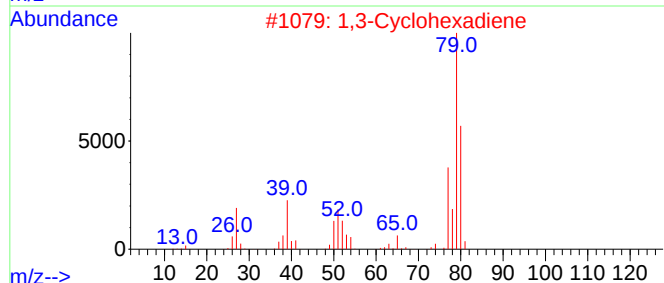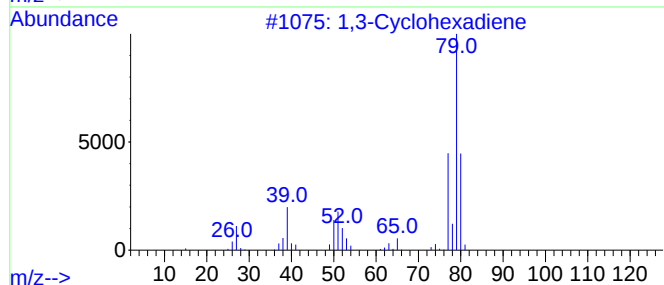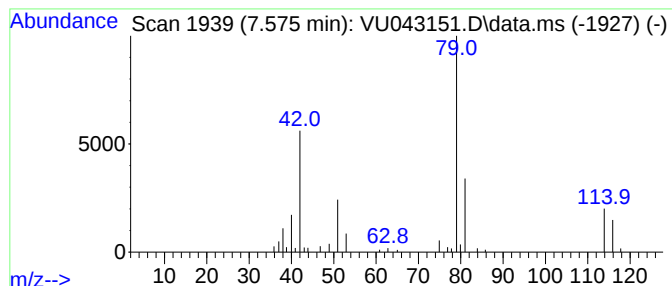

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041521\
Data File : VU043151.D
Acq On : 16 Apr 2021 03:46
Operator : SY/MD
Sample : M2055-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4495

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.575	1.7	ug/L	56435	1	6.260	166663	5.0