
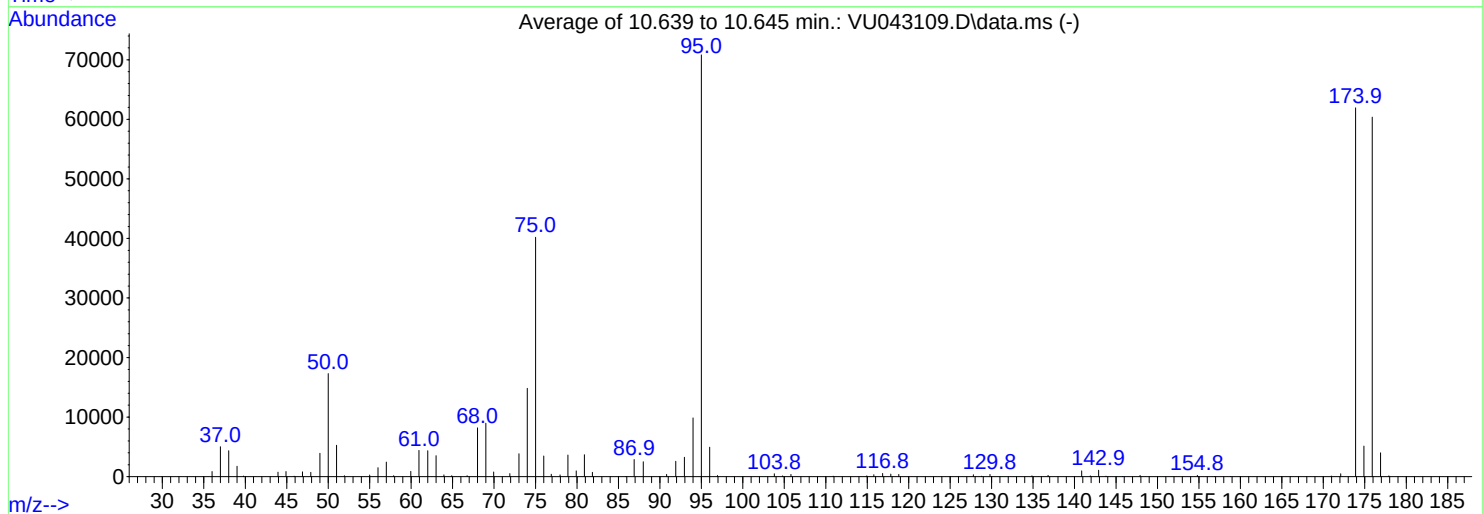


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU041521\  
 Data File : VU043109.D  
 Acq On : 15 Apr 2021 09:03  
 Operator : SY/MD  
 Sample : BFB31  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BFB131

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR041521WMA.M  
 Title : TRACE VOA SFAM1.0  
 Last Update : Fri Apr 16 07:14:05 2021

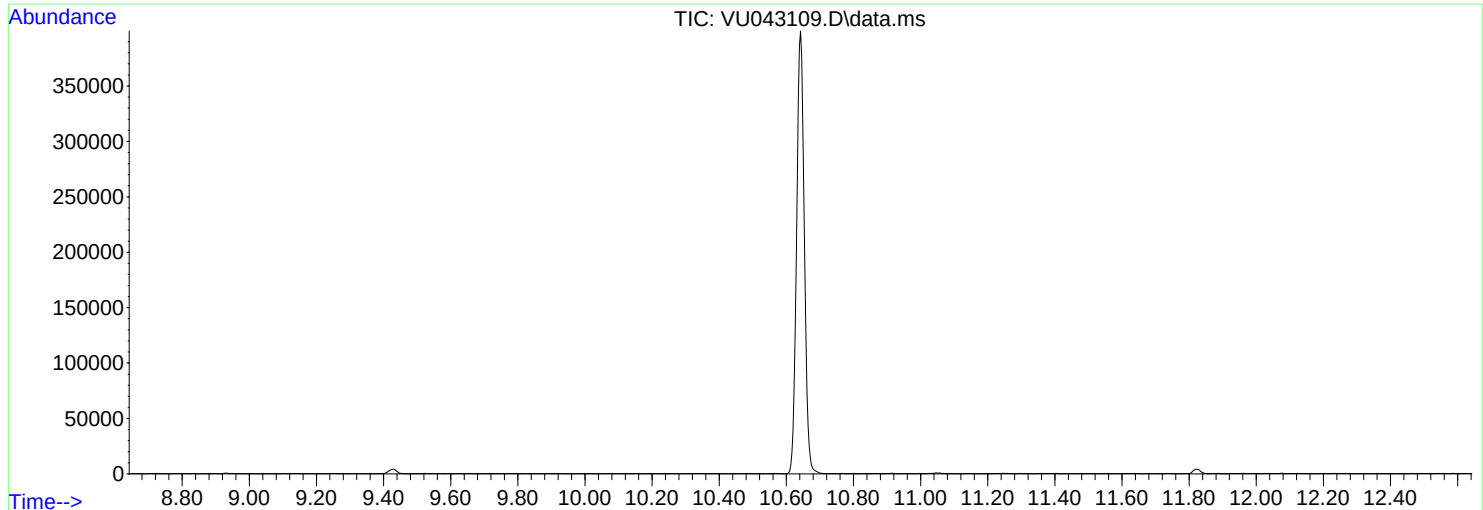

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 24.4         | 17315      | PASS                |
| 75             | 95              | 30              | 80              | 56.8         | 40205      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 70827      | PASS                |
| 96             | 95              | 5               | 9               | 7.0          | 4958       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 120             | 87.5         | 61939      | PASS                |
| 175            | 174             | 5               | 9               | 8.3          | 5126       | PASS                |
| 176            | 174             | 95              | 101             | 97.5         | 60379      | PASS                |
| 177            | 176             | 5               | 9               | 6.6          | 4007       | PASS                |

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 879.0     |
| 37.00  | 5228.0    |
| 38.00  | 4492.0    |
| 39.00  | 1808.0    |
| 39.80  | 103.0     |
| 44.00  | 961.0     |
| 44.90  | 906.0     |
| 45.90  | 100.0     |
| 46.90  | 865.0     |
| 47.90  | 769.0     |
| 49.00  | 4016.0    |
| 50.00  | 17896.0   |
| 51.00  | 5453.0    |
| 51.90  | 180.0     |
| 55.00  | 289.0     |
| 56.00  | 1549.0    |
| 57.00  | 2482.0    |
| 57.90  | 158.0     |
| 59.90  | 923.0     |
| 61.00  | 4564.0    |
| 62.00  | 4503.0    |
| 63.00  | 3640.0    |
| 63.90  | 308.0     |
| 64.90  | 170.0     |
| 66.70  | 180.0     |
| 68.00  | 8423.0    |
| 69.00  | 9259.0    |
| 69.90  | 792.0     |
| 71.90  | 536.0     |
| 73.00  | 3928.0    |
| 74.00  | 15299.0   |
| 75.00  | 41472.0   |
| 76.00  | 3596.0    |
| 76.90  | 395.0     |
| 78.00  | 296.0     |
| 78.90  | 3737.0    |
| 79.90  | 999.0     |
| 80.90  | 3793.0    |
| 81.80  | 704.0     |
| 86.90  | 3039.0    |
| 88.00  | 2586.0    |
| 90.80  | 390.0     |
| 91.90  | 2635.0    |
| 93.00  | 3347.0    |
| 94.00  | 10232.0   |
| 95.00  | 72784.0   |
| 96.00  | 5153.0    |
| 97.00  | 192.0     |
| 103.80 | 522.0     |
| 104.80 | 146.0     |
| 105.80 | 421.0     |
| 110.90 | 130.0     |
| 115.00 | 148.0     |
| 115.80 | 342.0     |
| 116.80 | 554.0     |
| 117.90 | 464.0     |
| 118.80 | 355.0     |
| 127.80 | 350.0     |
| 128.80 | 129.0     |
| 129.80 | 402.0     |
| 134.90 | 152.0     |
| 136.80 | 230.0     |
| 140.80 | 1014.0    |
| 141.90 | 132.0     |
| 142.90 | 1104.0    |
| 143.80 | 111.0     |
| 147.90 | 232.0     |
| 154.80 | 238.0     |
| 170.90 | 122.0     |
| 172.10 | 485.0     |
| 173.90 | 63880.0   |
| 174.90 | 5285.0    |
| 175.90 | 62312.0   |
| 176.90 | 4189.0    |
| 177.90 | 144.0     |

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB131

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 914.0     |
| 37.00  | 5122.0    |
| 38.00  | 4400.0    |
| 39.00  | 1747.0    |
| 39.70  | 135.0     |
| 44.00  | 944.0     |
| 44.90  | 909.0     |
| 45.90  | 121.0     |
| 46.90  | 841.0     |
| 47.90  | 731.0     |
| 49.00  | 4076.0    |
| 50.00  | 17592.0   |
| 51.00  | 5451.0    |
| 51.90  | 176.0     |
| 55.00  | 244.0     |
| 56.00  | 1543.0    |
| 57.00  | 2683.0    |
| 57.90  | 161.0     |
| 60.00  | 897.0     |
| 60.90  | 4409.0    |
| 62.00  | 4212.0    |
| 63.00  | 3606.0    |
| 64.00  | 286.0     |
| 64.90  | 166.0     |
| 66.70  | 198.0     |
| 68.00  | 8234.0    |
| 69.00  | 9024.0    |
| 70.00  | 834.0     |
| 71.90  | 522.0     |
| 73.00  | 3878.0    |
| 74.00  | 14841.0   |
| 75.00  | 39912.0   |
| 76.00  | 3413.0    |
| 76.90  | 442.0     |
| 77.90  | 320.0     |
| 78.90  | 3799.0    |
| 79.90  | 1038.0    |
| 80.90  | 3860.0    |
| 81.80  | 778.0     |
| 85.90  | 102.0     |
| 86.90  | 2866.0    |
| 88.00  | 2367.0    |
| 90.80  | 391.0     |
| 91.90  | 2618.0    |
| 93.00  | 3341.0    |
| 94.00  | 9837.0    |
| 95.00  | 70872.0   |
| 96.00  | 5277.0    |
| 96.90  | 224.0     |
| 103.80 | 427.0     |
| 104.70 | 137.0     |
| 105.80 | 383.0     |
| 110.90 | 131.0     |
| 115.00 | 113.0     |
| 115.80 | 310.0     |
| 116.80 | 527.0     |
| 117.90 | 481.0     |
| 118.80 | 391.0     |
| 127.80 | 344.0     |
| 129.80 | 330.0     |
| 134.90 | 174.0     |
| 136.80 | 215.0     |
| 140.80 | 967.0     |
| 141.90 | 130.0     |
| 142.90 | 990.0     |
| 143.80 | 105.0     |
| 145.80 | 101.0     |
| 147.90 | 198.0     |
| 154.80 | 224.0     |
| 156.90 | 107.0     |
| 170.90 | 106.0     |
| 172.10 | 449.0     |
| 173.90 | 60424.0   |
| 174.90 | 5178.0    |
| 175.90 | 58576.0   |
| 176.90 | 3954.0    |
| 177.90 | 163.0     |

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB131

| m/z   | Abundance |
|-------|-----------|
| 44.00 | 188.0     |

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB131

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 765.0     |
| 37.00  | 4698.0    |
| 38.00  | 4208.0    |
| 39.00  | 1689.0    |
| 39.90  | 115.0     |
| 43.90  | 896.0     |
| 44.90  | 808.0     |
| 46.90  | 756.0     |
| 47.90  | 670.0     |
| 49.00  | 3653.0    |
| 50.00  | 16456.0   |
| 51.00  | 4880.0    |
| 52.00  | 169.0     |
| 55.00  | 289.0     |
| 56.00  | 1414.0    |
| 57.00  | 2167.0    |
| 57.90  | 149.0     |
| 59.90  | 873.0     |
| 61.00  | 4218.0    |
| 62.00  | 4320.0    |
| 63.00  | 3306.0    |
| 63.90  | 321.0     |
| 64.90  | 155.0     |
| 66.80  | 140.0     |
| 68.00  | 7925.0    |
| 69.00  | 8620.0    |
| 69.90  | 714.0     |
| 71.90  | 490.0     |
| 73.00  | 3704.0    |
| 74.00  | 14391.0   |
| 75.00  | 39232.0   |
| 76.00  | 3391.0    |
| 76.90  | 397.0     |
| 78.00  | 256.0     |
| 78.90  | 3340.0    |
| 79.90  | 866.0     |
| 80.90  | 3406.0    |
| 81.90  | 666.0     |
| 86.90  | 2763.0    |
| 88.00  | 2568.0    |
| 90.80  | 380.0     |
| 91.90  | 2463.0    |
| 92.90  | 3108.0    |
| 94.00  | 9538.0    |
| 95.00  | 68824.0   |
| 96.00  | 4443.0    |
| 97.00  | 130.0     |
| 103.80 | 505.0     |
| 104.90 | 158.0     |
| 105.80 | 367.0     |
| 114.90 | 122.0     |
| 115.80 | 332.0     |
| 116.90 | 541.0     |
| 117.80 | 371.0     |
| 118.80 | 355.0     |
| 127.80 | 324.0     |
| 128.80 | 126.0     |
| 129.80 | 415.0     |
| 134.80 | 126.0     |
| 136.80 | 196.0     |
| 140.90 | 964.0     |
| 141.90 | 142.0     |
| 142.90 | 1100.0    |
| 147.90 | 244.0     |
| 154.80 | 208.0     |
| 158.80 | 111.0     |
| 171.00 | 112.0     |
| 172.10 | 483.0     |
| 173.90 | 61512.0   |
| 174.90 | 4914.0    |
| 175.90 | 60248.0   |
| 176.90 | 3877.0    |
| 177.90 | 107.0     |

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB131