

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048095.D
 Acq On : 15 Apr 2022 11:27
 Operator : SY/MD
 Sample : VU0415MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Quant Time: Apr 20 12:08:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 20 02:08:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	303790	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	326314	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	168678	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	75724	34.373	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.740%		
7) Chloroethane-d5	1.916	69	75558	43.498	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.000%		
11) 1,1-Dichloroethene-d2	2.568	63	108272	26.863	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	53.720%#		
21) 2-Butanone-d5	4.620	46	198623	105.044	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	105.040%		
24) Chloroform-d	5.067	84	191947	47.619	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.240%		
26) 1,2-Dichloroethane-d4	5.703	65	125590	50.801	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.600%		
32) Benzene-d6	5.729	84	368337	44.859	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.720%		
36) 1,2-Dichloropropane-d6	6.694	67	128402	50.920	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.840%		
41) Toluene-d8	7.899	98	311996	39.000	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.000%#		
43) trans-1,3-Dichloroprop...	8.182	79	52846	41.366	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.740%		
47) 2-Hexanone-d5	8.632	63	135284	91.644	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.640%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	209133	48.325	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.660%		
66) 1,2-Dichlorobenzene-d4	12.195	152	147092	49.015	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.040%		
Target Compounds						Qvalue
51) Chlorobenzene	9.449	112	11285	1.604	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048095.D
Acq On : 15 Apr 2022 11:27
Operator : SY/MD
Sample : VU0415MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Time: Apr 20 12:08:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 20 02:08:53 2022
Response via : Initial Calibration

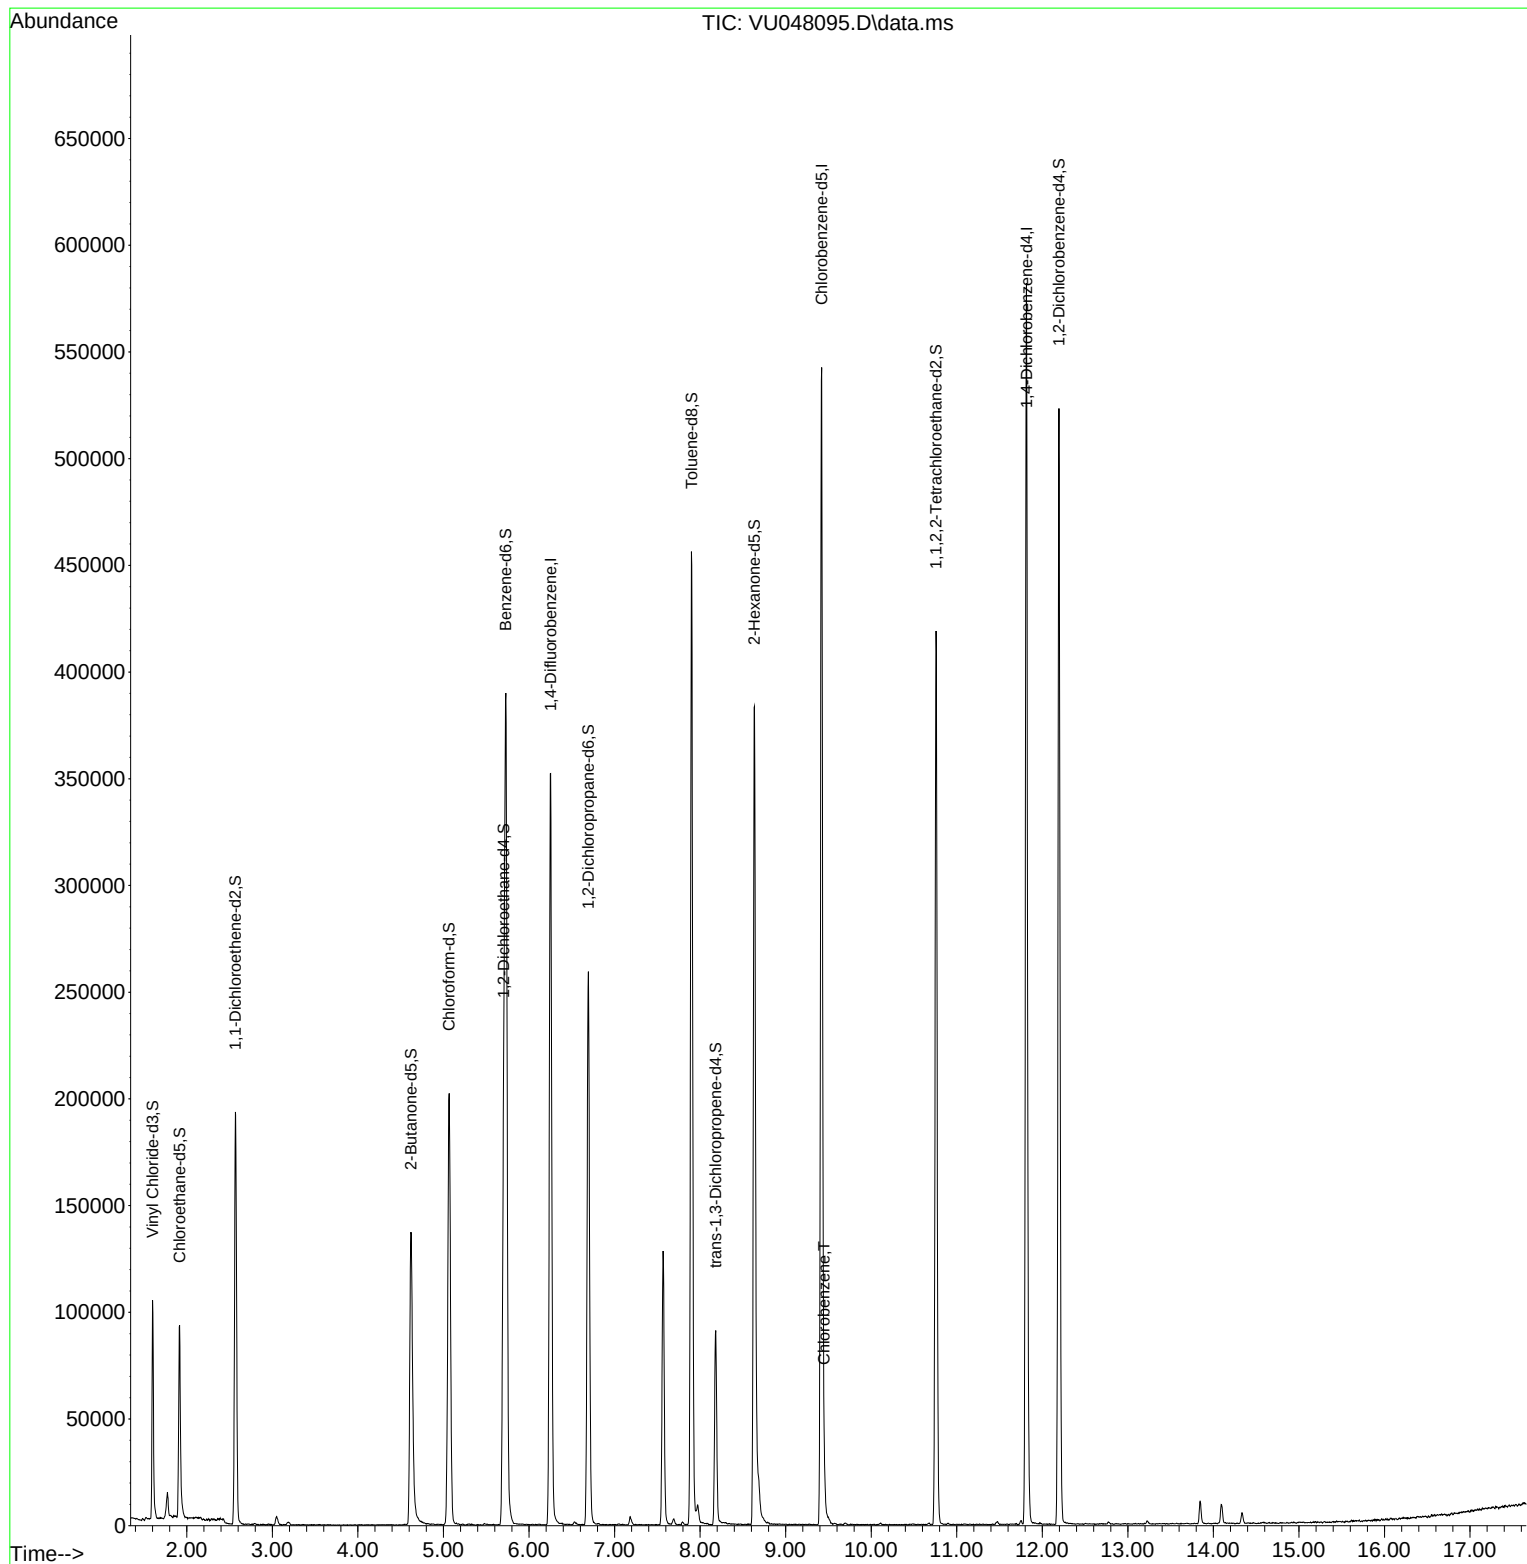

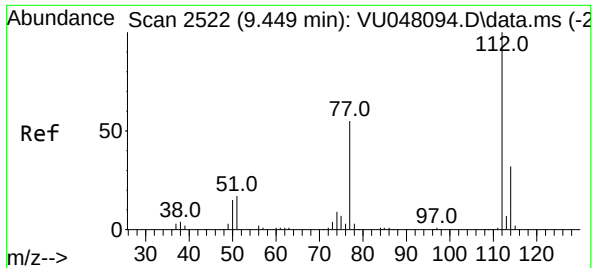

#51
 Chlorobenzene
 Concen: 1.604 ug/L
 RT: 9.449 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VU048095.D
 Acq: 15 Apr 2022 11:27

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Tgt Ion:112	Resp:	11285
Ion Ratio	Lower	Upper
112	100	
114	29.9	22.1 41.1
77	49.2	43.4 65.0

