

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048098.D
 Acq On : 15 Apr 2022 13:26
 Operator : SY/MD
 Sample : N2373-07ME
 Misc : 5.02g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFFD8ME

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 04/18/2022
 Supervised By :Mahesh Dadoda 04/20/2022

Quant Time: Apr 16 00:35:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 16 00:34:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	263705	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	252362	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	115593	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	48873	25.557	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	51.120%#		
7) Chloroethane-d5	1.900	69	37224m	24.687	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	49.380%#		
11) 1,1-Dichloroethene-d2	2.543	63	60974	17.428	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	34.860%#		
21) 2-Butanone-d5	4.646	46	166295	101.315	ug/L	0.03
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.320%		
24) Chloroform-d	5.064	84	138209	39.500	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.000%		
26) 1,2-Dichloroethane-d4	5.703	65	101619	47.353	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.700%		
32) Benzene-d6	5.723	84	252662	39.788	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.580%		
36) 1,2-Dichloropropane-d6	6.690	67	98007	50.255	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.520%		
41) Toluene-d8	7.899	98	184942	29.892	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	59.780%#		
43) trans-1,3-Dichloroprop...	8.182	79	35633	36.066	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	72.140%		
47) 2-Hexanone-d5	8.665	63	119076	104.303	ug/L	0.03
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.300%		
56) 1,1,2,2-Tetrachloroeth...	10.767	84	167980	50.190	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.380%		
66) 1,2-Dichlorobenzene-d4	12.198	152	79899	38.852	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	77.700%#		
Target Compounds						Qvalue
51) Chlorobenzene	9.452	112	12036	2.212	ug/L	95
65) 1,4-Dichlorobenzene	11.841	146	8004	2.225	ug/L	95
67) 1,2-Dichlorobenzene	12.221	146	6267	1.804	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048098.D
Acq On : 15 Apr 2022 13:26
Operator : SY/MD
Sample : N2373-07ME
Misc : 5.02g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BFFD8ME

Quant Time: Apr 16 00:35:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 16 00:34:16 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 04/18/2022
Supervised By :Mahesh Dadoda 04/20/2022

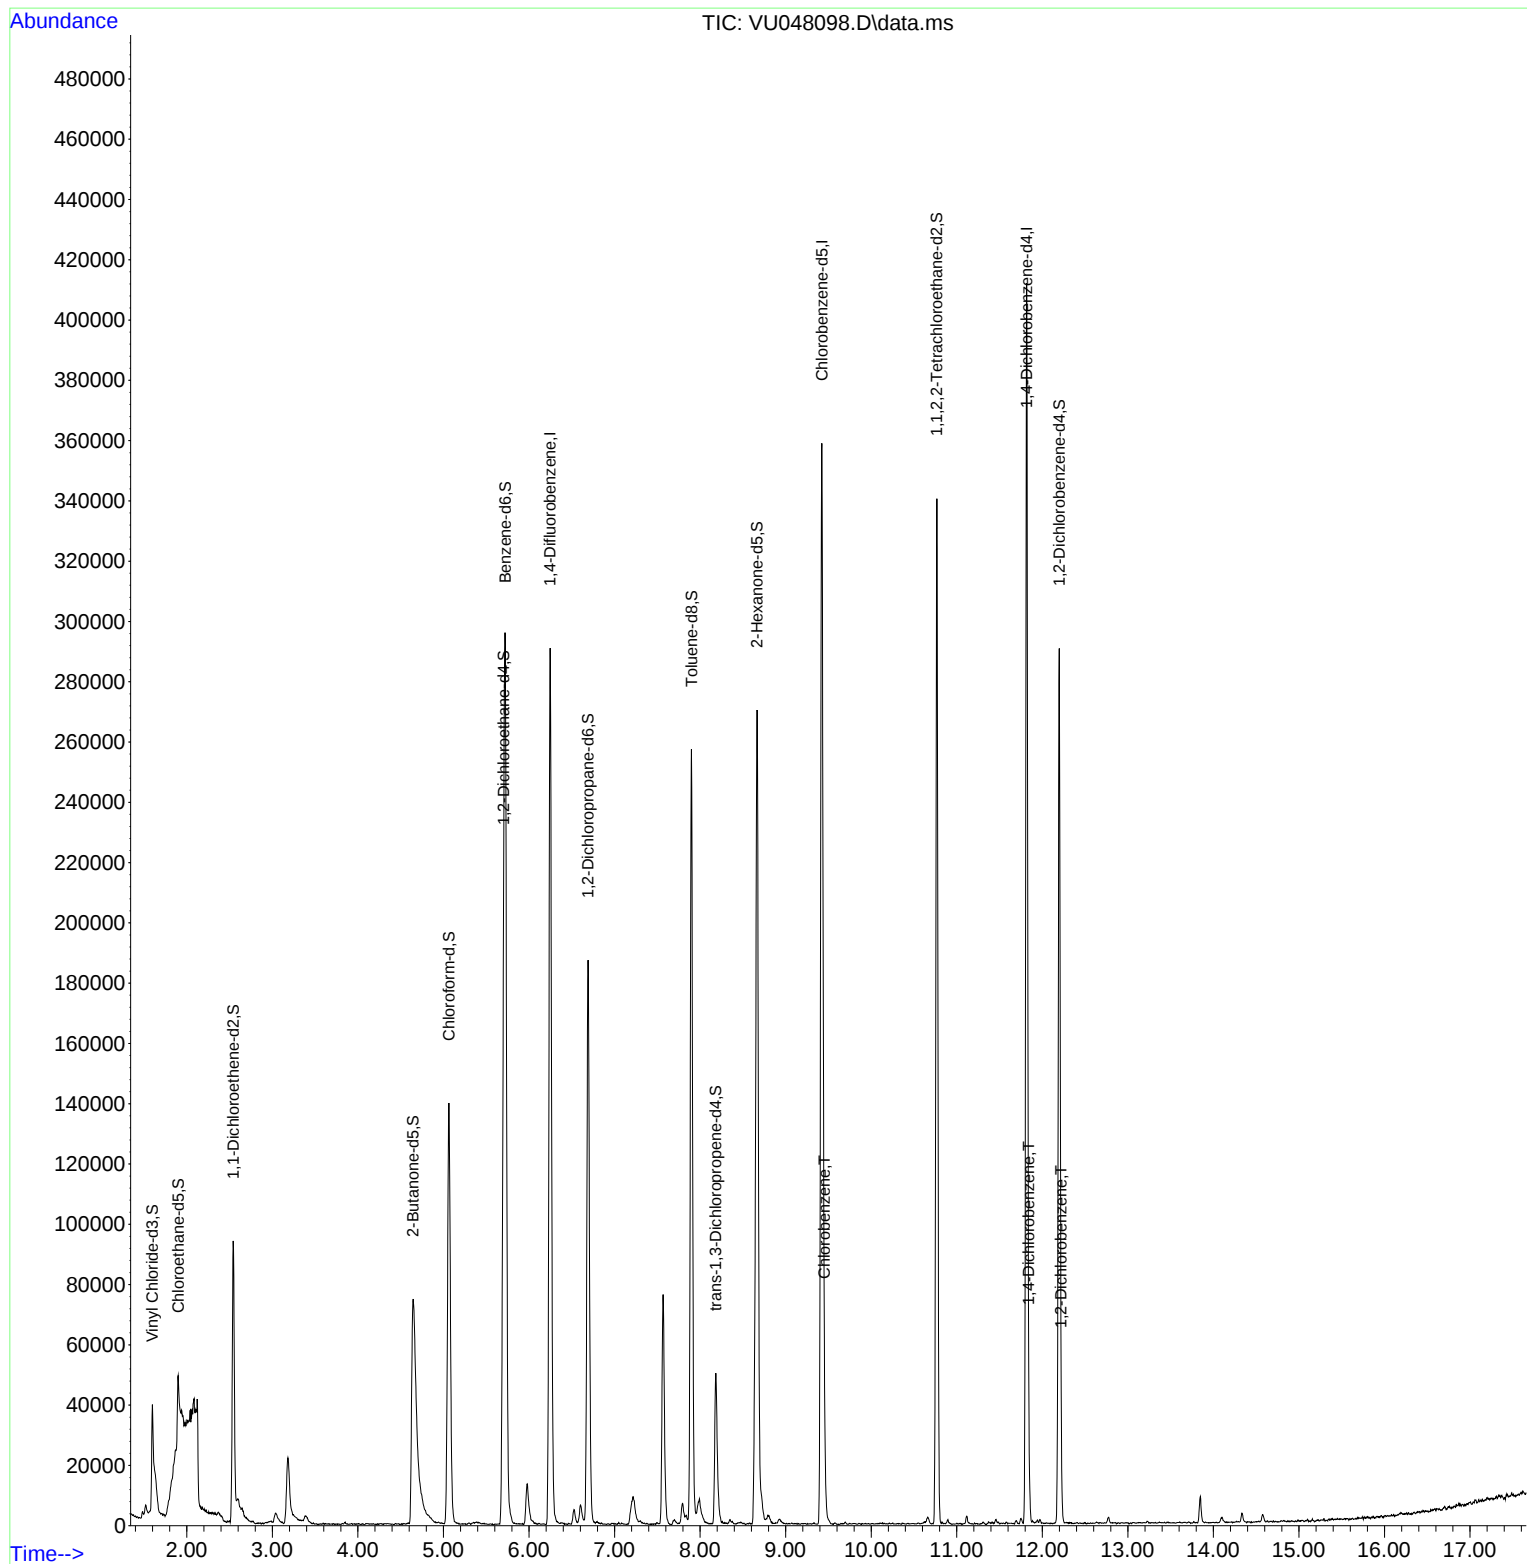

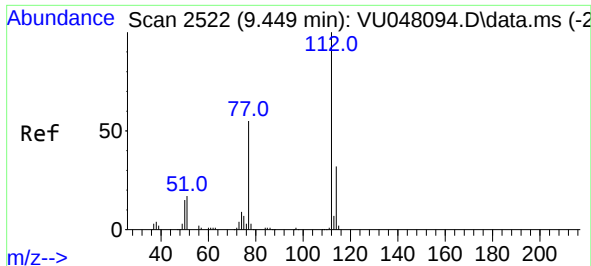

#51
Chlorobenzene
Concen: 2.212 ug/L
RT: 9.452 min Scan# 21
Delta R.T. 0.003 min
Lab File: VU048098.D
Acq: 15 Apr 2022 13:26




Instrument :
MSVOA_U
ClientSampleId :
BFFD8ME

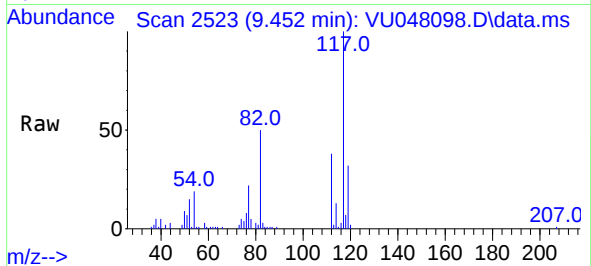


Tgt Ion:112 Resp: 1203
Ion Ratio Lower Upper
112 100
114 34.7 22.1 41.1
77 58.0 43.4 65.0

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 04/18/2022
Supervised By :Mahesh Dadoda 04/20/2022

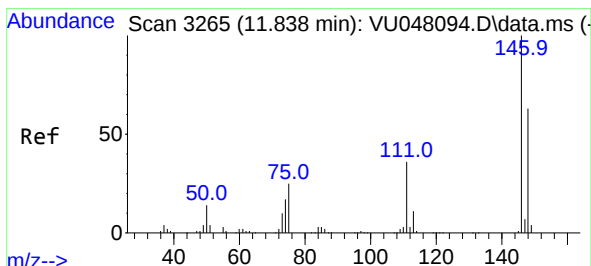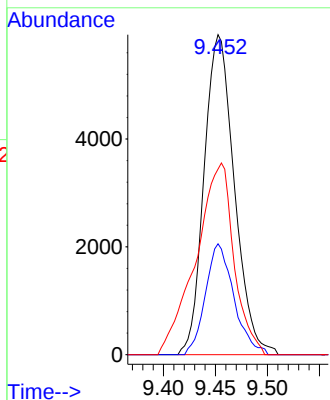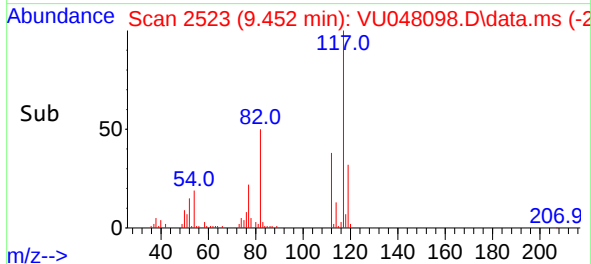


#65
1,4-Dichlorobenzene
Concen: 2.225 ug/L
RT: 11.841 min Scan# 3266
Delta R.T. 0.003 min
Lab File: VU048098.D
Acq: 15 Apr 2022 13:26

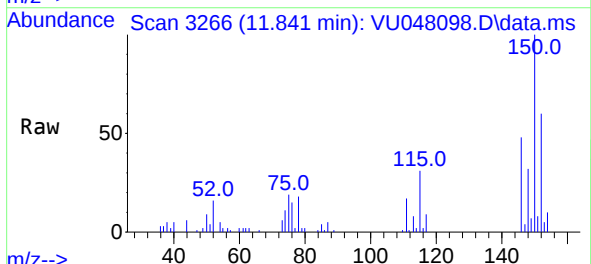


Tgt Ion:146 Resp: 8004
Ion Ratio Lower Upper
146 100
111 38.5 25.3 47.1
148 67.6 44.5 82.7

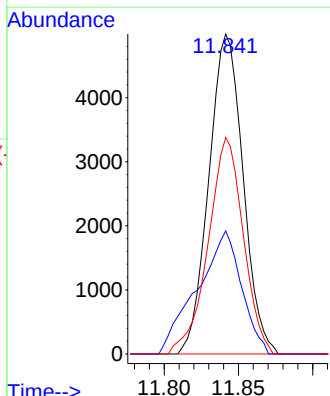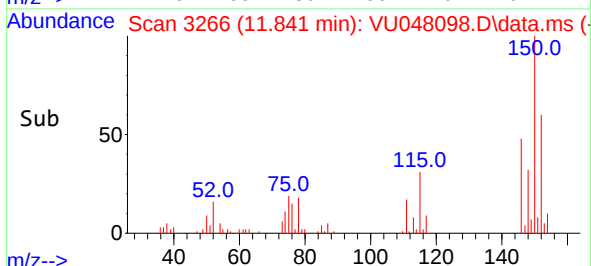


Abundance Scan 3382 (12.214 min): VU048094.D\data.ms (-

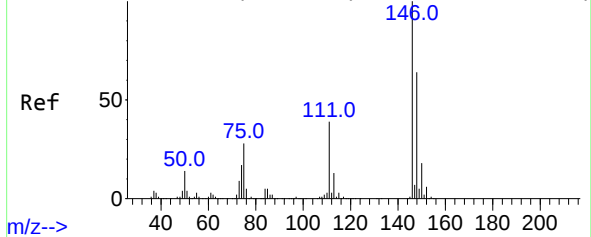

Abundance Scan 3384 (12.221 min): VU048098.D\data.ms (-

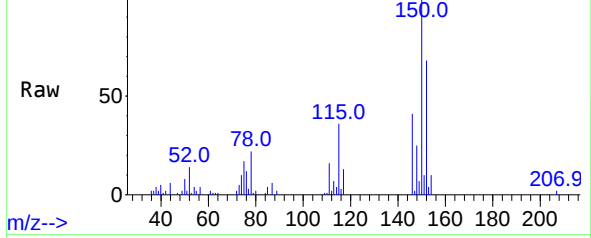

Abundance Scan 3384 (12.221 min): VU048098.D\data.ms (-

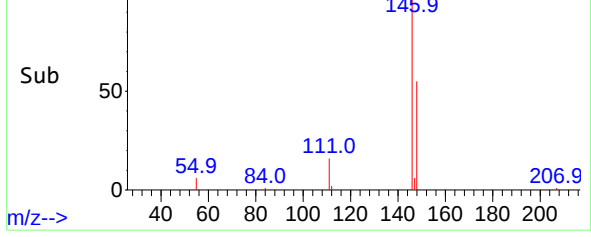

#67
1,2-Dichlorobenzene
Concen: 1.804 ug/L
RT: 12.221 min Scan# 31
Delta R.T. 0.006 min
Lab File: VU048098.D
Acq: 15 Apr 2022 13:26

Instrument :
MSVOA_U
ClientSampleId :
BFFD8ME

Tgt Ion:	146	Resp:	626
Ion	Ratio	Lower	Upper
146	100		
111	38.1	31.7	47.5
148	60.5	51.4	77.2

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 04/18/2022
Supervised By :Mahesh Dadoda 04/20/2022

