

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048100.D
 Acq On : 15 Apr 2022 14:12
 Operator : SY/MD
 Sample : N2345-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Apr 16 00:36:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 16 00:34:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	417539	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	418254	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	214355	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	135402	44.719	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	89.440%	
7) Chloroethane-d5	1.916	69	107346	44.962	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	89.920%	
11) 1,1-Dichloroethene-d2	2.568	63	167567	30.248	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	60.500%	
21) 2-Butanone-d5	4.629	46	179604	69.109	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	69.110%	
24) Chloroform-d	5.067	84	211579	38.190	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	76.380%	
26) 1,2-Dichloroethane-d4	5.703	65	134739	39.654	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	79.300%	
32) Benzene-d6	5.729	84	452057	42.953	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	85.900%	
36) 1,2-Dichloropropane-d6	6.690	67	141738	43.853	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	87.700%	
41) Toluene-d8	7.899	98	395256	38.547	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	77.100%#	
43) trans-1,3-Dichloroprop...	8.179	79	57749	35.267	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	70.540%	
47) 2-Hexanone-d5	8.636	63	123887	65.476	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	65.480%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	199753	36.011	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	72.020%	
66) 1,2-Dichlorobenzene-d4	12.195	152	156788	41.113	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	82.220%	
Target Compounds						
					Qvalue	
51) Chlorobenzene	9.446	112	8582	0.951	ug/L	90
65) 1,4-Dichlorobenzene	11.838	146	6302	0.945	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048100.D
Acq On : 15 Apr 2022 14:12
Operator : SY/MD
Sample : N2345-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Apr 16 00:36:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 16 00:34:16 2022
Response via : Initial Calibration




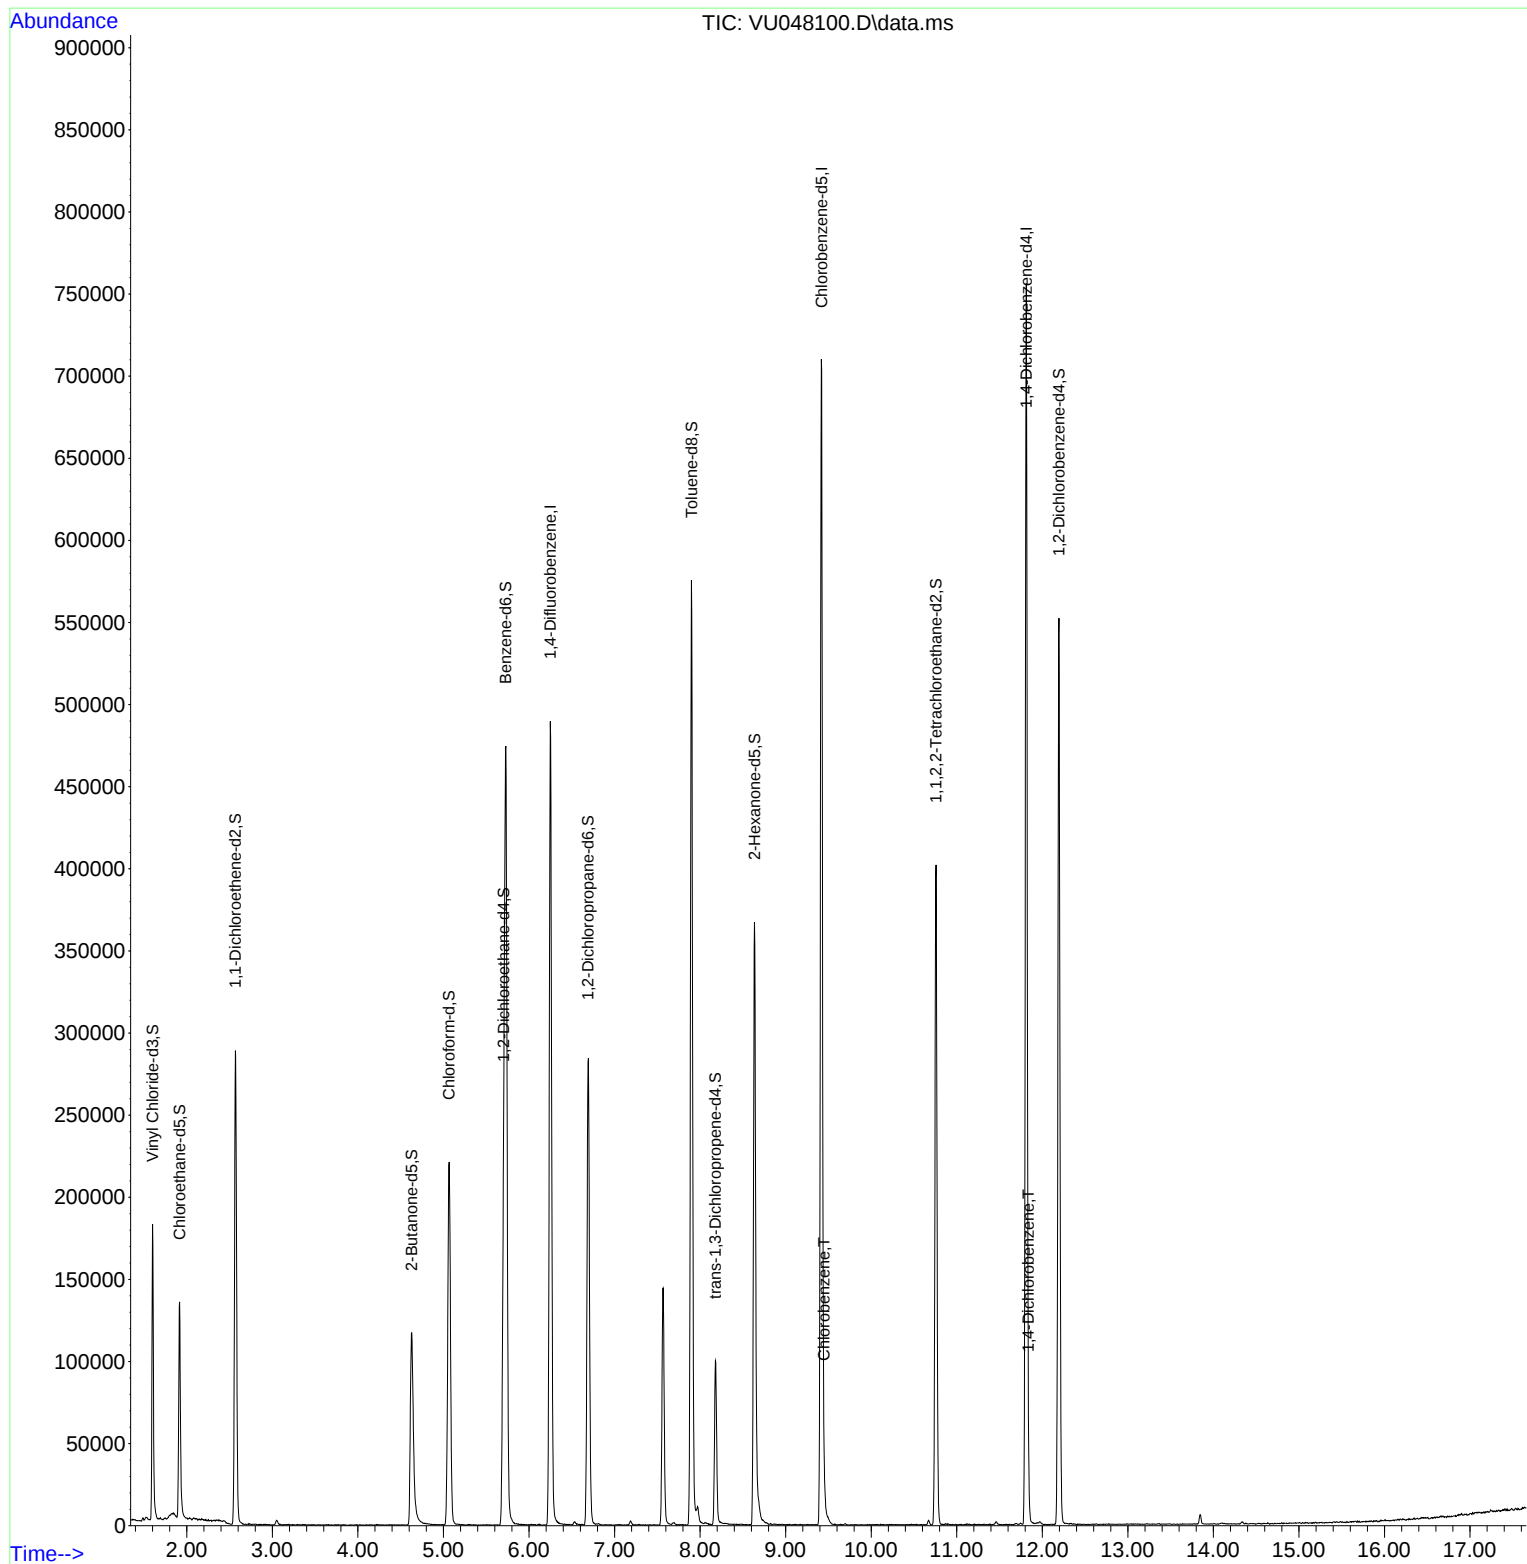


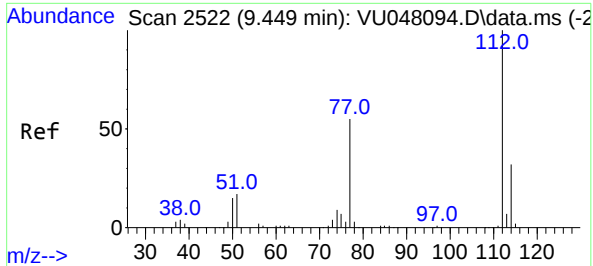

#51
Chlorobenzene
Concen: 0.951 ug/L
RT: 9.446 min Scan# 211
Delta R.T. -0.003 min
Lab File: VU048100.D
Acq: 15 Apr 2022 14:12

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Tgt Ion:112	Resp:	8582
Ion Ratio	Lower	Upper
112	100	
114	30.3	22.1 41.1
77	64.1	43.4 65.0

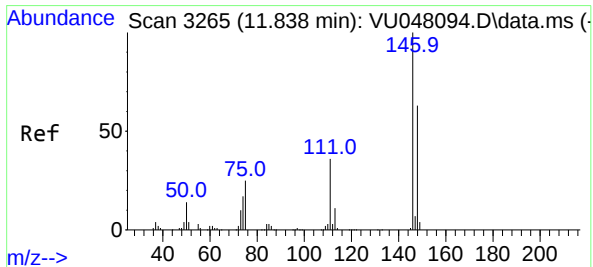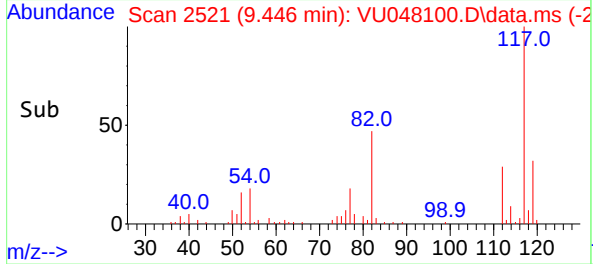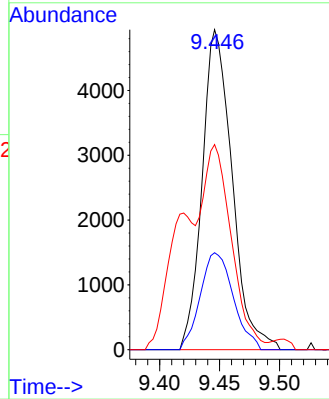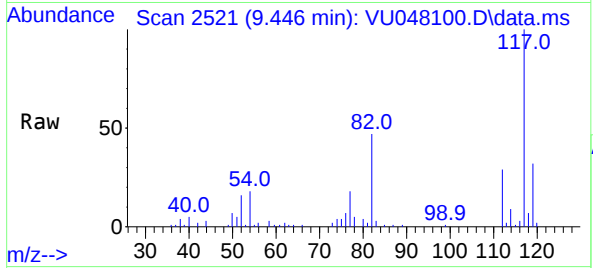

#65
1,4-Dichlorobenzene
Concen: 0.945 ug/L
RT: 11.838 min Scan# 3265
Delta R.T. -0.000 min
Lab File: VU048100.D
Acq: 15 Apr 2022 14:12

Tgt Ion:146	Resp:	6302
Ion Ratio	Lower	Upper
146	100	
111	43.4	25.3 47.1
148	71.0	44.5 82.7

