

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048095.D
 Acq On : 15 Apr 2022 11:27
 Operator : SY/MD
 Sample : VU0415MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rVB	102226	120572	11.15%	1.328%
2	1.774	126	135	143	rBV3	11173	15698	1.45%	0.173%
3	1.916	170	179	199	rVB	90209	132974	12.30%	1.465%
4	2.568	370	382	399	rBV	193212	318019	29.41%	3.503%
5	2.687	413	419	422	rBV2	247	267	0.02%	0.003%
6	2.935	492	496	498	rBV2	239	193	0.02%	0.002%
7	2.961	500	504	508	rVV2	525	528	0.05%	0.006%
8	3.051	521	532	544	rBV3	3903	7623	0.71%	0.084%
9	3.093	544	545	549	rVB2	408	241	0.02%	0.003%
10	3.131	553	557	561	rBV	278	306	0.03%	0.003%
11	3.186	566	574	575	rBV3	1120	1377	0.13%	0.015%
12	3.305	605	611	612	rBV2	229	198	0.02%	0.002%
13	3.359	623	628	630	rVV2	345	303	0.03%	0.003%
14	3.491	666	669	674	rBV2	260	218	0.02%	0.002%
15	3.517	674	677	683	rBV2	204	241	0.02%	0.003%
16	3.594	697	701	706	rBV2	205	219	0.02%	0.002%
17	3.652	711	719	722	rVB2	231	288	0.03%	0.003%
18	4.002	825	828	831	rBV2	240	221	0.02%	0.002%
19	4.163	873	878	880	rBV2	279	181	0.02%	0.002%
20	4.485	975	978	982	rBV2	222	186	0.02%	0.002%
21	4.523	987	990	994	rBV2	200	188	0.02%	0.002%
22	4.543	994	996	999	rBV	279	209	0.02%	0.002%
23	4.620	1005	1020	1045	rBV	137098	325642	30.12%	3.587%
24	5.067	1135	1159	1183	rBV	202123	443855	41.05%	4.889%
25	5.150	1183	1185	1190	rVB2	555	345	0.03%	0.004%
26	5.301	1226	1232	1236	rVB4	481	621	0.06%	0.007%
27	5.330	1236	1241	1243	rBV2	444	374	0.03%	0.004%
28	5.478	1280	1287	1292	rBV2	759	1031	0.10%	0.011%
29	5.514	1296	1298	1304	rVB	318	208	0.02%	0.002%
30	5.729	1343	1365	1393	rVV2	389631	1081205	100.00%	11.909%
31	5.973	1436	1441	1445	rBV2	222	288	0.03%	0.003%
32	6.044	1459	1463	1467	rVB3	243	235	0.02%	0.003%
33	6.253	1513	1528	1559	rVV	351938	680561	62.94%	7.496%
34	6.446	1586	1588	1593	rVB3	246	186	0.02%	0.002%
35	6.533	1608	1615	1620	rVV2	1310	1780	0.16%	0.020%
36	6.555	1620	1622	1629	rVB2	736	550	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048095.D
 Acq On : 15 Apr 2022 11:27
 Operator : SY/MD
 Sample : VU0415MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1684	rBV	259248	507973	46.98%	5.595%
38	6.941	1739	1742	1744	rBV	296	214	0.02%	0.002%
39	7.044	1766	1774	1776	rBV2	432	459	0.04%	0.005%
40	7.182	1809	1817	1833	rVB	3900	6723	0.62%	0.074%
41	7.247	1834	1837	1842	rVB2	316	266	0.02%	0.003%
42	7.282	1842	1848	1850	rBV2	194	241	0.02%	0.003%
43	7.488	1910	1912	1916	rVB	318	201	0.02%	0.002%
44	7.568	1925	1937	1958	rBV	128294	227245	21.02%	2.503%
45	7.694	1967	1976	1988	rVB5	2802	5076	0.47%	0.056%
46	7.764	1996	1998	2002	rVB2	350	267	0.02%	0.003%
47	7.793	2002	2007	2014	rBV6	1380	2134	0.20%	0.024%
48	7.842	2019	2022	2026	rBV3	273	228	0.02%	0.003%
49	7.899	2026	2040	2055	rBV	455886	794523	73.48%	8.751%
50	8.182	2116	2128	2142	rBV	90971	156961	14.52%	1.729%
51	8.446	2207	2210	2212	rBV	354	216	0.02%	0.002%
52	8.552	2241	2243	2247	rBV3	350	208	0.02%	0.002%
53	8.636	2256	2269	2314	rBV	383575	727635	67.30%	8.015%
54	9.041	2393	2395	2399	rVV	365	288	0.03%	0.003%
55	9.092	2407	2411	2413	rBV2	196	194	0.02%	0.002%
56	9.118	2417	2419	2425	rVB2	290	235	0.02%	0.003%
57	9.263	2460	2464	2466	rBV	210	176	0.02%	0.002%
58	9.276	2466	2468	2472	rVV3	334	246	0.02%	0.003%
59	9.324	2480	2483	2486	rBV3	274	186	0.02%	0.002%
60	9.420	2499	2513	2536	rBV	542232	944766	87.38%	10.406%
61	9.645	2581	2583	2587	rVB	256	174	0.02%	0.002%
62	9.687	2591	2596	2597	rBV	843	652	0.06%	0.007%
63	9.761	2615	2619	2621	rBV2	384	281	0.03%	0.003%
64	9.832	2638	2641	2645	rBV2	185	177	0.02%	0.002%
65	9.890	2657	2659	2663	rBV	242	228	0.02%	0.003%
66	9.931	2670	2672	2676	rBV2	197	172	0.02%	0.002%
67	10.166	2743	2745	2750	rVB2	246	208	0.02%	0.002%
68	10.481	2840	2843	2845	rBV	344	285	0.03%	0.003%
69	10.546	2859	2863	2868	rBV2	212	225	0.02%	0.002%
70	10.677	2892	2904	2909	rBV3	921	1452	0.13%	0.016%
71	10.758	2916	2929	2950	rBV	418738	678472	62.75%	7.473%
72	10.899	2967	2973	2978	rBV3	656	785	0.07%	0.009%
73	11.147	3045	3050	3051	rBV3	354	238	0.02%	0.003%
74	11.475	3144	3152	3161	rVB5	1446	2651	0.25%	0.029%
75	11.513	3161	3164	3167	rBV2	294	251	0.02%	0.003%
76	11.584	3183	3186	3192	rVB	349	348	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048095.D
 Acq On : 15 Apr 2022 11:27
 Operator : SY/MD
 Sample : VU0415MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.697	3219	3221	3225	rVB2	688	478	0.04%	0.005%
78	11.719	3225	3228	3230	rBV	321	216	0.02%	0.002%
79	11.751	3230	3238	3245	rBV5	1980	3064	0.28%	0.034%
80	11.816	3245	3258	3281	rVV	581301	965548	89.30%	10.635%
81	11.973	3304	3307	3310	rBV3	755	606	0.06%	0.007%
82	12.102	3345	3347	3350	rBV2	292	198	0.02%	0.002%
83	12.195	3363	3376	3397	rBV	522798	863247	79.84%	9.508%
84	12.507	3466	3473	3476	rBV3	557	704	0.07%	0.008%
85	12.645	3512	3516	3520	rBV2	242	226	0.02%	0.002%
86	12.668	3520	3523	3527	rBV4	297	273	0.03%	0.003%
87	12.771	3551	3555	3556	rBV2	839	574	0.05%	0.006%
88	12.944	3600	3609	3611	rBV3	356	547	0.05%	0.006%
89	13.002	3624	3627	3629	rBV	408	247	0.02%	0.003%
90	13.092	3652	3655	3658	rVB2	338	187	0.02%	0.002%
91	13.192	3684	3686	3689	rBV3	340	252	0.02%	0.003%
92	13.224	3692	3696	3702	rVV5	1156	1462	0.14%	0.016%
93	13.336	3727	3731	3735	rBV3	281	320	0.03%	0.004%
94	13.452	3763	3767	3770	rBV2	303	252	0.02%	0.003%
95	13.844	3880	3889	3903	rBV4	10436	16760	1.55%	0.185%
96	14.060	3951	3956	3957	rBV	470	351	0.03%	0.004%
97	14.092	3959	3966	3978	rVB	8748	14652	1.36%	0.161%
98	14.333	4033	4041	4054	rBV2	4984	7670	0.71%	0.084%
99	14.806	4186	4188	4195	rBV2	345	397	0.04%	0.004%
100	14.941	4227	4230	4232	rBV2	524	292	0.03%	0.003%




Sum of corrected areas: 9078914

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048095.D
Acq On : 15 Apr 2022 11:27
Operator : SY/MD
Sample : VU0415MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

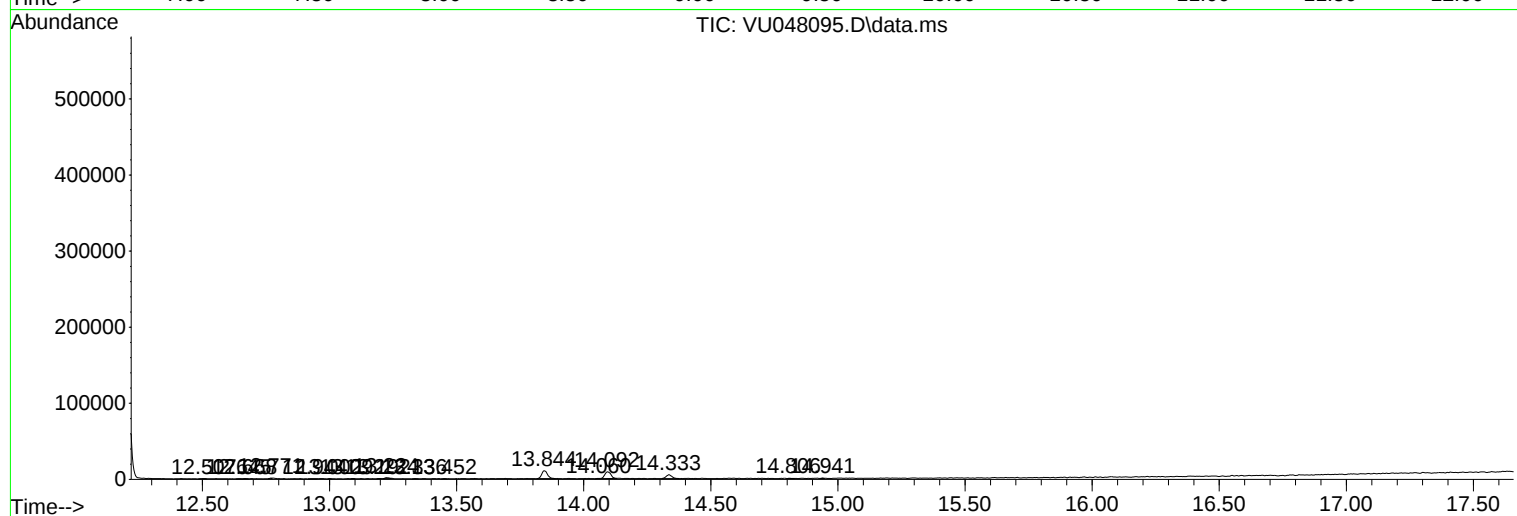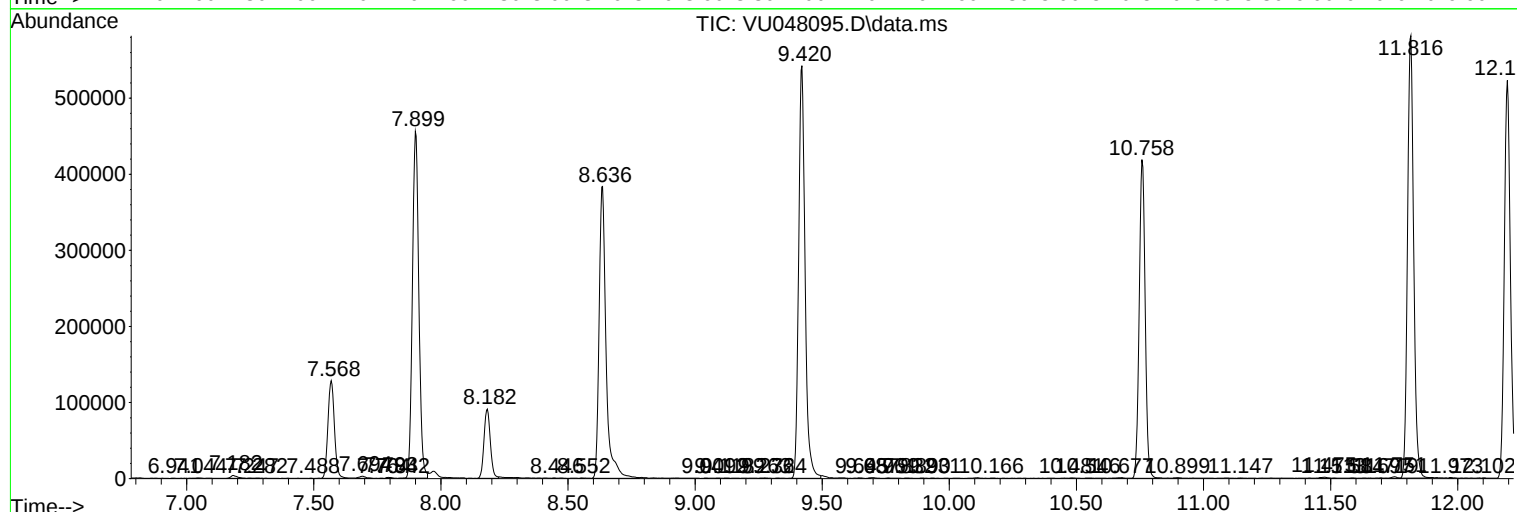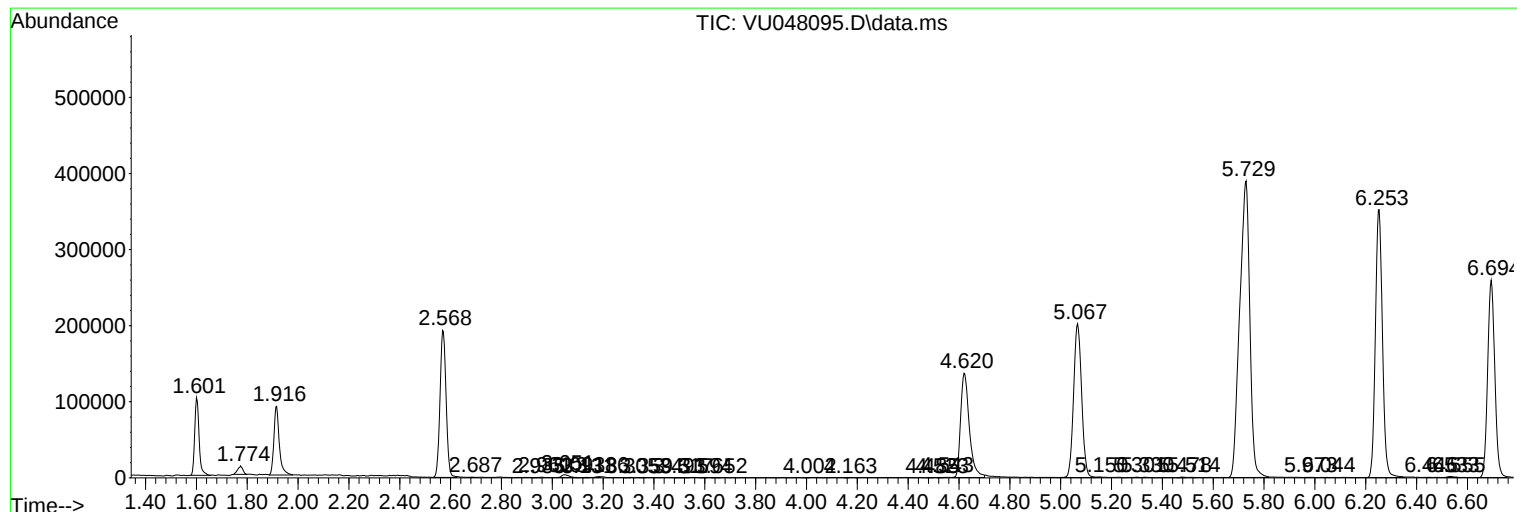

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048095.D
Acq On : 15 Apr 2022 11:27
Operator : SY/MD
Sample : VU0415MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048095.D
Acq On : 15 Apr 2022 11:27
Operator : SY/MD
Sample : VU0415MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc