

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048100.D
 Acq On : 15 Apr 2022 14:12
 Operator : SY/MD
 Sample : N2345-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	100	rBV	179583	213276	16.71%	2.015%
2	1.916	170	179	204	rVB	131691	187069	14.65%	1.768%
3	2.568	369	382	403	rBV	288316	480190	37.62%	4.537%
4	2.726	429	431	434	rBV3	547	277	0.02%	0.003%
5	2.838	463	466	469	rBV3	260	206	0.02%	0.002%
6	2.861	469	473	474	rBV	336	212	0.02%	0.002%
7	3.051	523	532	543	rBV4	2843	5309	0.42%	0.050%
8	3.144	557	561	565	rBV2	390	454	0.04%	0.004%
9	3.244	589	592	596	rBV2	271	227	0.02%	0.002%
10	3.289	602	606	610	rBV3	283	219	0.02%	0.002%
11	3.356	619	627	633	rBV4	409	710	0.06%	0.007%
12	3.385	633	636	639	rVB2	316	188	0.01%	0.002%
13	3.526	675	680	682	rBV	273	261	0.02%	0.002%
14	3.687	726	730	733	rVB2	253	231	0.02%	0.002%
15	3.771	751	756	761	rBV3	318	342	0.03%	0.003%
16	3.825	769	773	775	rBV2	361	298	0.02%	0.003%
17	3.912	798	800	804	rBV	274	195	0.02%	0.002%
18	4.022	831	834	837	rVV	287	224	0.02%	0.002%
19	4.131	866	868	873	rBV2	280	287	0.02%	0.003%
20	4.218	890	895	900	rVV2	317	421	0.03%	0.004%
21	4.362	936	940	943	rBV2	209	176	0.01%	0.002%
22	4.472	970	974	976	rVB2	305	234	0.02%	0.002%
23	4.629	1008	1023	1055	rVV	116955	300248	23.52%	2.837%
24	5.067	1143	1159	1185	rBV	220898	492015	38.54%	4.649%
25	5.295	1223	1230	1232	rBV3	550	696	0.05%	0.007%
26	5.308	1232	1234	1236	rVV	429	189	0.01%	0.002%
27	5.324	1236	1239	1243	rVV	231	223	0.02%	0.002%
28	5.507	1293	1296	1301	rBV2	296	222	0.02%	0.002%
29	5.597	1319	1324	1329	rBV2	190	175	0.01%	0.002%
30	5.729	1343	1365	1399	rBV2	474200	1276582	100.00%	12.062%
31	5.877	1409	1411	1414	rVB3	500	279	0.02%	0.003%
32	5.948	1429	1433	1437	rBV3	241	204	0.02%	0.002%
33	6.022	1451	1456	1457	rBV2	339	300	0.02%	0.003%
34	6.102	1476	1481	1483	rBV3	383	359	0.03%	0.003%
35	6.118	1483	1486	1489	rVB2	482	328	0.03%	0.003%
36	6.250	1512	1527	1549	rBV	489358	930451	72.89%	8.792%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048100.D
 Acq On : 15 Apr 2022 14:12
 Operator : SY/MD
 Sample : N2345-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.478	1595	1598	1602	rBV3	382	317	0.02%	0.003%
38	6.536	1608	1616	1622	rBV6	1836	2964	0.23%	0.028%
39	6.562	1622	1624	1629	rVB3	586	520	0.04%	0.005%
40	6.591	1629	1633	1636	rVB2	466	345	0.03%	0.003%
41	6.623	1639	1643	1646	rBV4	394	277	0.02%	0.003%
42	6.694	1650	1665	1683	rBV	284163	562656	44.08%	5.316%
43	6.784	1691	1693	1698	rBV2	314	230	0.02%	0.002%
44	6.960	1745	1748	1751	rBV3	270	213	0.02%	0.002%
45	6.993	1754	1758	1761	rBV2	204	187	0.01%	0.002%
46	7.018	1761	1766	1768	rBV	358	266	0.02%	0.003%
47	7.189	1811	1819	1826	rBV3	2484	3791	0.30%	0.036%
48	7.263	1840	1842	1847	rVV2	202	203	0.02%	0.002%
49	7.285	1847	1849	1852	rVV2	484	228	0.02%	0.002%
50	7.362	1870	1873	1877	rVB2	318	189	0.01%	0.002%
51	7.391	1877	1882	1884	rBV3	244	190	0.01%	0.002%
52	7.407	1884	1887	1895	rVB2	249	358	0.03%	0.003%
53	7.462	1895	1904	1908	rBV	383	509	0.04%	0.005%
54	7.568	1924	1937	1964	rVV	144396	261341	20.47%	2.469%
55	7.697	1968	1977	1986	rVB5	1613	3428	0.27%	0.032%
56	7.767	1995	1999	2000	rBV	489	336	0.03%	0.003%
57	7.800	2007	2009	2015	rVB3	261	207	0.02%	0.002%
58	7.829	2015	2018	2022	rVB2	294	202	0.02%	0.002%
59	7.899	2022	2040	2056	rBV	575222	999223	78.27%	9.441%
60	8.179	2113	2127	2143	rBV	99829	172152	13.49%	1.627%
61	8.529	2233	2236	2239	rVB2	255	177	0.01%	0.002%
62	8.636	2257	2269	2296	rBV	366726	667897	52.32%	6.311%
63	8.825	2326	2328	2332	rVB	587	351	0.03%	0.003%
64	8.928	2356	2360	2363	rBV3	408	349	0.03%	0.003%
65	9.047	2393	2397	2404	rVB3	489	682	0.05%	0.006%
66	9.082	2404	2408	2410	rBV2	325	269	0.02%	0.003%
67	9.115	2415	2418	2422	rVB	437	283	0.02%	0.003%
68	9.169	2430	2435	2437	rBV	354	286	0.02%	0.003%
69	9.417	2499	2512	2535	rBV	709776	1217720	95.39%	11.506%
70	9.574	2559	2561	2567	rVB3	596	433	0.03%	0.004%
71	9.700	2591	2600	2605	rVB3	811	1077	0.08%	0.010%
72	9.758	2615	2618	2620	rBV2	370	269	0.02%	0.003%
73	9.793	2626	2629	2631	rVV	240	203	0.02%	0.002%
74	9.806	2631	2633	2640	rVV2	304	361	0.03%	0.003%
75	9.980	2684	2687	2691	rVB2	244	196	0.02%	0.002%
76	10.108	2724	2727	2729	rBV	470	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048100.D
 Acq On : 15 Apr 2022 14:12
 Operator : SY/MD
 Sample : N2345-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.234	2763	2766	2768	rBV2	240	190	0.01%	0.002%
78	10.468	2836	2839	2844	rBV2	386	286	0.02%	0.003%
79	10.671	2894	2902	2910	rVB5	2862	4170	0.33%	0.039%
80	10.758	2915	2929	2948	rBV	401812	648287	50.78%	6.125%
81	10.870	2960	2964	2967	rBV3	615	455	0.04%	0.004%
82	11.050	3018	3020	3028	rVB2	346	296	0.02%	0.003%
83	11.121	3038	3042	3045	rVB5	427	342	0.03%	0.003%
84	11.147	3047	3050	3053	rVB3	326	207	0.02%	0.002%
85	11.256	3078	3084	3087	rBV3	381	448	0.04%	0.004%
86	11.346	3108	3112	3116	rBV	218	193	0.02%	0.002%
87	11.385	3121	3124	3126	rBV2	364	179	0.01%	0.002%
88	11.455	3140	3146	3147	rBV3	1511	1120	0.09%	0.011%
89	11.677	3211	3215	3216	rBV	455	318	0.02%	0.003%
90	11.745	3226	3236	3243	rBV4	855	1165	0.09%	0.011%
91	11.812	3244	3257	3279	rBV	755623	1212803	95.00%	11.459%
92	12.195	3363	3376	3399	rBV	551511	907692	71.10%	8.577%
93	12.330	3415	3418	3420	rBV3	431	288	0.02%	0.003%
94	12.362	3425	3428	3430	rBV3	318	189	0.01%	0.002%
95	12.986	3619	3622	3624	rBV	283	203	0.02%	0.002%
96	13.391	3745	3748	3751	rBV2	320	272	0.02%	0.003%
97	13.642	3824	3826	3831	rVB2	355	228	0.02%	0.002%
98	13.848	3881	3890	3900	rBV3	5681	8667	0.68%	0.082%
99	14.667	4142	4145	4147	rBV3	510	379	0.03%	0.004%
100	15.873	4518	4520	4524	rBV3	891	684	0.05%	0.006%




Sum of corrected areas: 10583414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048100.D
Acq On : 15 Apr 2022 14:12
Operator : SY/MD
Sample : N2345-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

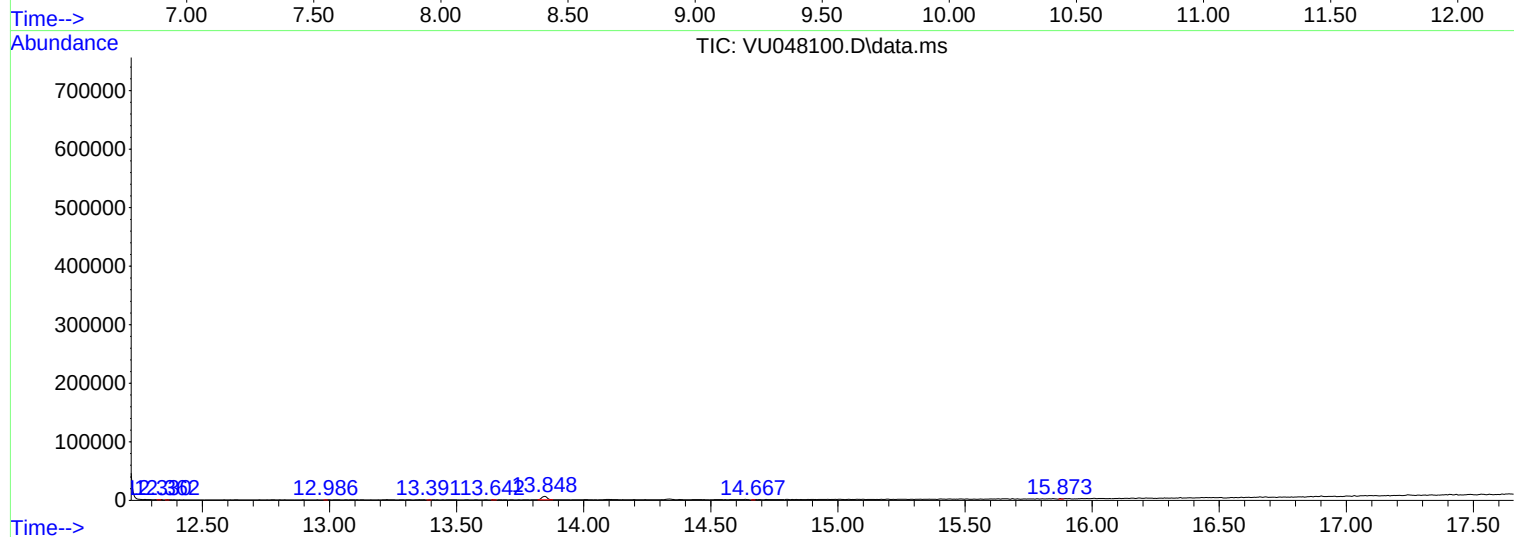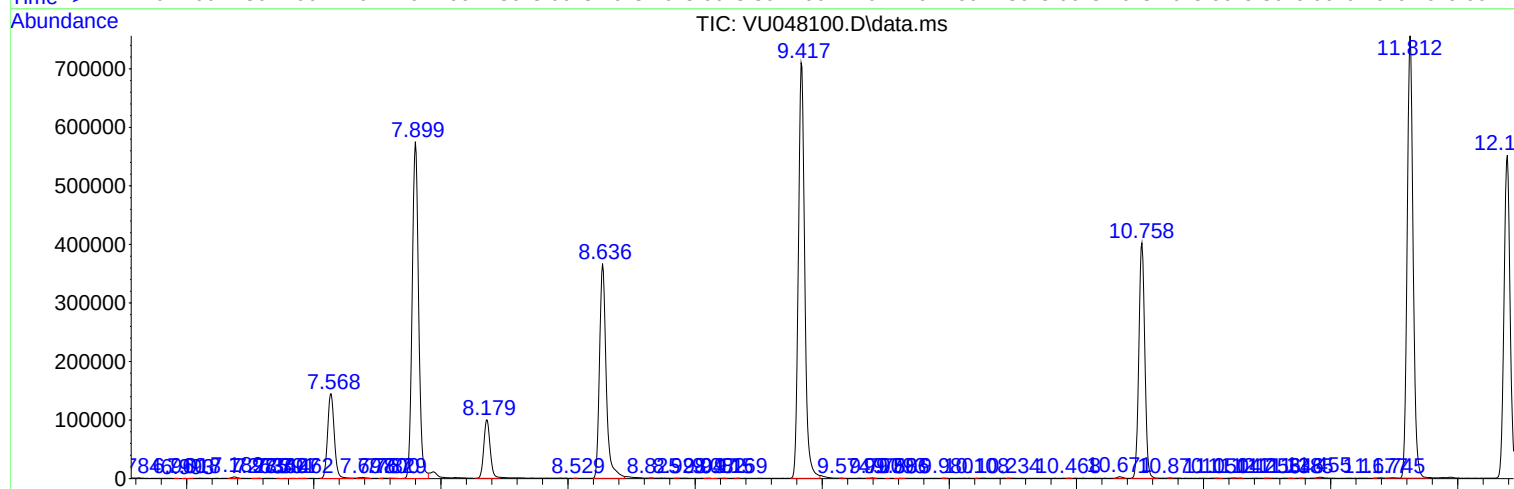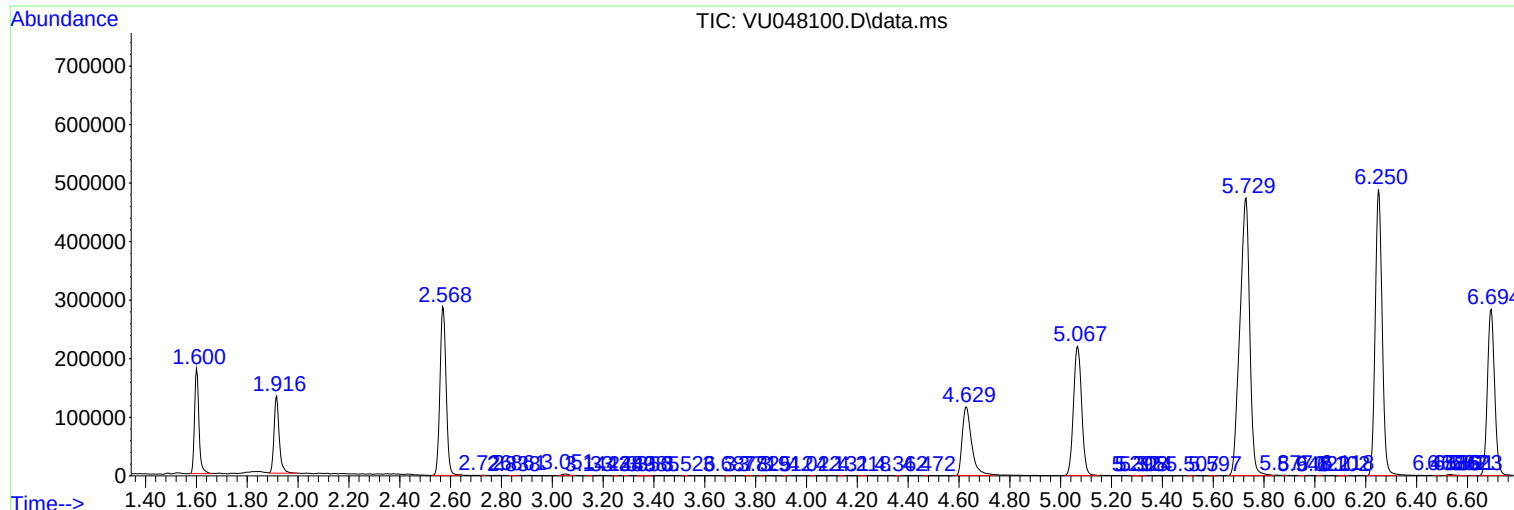

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048100.D
Acq On : 15 Apr 2022 14:12
Operator : SY/MD
Sample : N2345-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048100.D
Acq On : 15 Apr 2022 14:12
Operator : SY/MD
Sample : N2345-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------